

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
Data File : PD071990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 16:26
Operator : AR\AJ
Sample : N4706-07
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
CB8L2

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/23/2022
Supervised By :Ankita Jodhani 09/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 23:58:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

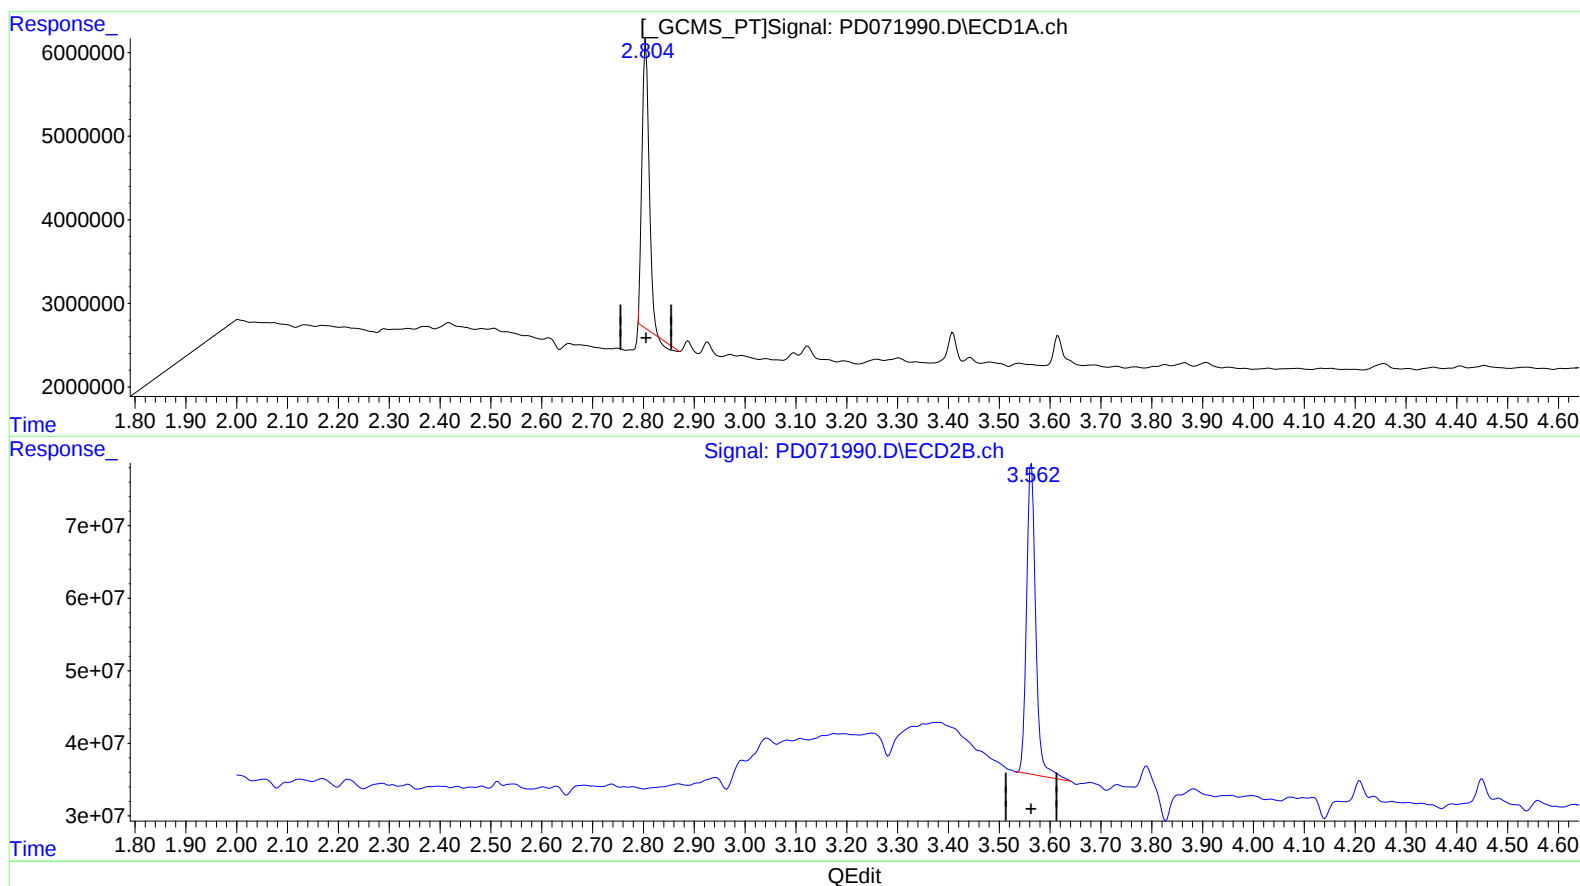

(1) Tetrachloro-m-xylene (SA)

2.805min 12.639 ng/ml

response 32961823

(1) Tetrachloro-m-xylene #2 (SA)

3.563min 16.423 ng/ml

response 538150680


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
Data File : PD071990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 16:26
Operator : AR\AJ
Sample : N4706-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
CB8L2

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 23:58:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

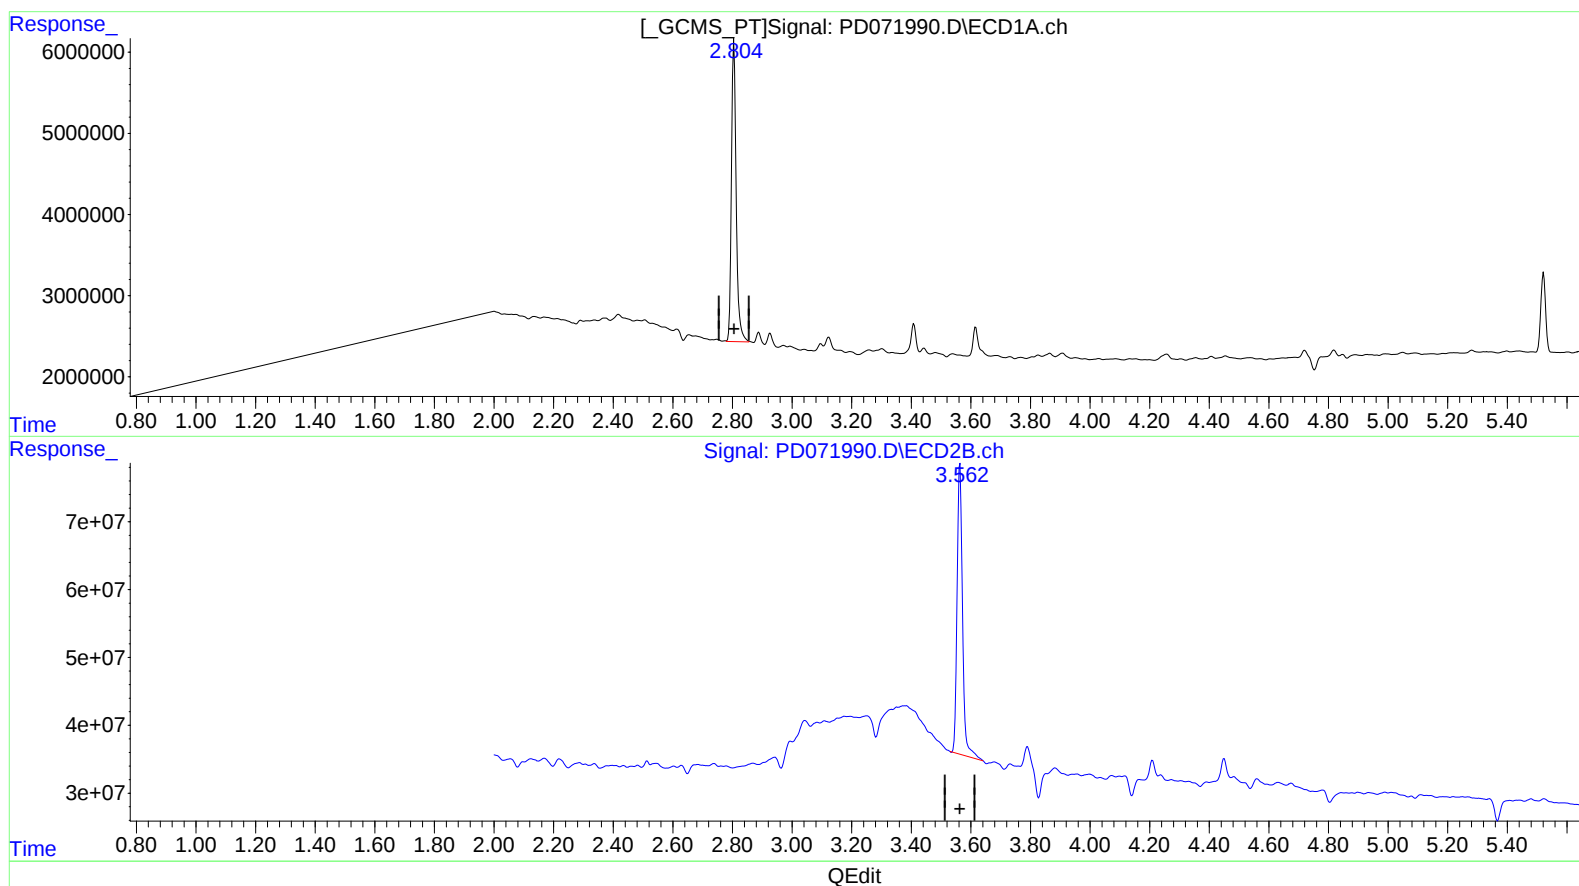

(1) Tetrachloro-m-xylene (SA)

2.804min 15.795 ng/ml m

response 41191954

(1) Tetrachloro-m-xylene #2 (SA)

3.563min 16.423 ng/ml

response 538150680