

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092322\  
Data File : PD071998.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Sep 2022 18:12  
Operator : AR\AJ  
Sample : INDA323  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

## Instrument :

ECD\_D

## LabSampleId :

INDA323


## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/23/2022  
Supervised By :Ankita Jodhani 09/23/2022

Supervised By :Ankita  
Jodhani  
09/23/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 23 00:04:40 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082622CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Aug 27 07:11:22 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

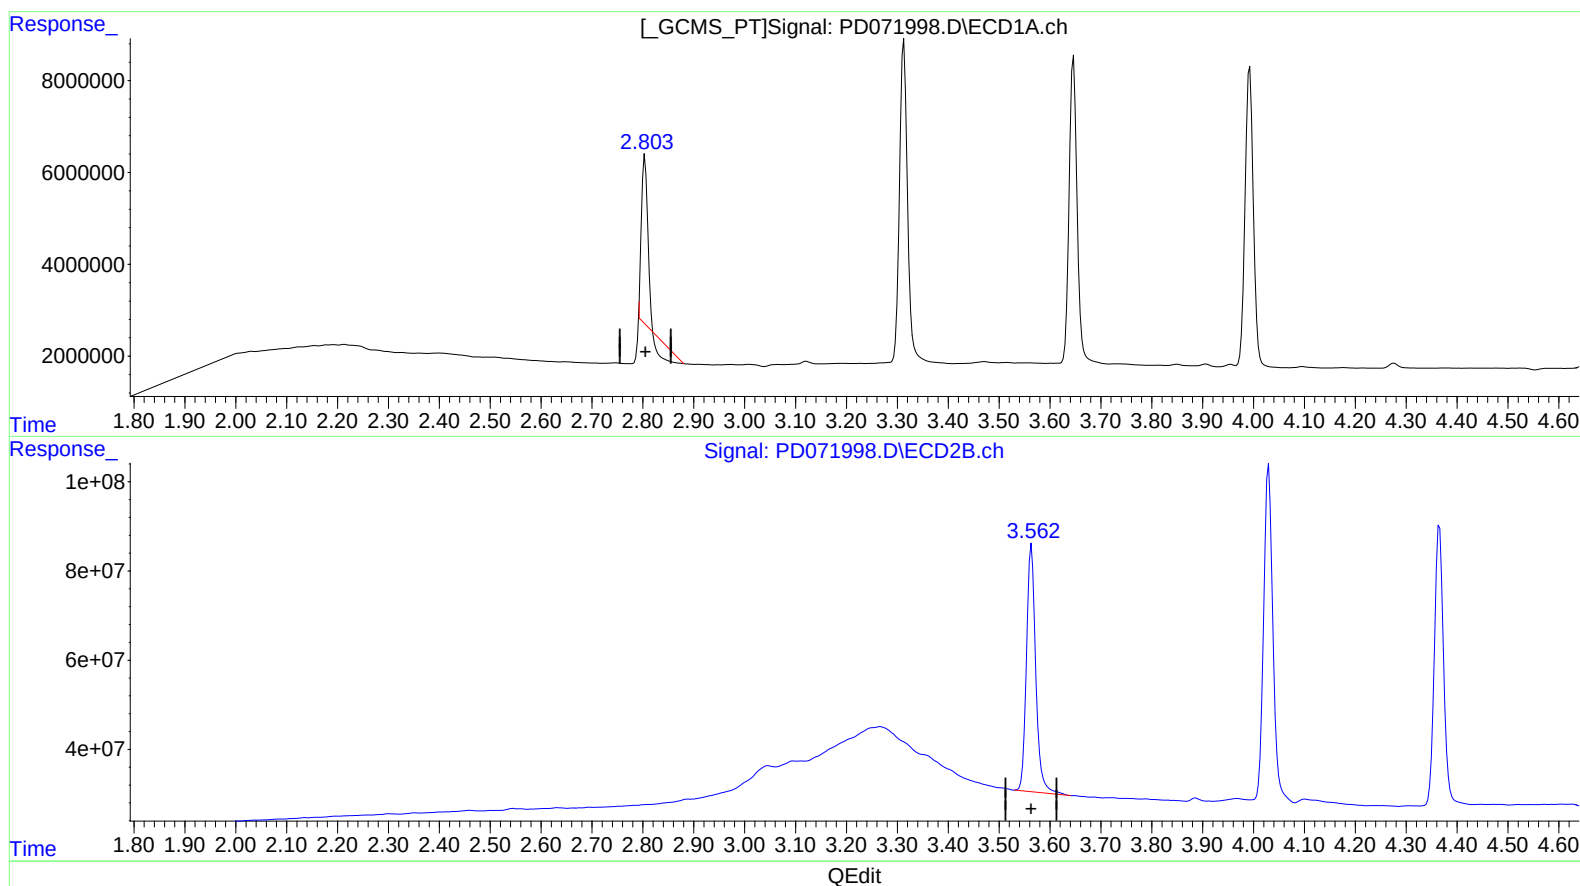

(1) Tetrachloro-m-xylene (SA)

2.804min 8.662 ng/ml

response 22589844

(1) Tetrachloro-m-xylene #2 (SA)

3.564min 21.376 ng/ml

response 700428724

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092322\  
Data File : PD071998.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Sep 2022 18:12  
Operator : AR\AJ  
Sample : INDA323  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

## Instrument :

ECD\_D

## LabSampleId :

INDA323


## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/23/2022  
Supervised By :Ankita Jodhani 09/23/2022

Supervised By :Ankita  
Jodhani  
09/23/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 23 00:04:40 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082622CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Aug 27 07:11:22 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

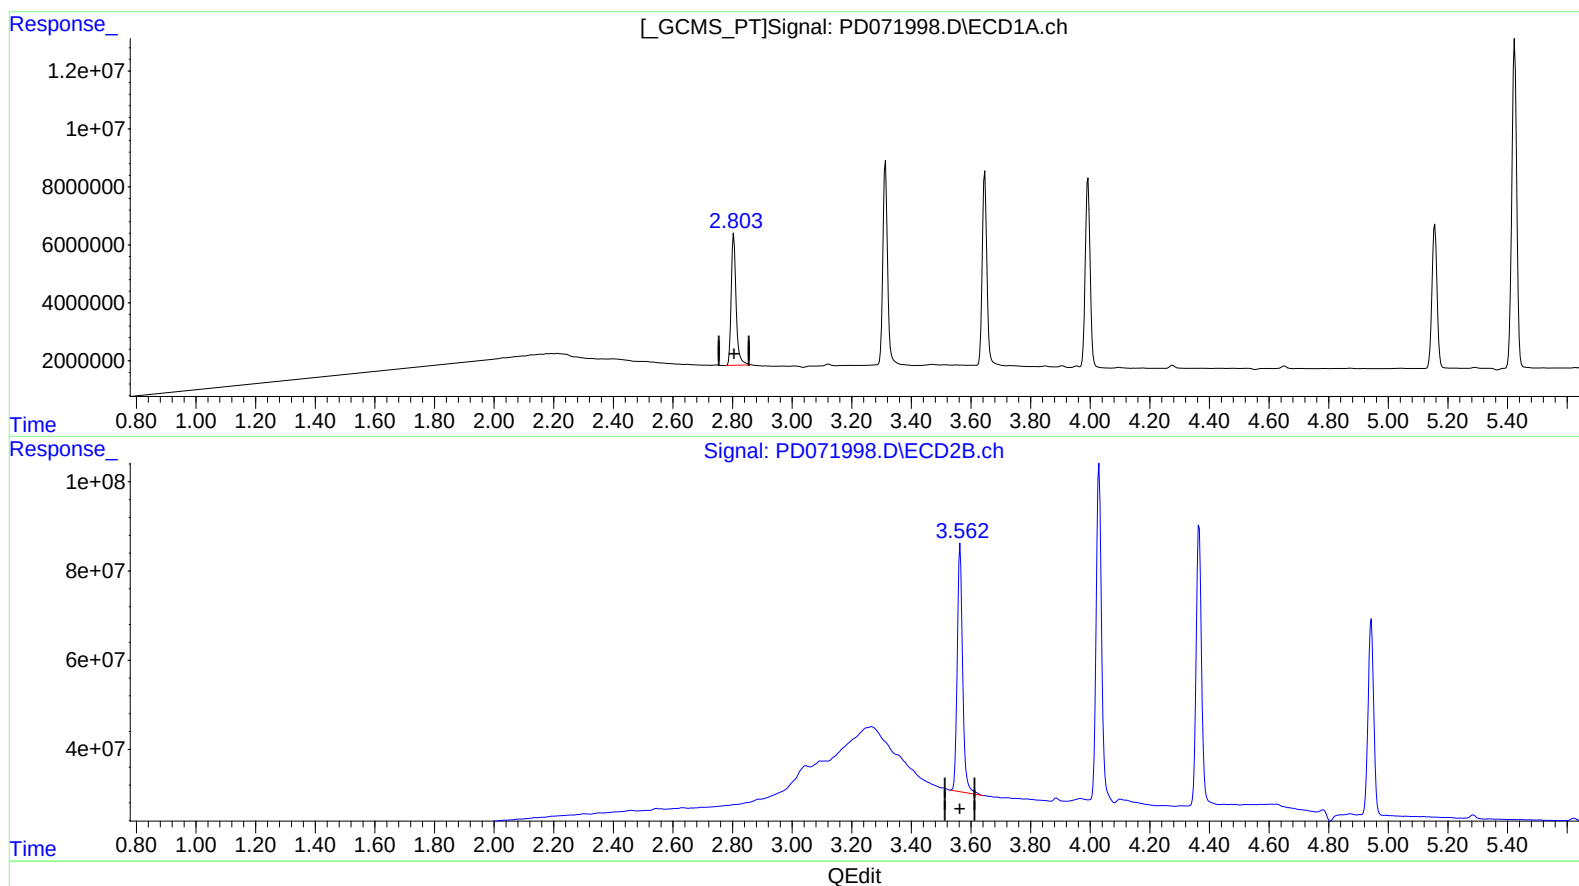

(1) Tetrachloro-m-xylene (SA)

2.803min 19.708 ng/ml m

response 51397862

(1) Tetrachloro-m-xylene #2 (SA)

3.564min 21.376 ng/ml

response 700428724

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092322\  
Data File : PD071998.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Sep 2022 18:12  
Operator : AR\AJ  
Sample : INDA323  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

## Instrument :

ECD\_D

## LabSampleId :

INDA323


## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/23/2022  
Supervised By :Ankita Jodhani 09/23/2022

Supervised By :Ankita  
Jodhani  
09/23/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 23 00:04:40 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082622CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Aug 27 07:11:22 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

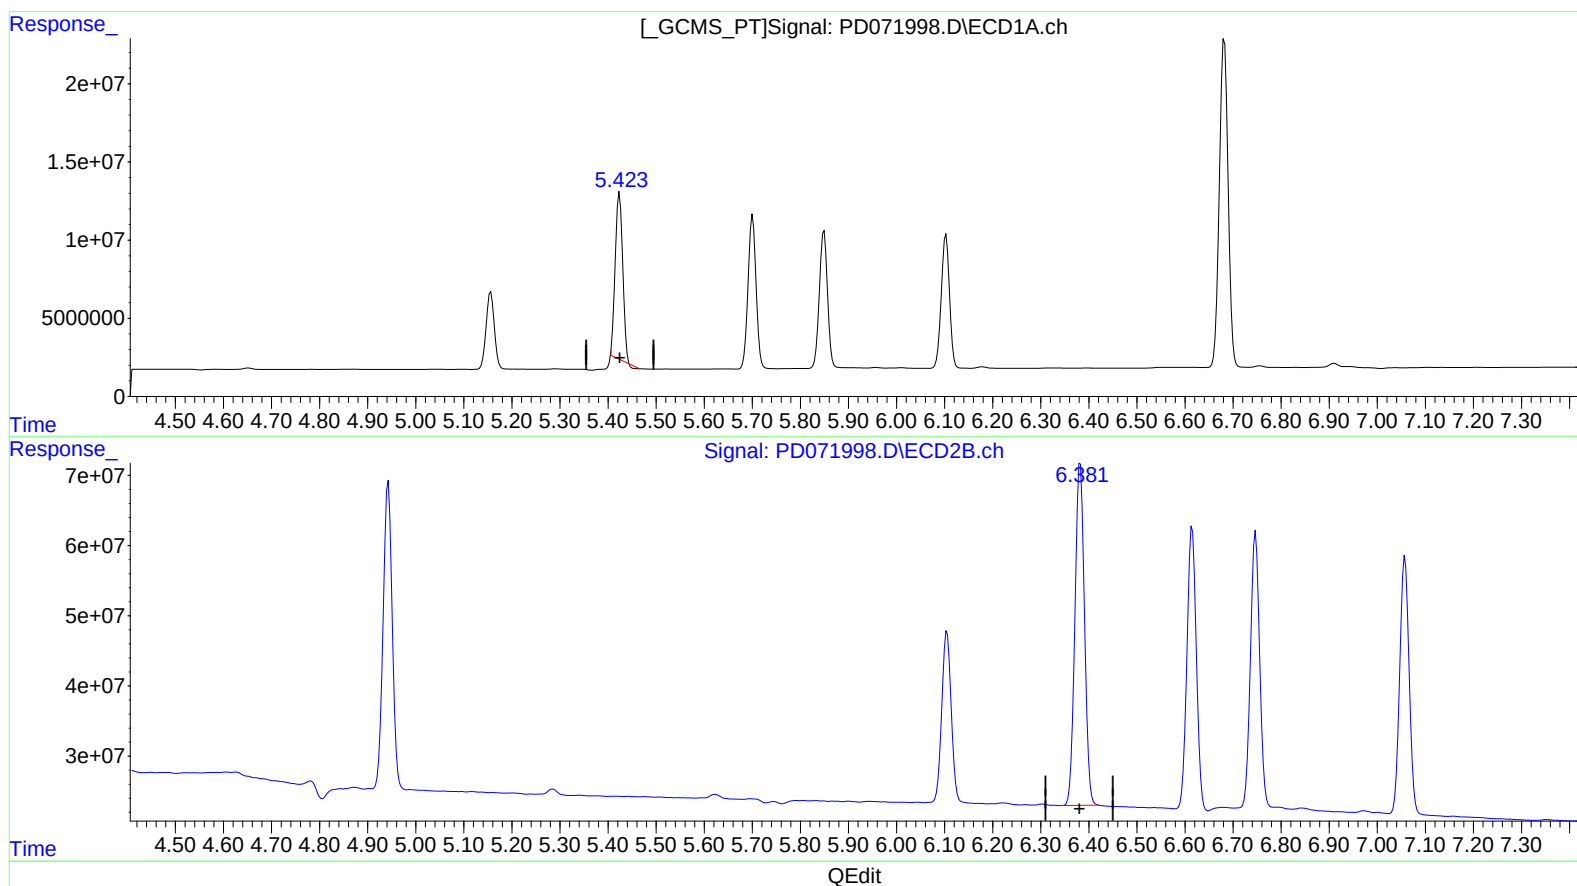

(13) Dieldrin (MA)

5.424min 32.106 ng/ml

response 111183783

(13) Dieldrin #2 (MA)

6.382min 42.104 ng/ml

response 673841004

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092322\  
Data File : PD071998.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Sep 2022 18:12  
Operator : AR\AJ  
Sample : INDA323  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

## Instrument :

ECD\_D

## LabSampleId :

INDA323


## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/23/2022  
Supervised By :Ankita Jodhani 09/23/2022

Supervised By :Ankita  
Jodhani  
09/23/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 23 00:04:40 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082622CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Aug 27 07:11:22 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

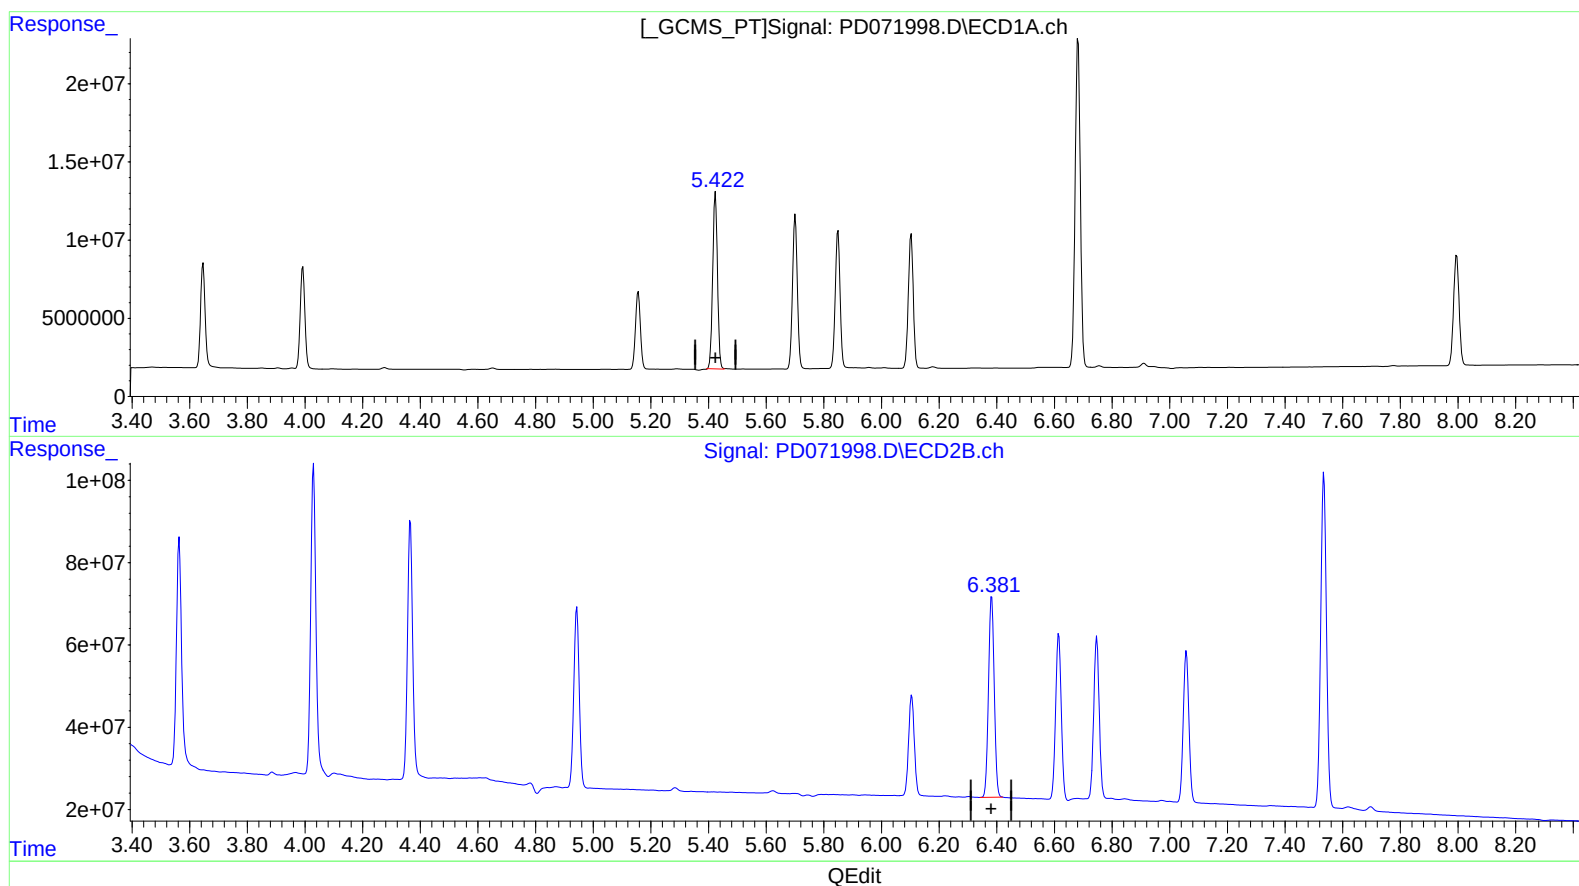

(13) Dieldrin (MA)

5.422min 37.459 ng/ml m

response 129719843

(13) Dieldrin #2 (MA)

6.382min 42.104 ng/ml

response 673841004