

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
 Data File : PD071995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2022 17:32
 Operator : AR\AJ
 Sample : N4706-12MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8M1MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/23/2022
 Supervised By :Ankita Jodhani 09/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 00:02:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.563	34980815	510.0E6	13.413m	15.564
27)	SA Decachlor...	7.995	9.092	44765849	176.2E6	17.059	18.433
Target Compounds							
2)	A alpha-BHC	3.313	4.030	178.7E6	1976.5E6	46.325	44.798
3)	MA gamma-BHC...	3.647	4.365	168.7E6	1648.4E6	45.688	44.322
4)	MA Heptachlor	3.993	4.942	153.9E6	1103.4E6	40.433	40.863
5)	MB Aldrin	4.276	5.285	151.1E6	896.8E6	42.451	41.512
6)	B beta-BHC	3.945	4.572	67354448	640.4E6	42.401	44.746
7)	B delta-BHC	4.179	4.820	164.2E6	1268.3E6	46.985	48.255
8)	B Heptachlo...	4.782	5.717	146.9E6	777.2E6	45.079	45.958
9)	A Endosulfan I	5.157	6.105	133.9E6	692.4E6	42.489	44.085
10)	B trans-Chl...	5.035	5.972	143.8E6	733.6E6	42.477	43.336
11)	B cis-Chlor...	5.100	6.050	142.4E6	715.8E6	42.682	43.919
12)	B 4,4'-DDE	5.291	6.222	267.0E6	1298.0E6	87.046	88.956
13)	MA Dieldrin	5.422	6.383	299.2E6	1434.6E6	86.408m	89.639
14)	MA Endrin	5.701	6.615	266.2E6	1214.3E6	88.892	92.290
15)	B Endosulfa...	5.996	6.841	246.6E6	1145.0E6	92.789	94.990
16)	A 4,4'-DDD	5.849	6.747	232.0E6	1097.8E6	88.131	89.713
17)	MA 4,4'-DDT	6.103	7.058	240.5E6	1095.7E6	88.336	90.805
18)	B Endrin al...	6.176	6.972	191.9E6	892.9E6	82.956	87.520
19)	B Endosulfa...	6.401	7.205	225.0E6	1019.0E6	84.446	89.730
20)	A Methoxychlor	6.682	7.535	588.1E6	2412.2E6	409.470	439.634
21)	B Endrin ke...	6.909	7.697	270.2E6	1150.9E6	90.298m	92.974

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
Data File : PD071995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 17:32
Operator : AR\AJ
Sample : N4706-12MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 00:02:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

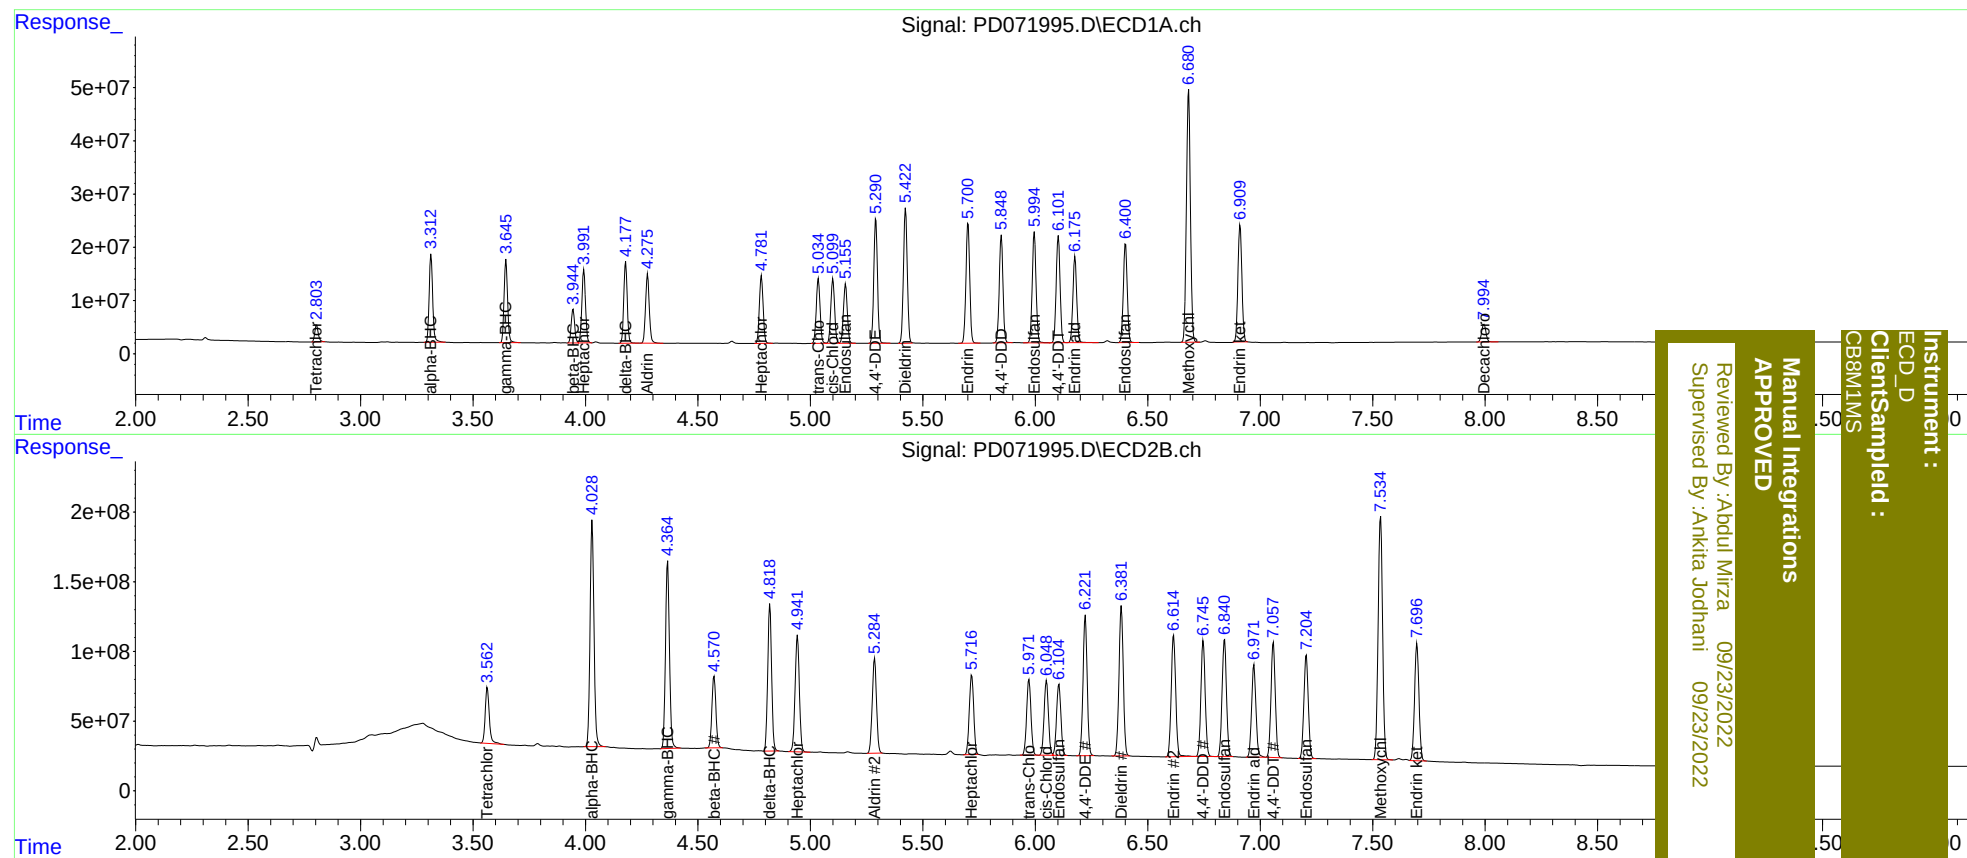

Reviewed By: Abdul Mirza 09/23/2022
Supervised By: Ankita Jodhani 09/23/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CB8M1MS