

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
 Data File : PD071996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2022 17:46
 Operator : AR\AJ
 Sample : N4706-13MSD
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8M1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2022
 Supervised By : Ankita Jodhani 09/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 00:03:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.584	41669156	570.3E6	15.978m	17.403
27)	SA Decachlor...	7.994	9.111	54603798	211.7E6	20.808	22.151
Target Compounds							
2)	A alpha-BHC	3.313	4.048	190.9E6	2076.0E6	49.498	47.052m
3)	MA gamma-BHC...	3.647	4.385	179.8E6	1710.9E6	48.694	46.002
4)	MA Heptachlor	3.992	4.963	161.9E6	1146.2E6	42.534	42.450
5)	MB Aldrin	4.276	5.304	160.6E6	951.1E6	45.122	44.025m
6)	B beta-BHC	3.945	4.591	71151130	661.8E6	44.791	46.237m
7)	B delta-BHC	4.179	4.839	175.2E6	1328.6E6	50.130	50.549m
8)	B Heptachlo...	4.782	5.736	155.2E6	811.8E6	47.614	48.006m
9)	A Endosulfan I	5.155	6.123	141.6E6	734.0E6	44.924	46.735m
10)	B trans-Chl...	5.035	5.990	149.8E6	755.4E6	44.242	44.627m
11)	B cis-Chlor...	5.099	6.068	147.9E6	741.7E6	44.356	45.507m
12)	B 4,4'-DDE	5.291	6.241	275.5E6	1329.0E6	89.809	91.080m
13)	MA Dieldrin	5.422	6.401	315.2E6	1505.2E6	91.021m	94.047m
14)	MA Endrin	5.701	6.635	283.4E6	1263.8E6	94.628	96.054
15)	B Endosulfa...	5.996	6.859	260.1E6	1209.6E6	97.849	100.345m
16)	A 4,4'-DDD	5.849	6.766	241.1E6	1126.3E6	91.617	92.046
17)	MA 4,4'-DDT	6.103	7.076	245.4E6	1119.0E6	90.133	92.737m
18)	B Endrin al...	6.177	6.992	205.9E6	913.2E6	88.990	89.512
19)	B Endosulfa...	6.401	7.224	239.8E6	1037.4E6	90.021	91.345
20)	A Methoxychlor	6.682	7.555	614.5E6	2511.9E6	427.844	457.791
21)	B Endrin ke...	6.910	7.715	291.3E6	1225.2E6	97.349m	98.980m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
Data File : PD071996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 17:46
Operator : AR\AJ
Sample : N4706-13MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 00:03:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

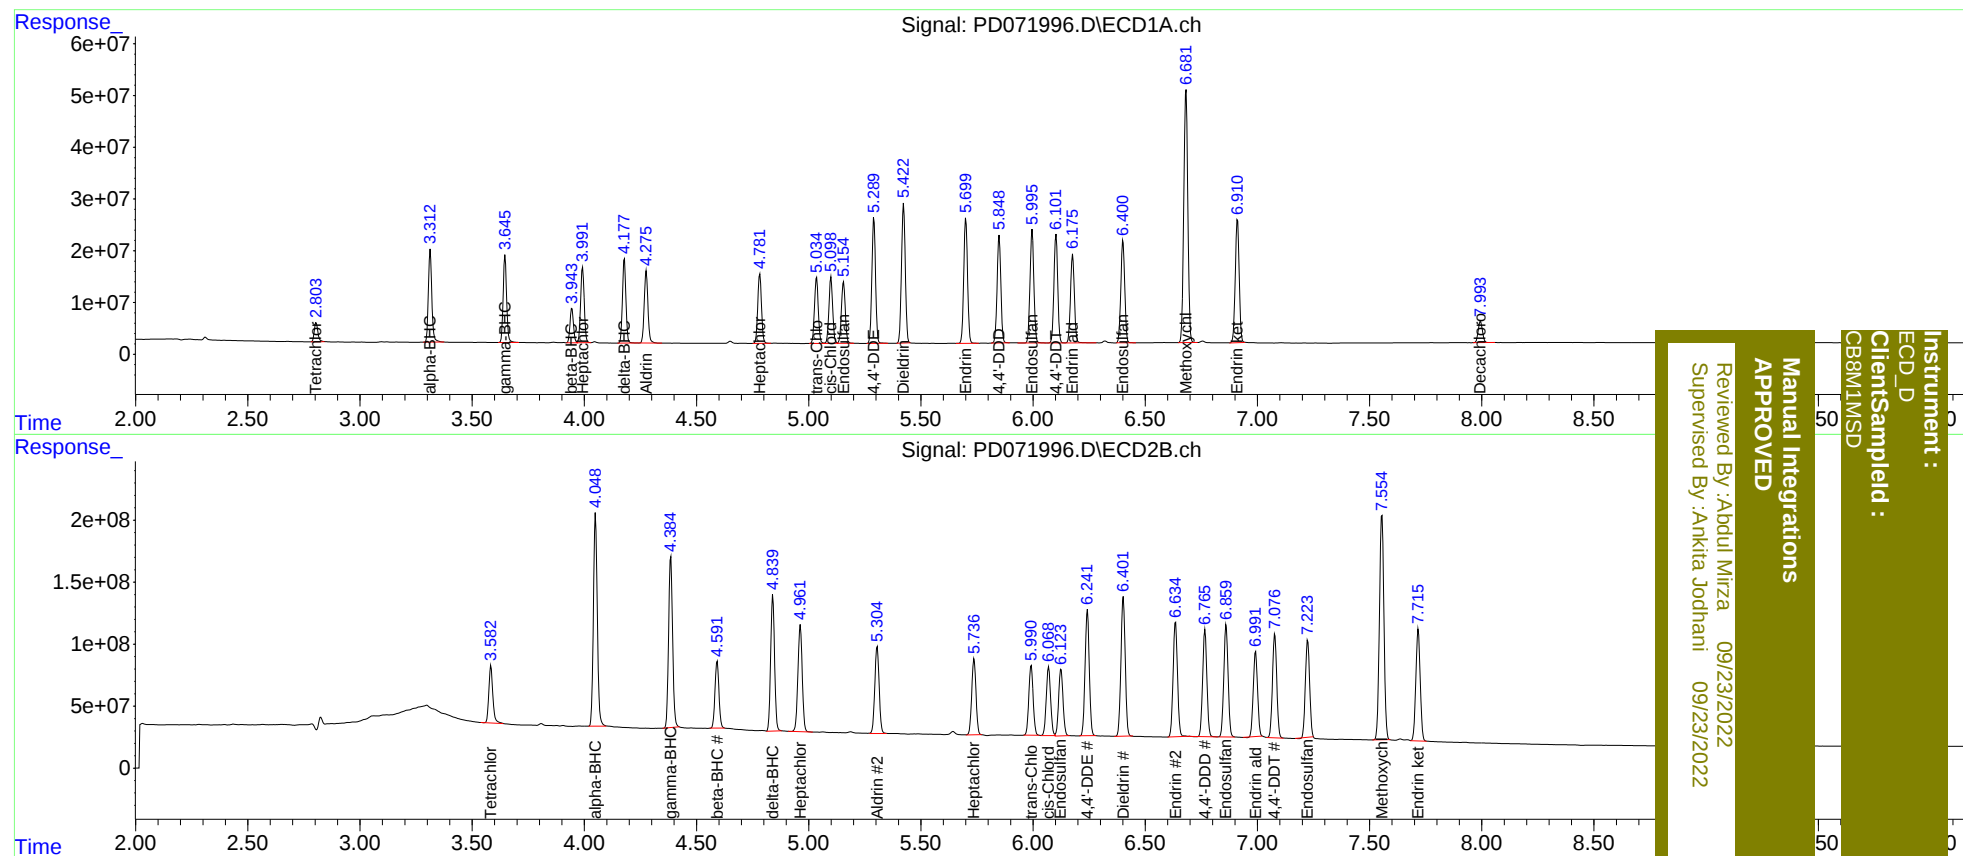

Instrument :
ECD_D
ClientSampled :
CB8M1MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/23/2022
Supervised By: Ankita Jodhani 09/23/2022