

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
 Data File : PD078207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2023 18:24
 Operator : AR\AJ
 Sample : 04417-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYF2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/22/2023
 Supervised By : Ankita Jodhani 09/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 00:59:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.760	34995962	24170361	13.790	16.355
2) SA Decachlor...	9.079	7.896	46892957	25698742	15.011	15.868
Target Compounds						
8) B Heptachlo...	5.687	4.708	3016239	1248533	0.780	0.594m
9) A Endosulfan I	6.067	5.108	1419700	1311314	0.423	0.731 #
17) MA 4,4'-DDT	7.003	6.012	4408490	1584442	1.609	1.121 #
19) B Endosulfa...	7.164	6.314	5118509	1112972	1.689	0.674 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
Data File : PD078207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2023 18:24
Operator : AR\AJ
Sample : 04417-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 00:59:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

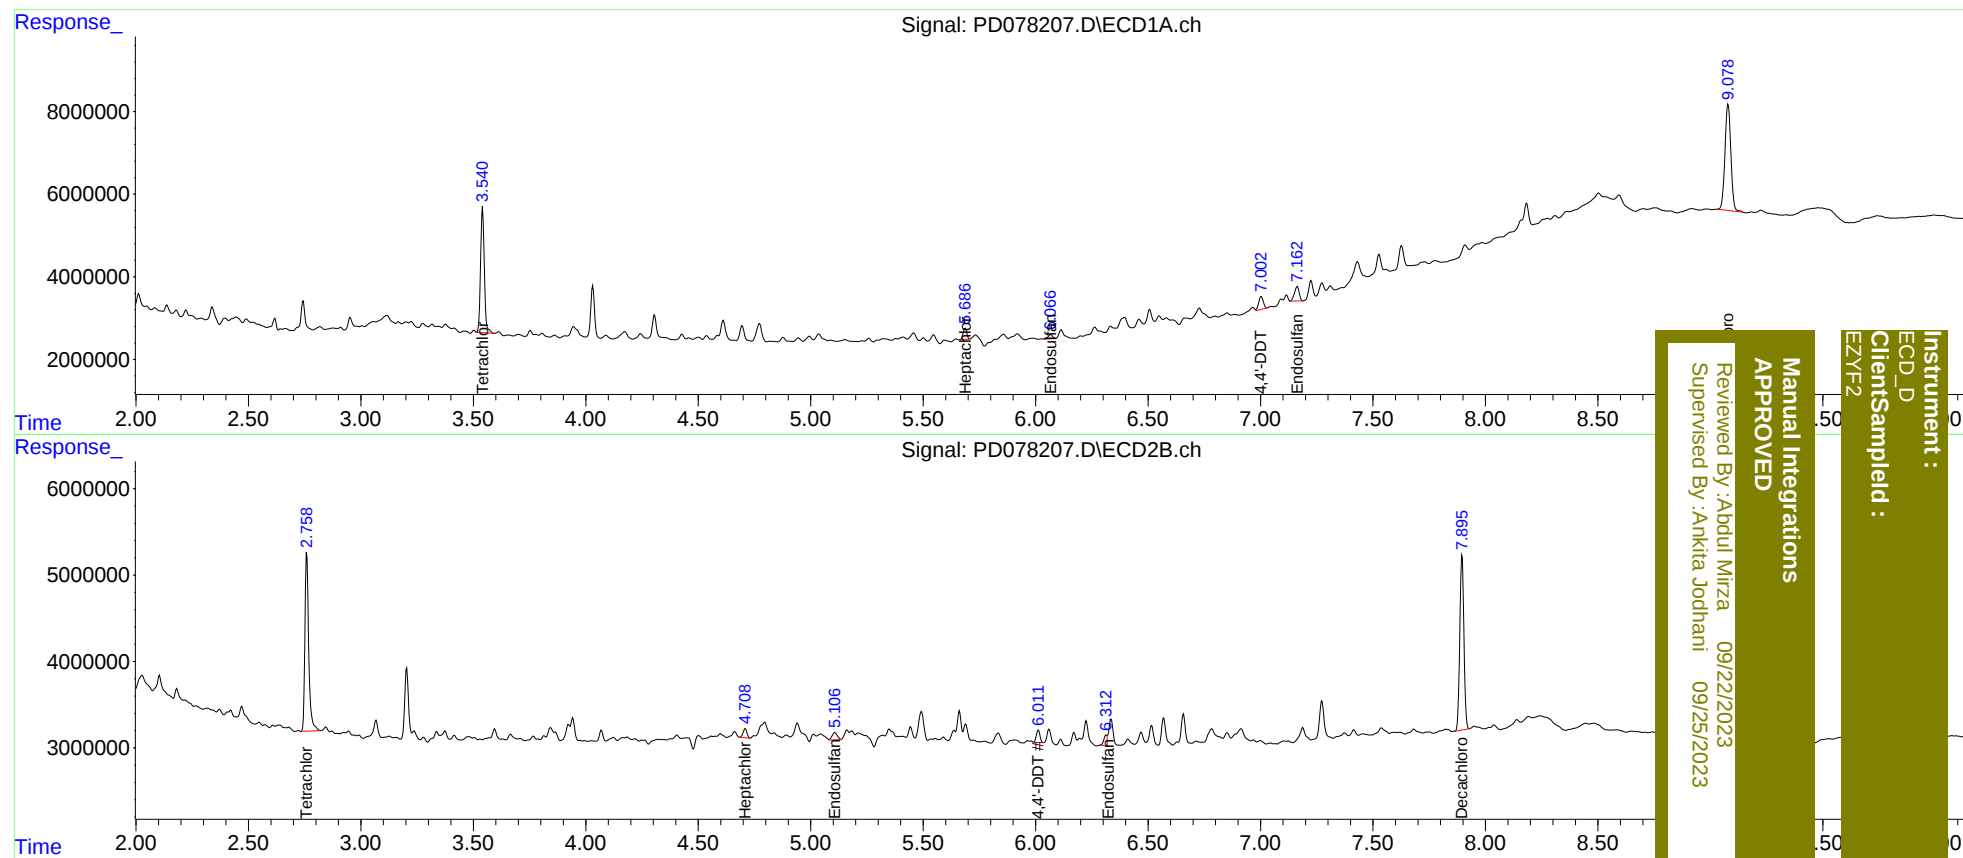

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/22/2023
Supervised By: Ankita Jodhani 09/25/2023

Instrument :
ECD_D
ClientSampled :
EZYF2