

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
 Data File : PD078214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2023 21:31
 Operator : AR\AJ
 Sample : 04417-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYE6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/22/2023
 Supervised By : Ankita Jodhani 09/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 01:02:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.760	27941953	39049580	11.011m	26.423 #
2)	SA Decachlor...	9.076	7.894	53297295	29851532	17.061	18.432
Target Compounds							
5)	MB Aldrin	5.258	4.218	32553204	10162088	7.798	4.534 #
19)	B Endosulfa...	7.162	6.336	527.7E6	396.8E6	174.147m	240.145 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
Data File : PD078214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2023 21:31
Operator : AR\AJ
Sample : 04417-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 01:02:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

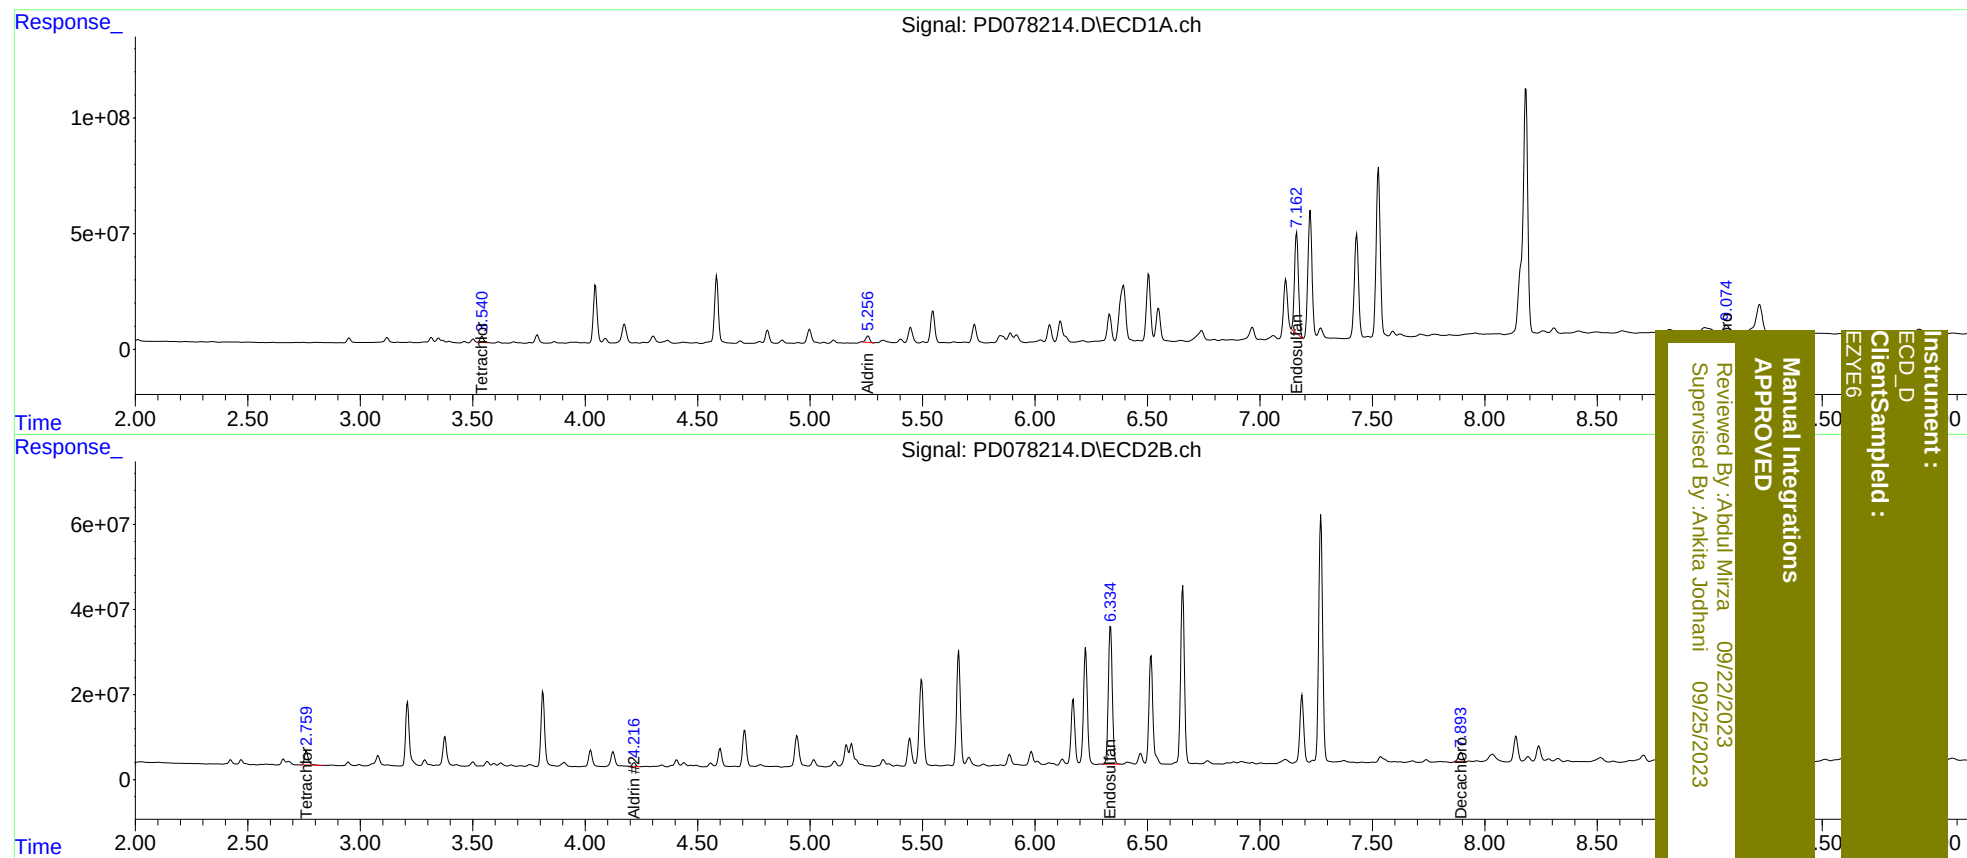

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/22/2023
Supervised By: Ankita Jodhani 09/25/2023

Instrument :
ECD_D
Client Sampled :
EZY6