

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
 Data File : PD078224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2023 01:44
 Operator : AR\AJ
 Sample : 04417-11DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYM9DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/22/2023
 Supervised By : Ankita Jodhani 09/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 05:49:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.758	5621092	5882107	2.215m	3.980m#
2)	SA Decachlor...	9.072	7.896	12740196	3549032	4.078m	2.191 #
Target Compounds							
14)	MA Endrin	6.589	5.626	23201749	18003247	7.520	9.847 #
15)	B Endosulfa...	6.801	5.905	48343324	11438824	14.600	6.321 #
17)	MA 4,4'-DDT	7.004	6.012	202.0E6	102.1E6	73.724m	72.224
19)	B Endosulfa...	7.147	6.312	92623637	67136400	30.566m	40.633 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
Data File : PD078224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2023 01:44
Operator : AR\AJ
Sample : 04417-11DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 05:49:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

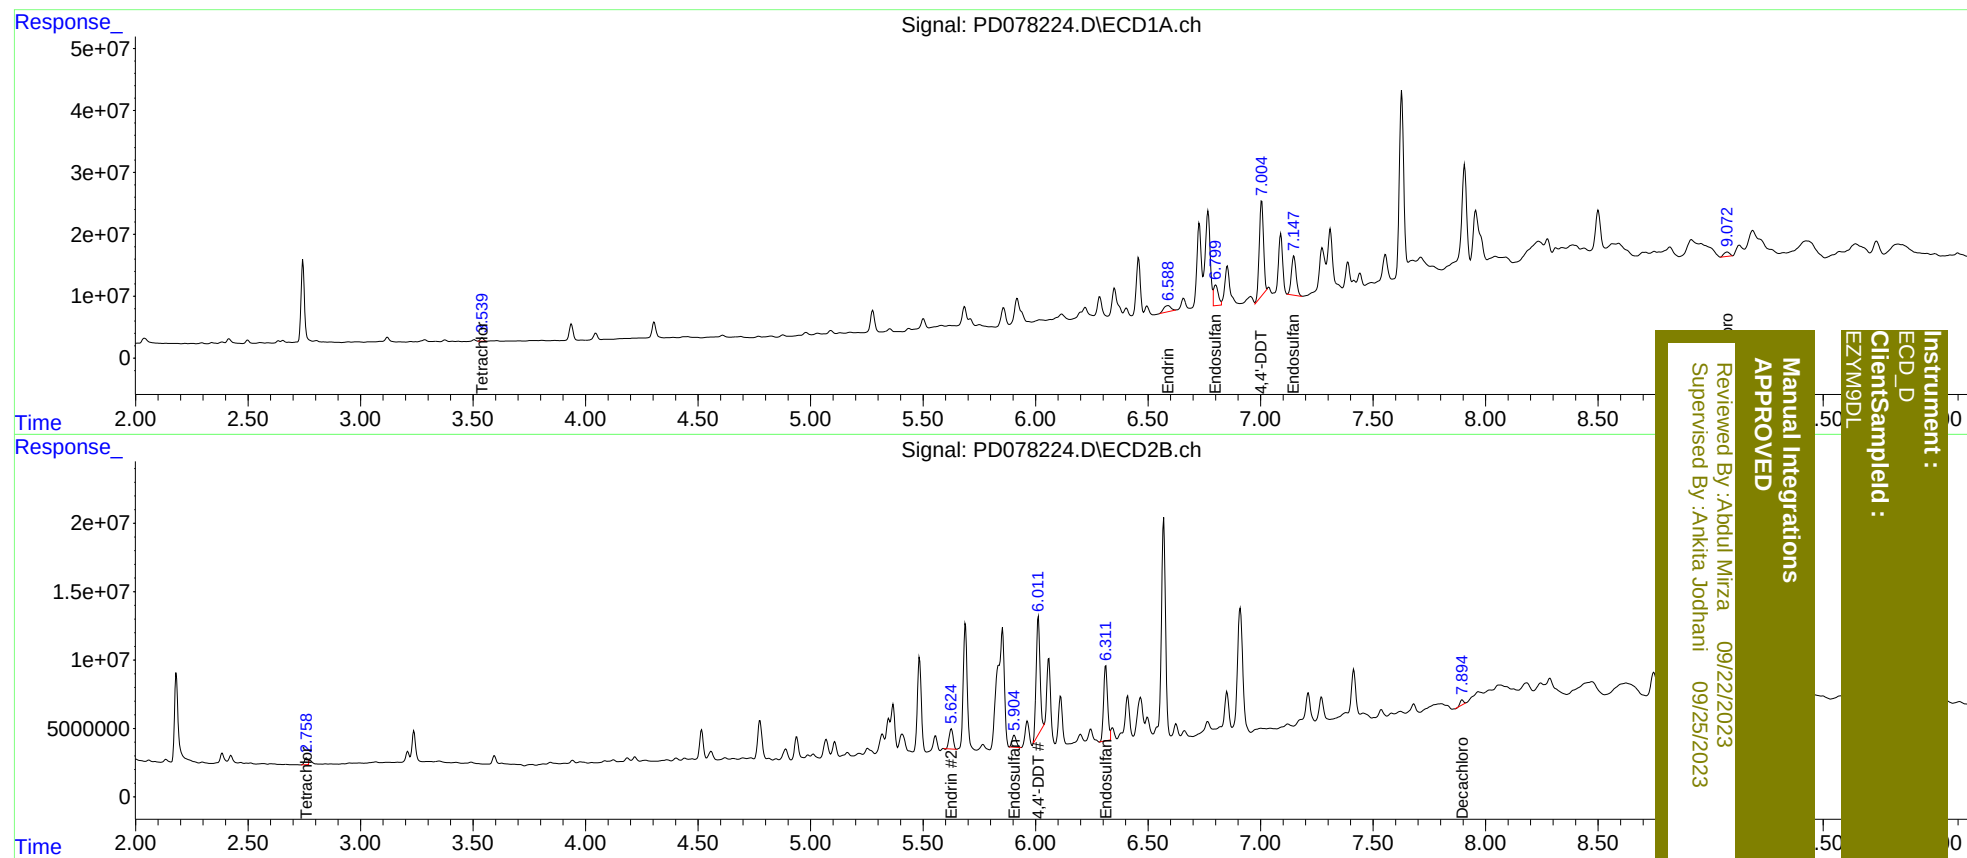

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/22/2023
Supervised By: Ankita Jodhani 09/25/2023

Instrument :
ECD_D
Client Sampled :
EZYM9DL