

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
 Data File : PD078225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2023 02:11
 Operator : AR\AJ
 Sample : 04417-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYN0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/27/2023
 Supervised By : Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 05:49:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.759	36277275	29194724	14.295m	19.754 #
2)	SA Decachlor...	9.075	7.895	54776046	22943014	17.534	14.167
Target Compounds							
10)	B trans-Chl...	5.915	4.938	26725402	6662760	7.178m	3.337m#
13)	MA Dieldrin	6.350	5.344	20307220	23425393	5.425	11.336m#
15)	B Endosulfa...	6.797	5.907	11811291	6800081	3.567	3.758
17)	MA 4,4'-DDT	7.003	6.010	53127008	37739315	19.391m	26.702m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092323\
Data File : PD078225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2023 02:11
Operator : AR\AJ
Sample : 04417-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 05:49:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

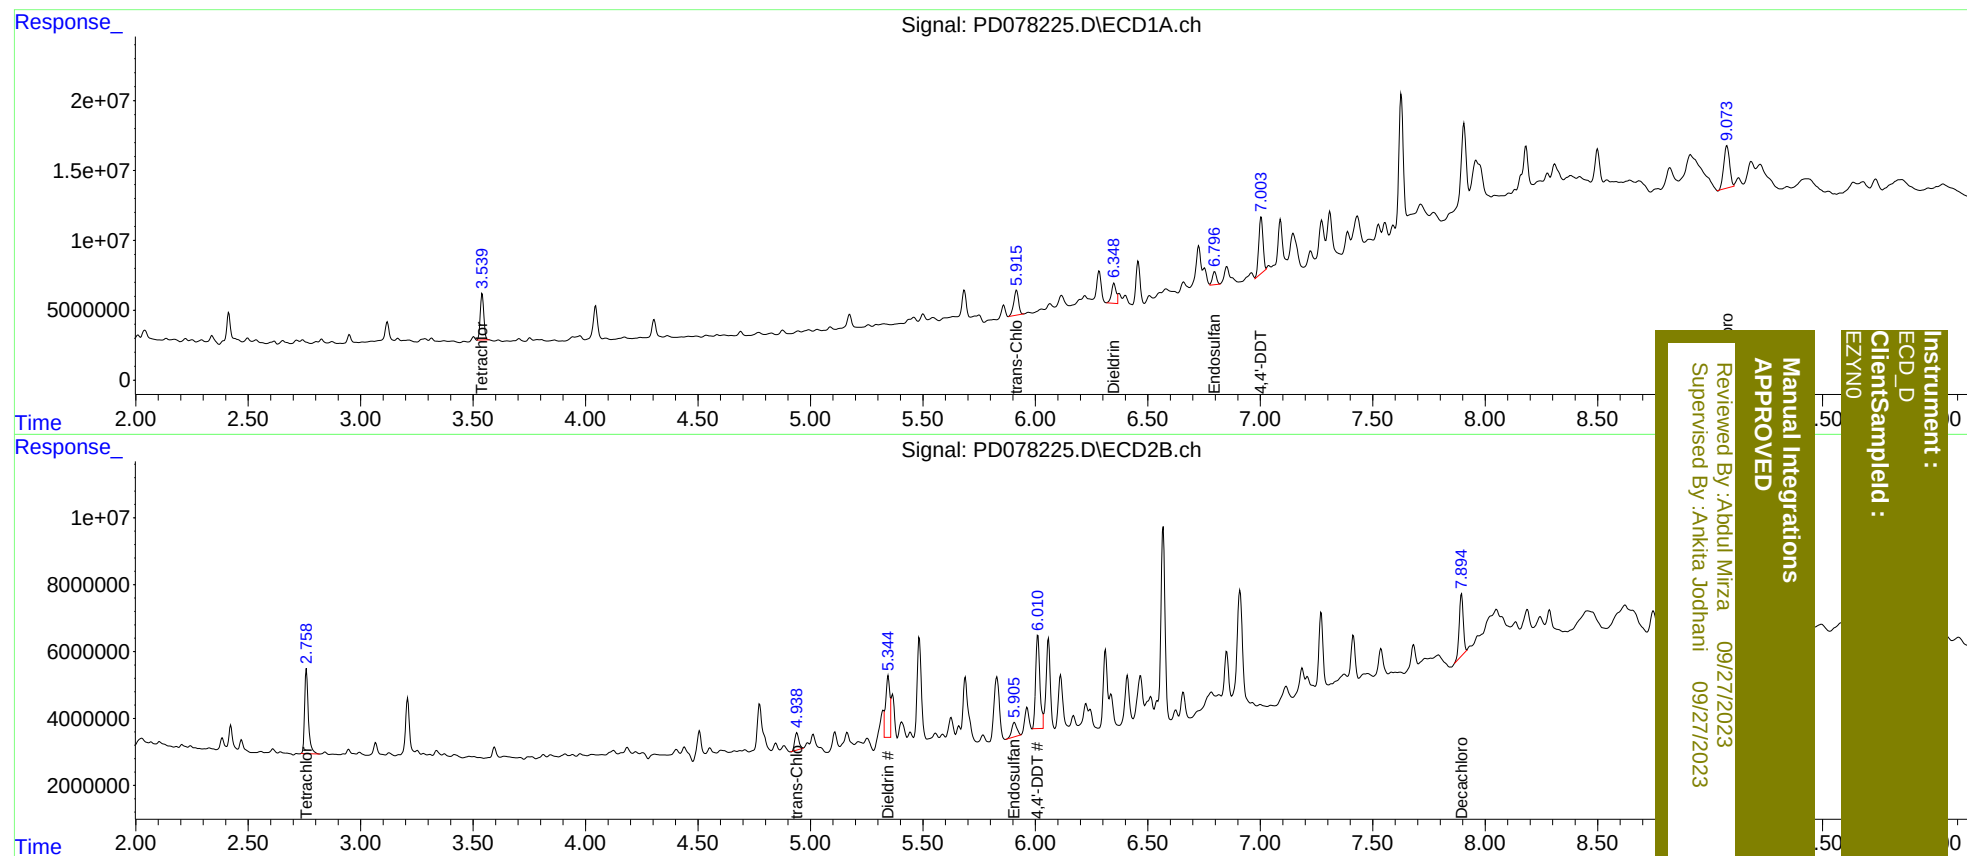

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/27/2023
Supervised By: Ankita Jodhani 09/27/2023

Instrument :
ECD_D
ClientSampled :
EZYNO