

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 12:02
 Operator : AR\AJ
 Sample : P4080-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:33:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	2.892	22853083	57163671	18.872	15.123
27)	SA Decachlor...	8.958	8.084	31281613	60149891	19.069	22.500
Target Compounds							
3)	MA gamma-BHC...	4.216f	0.000	196.8E6	0	78.675	N.D. #
7)	B delta-BHC	4.710	0.000	2364470	0	1.037	N.D. #
8)	B Heptachlo...	5.565f	0.000	856630	0	0.429	N.D. #
15)	B Endosulfa...	6.702	0.000	1574102	0	0.859	N.D. #
16)	A 4,4'-DDD	6.622	0.000	112379	0	<MDL	N.D. #
20)	A Methoxychlor	7.465f	0.000	3285287	0	4.490	N.D. #
26)	Toxaphene-5	7.874	0.000	9409289	0	408.565	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 12:02
Operator : AR\AJ
Sample : P4080-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:33:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

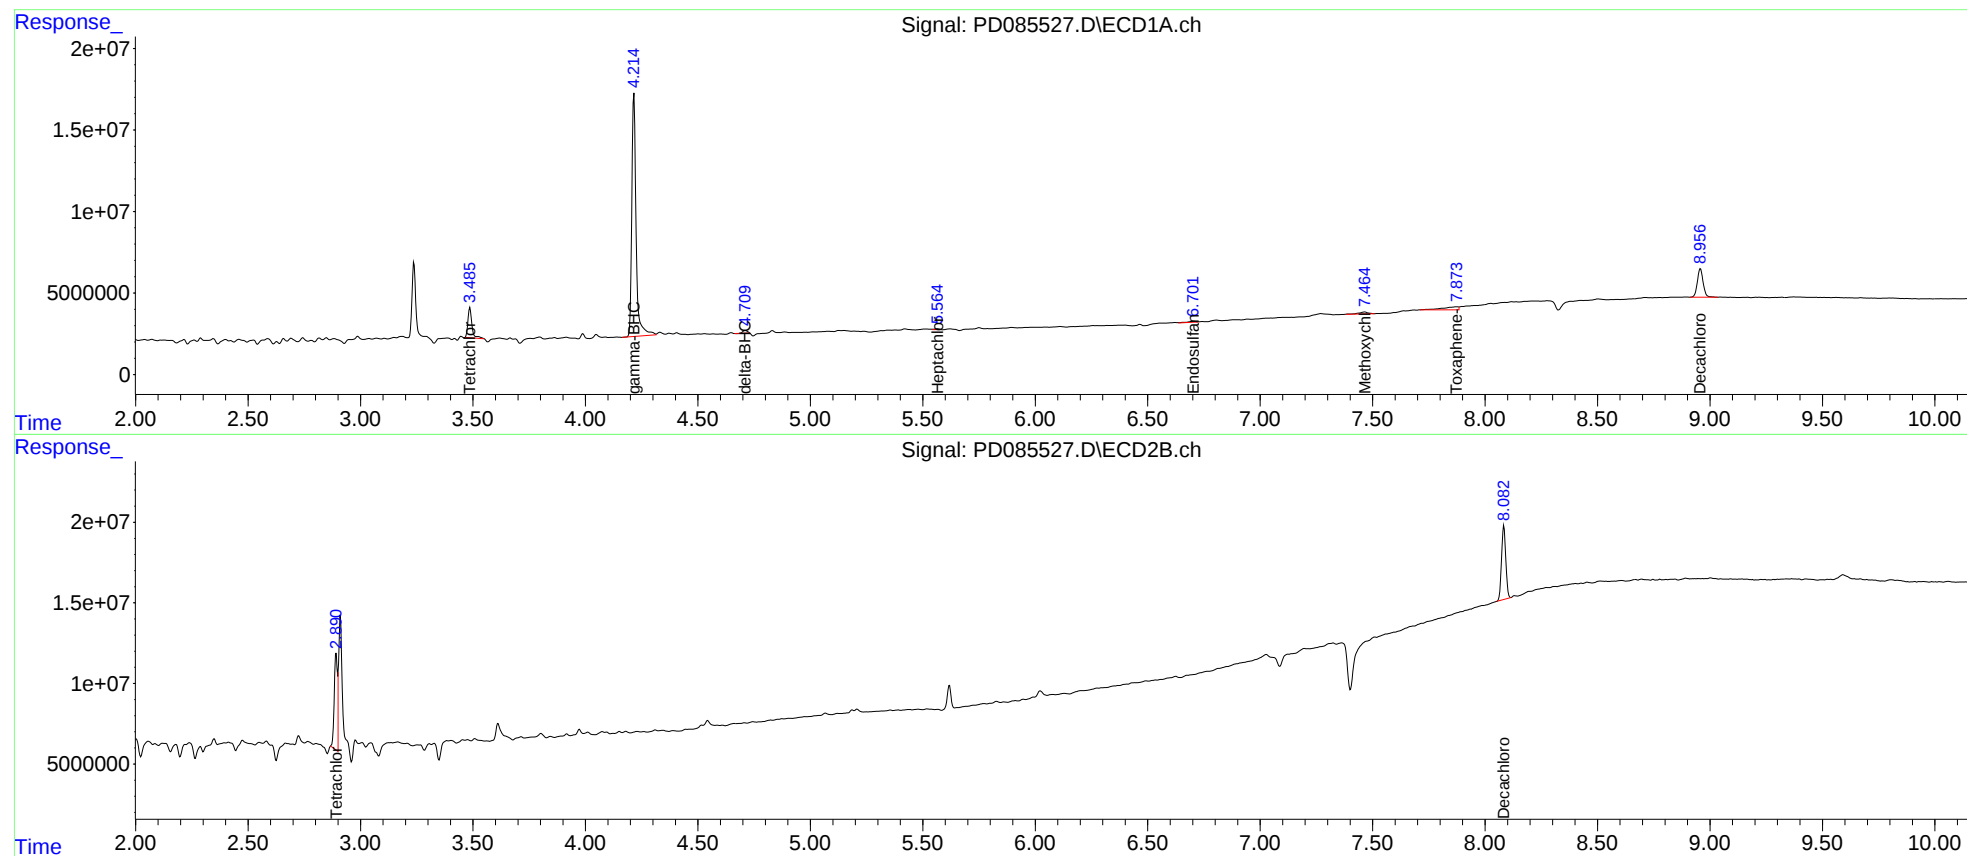

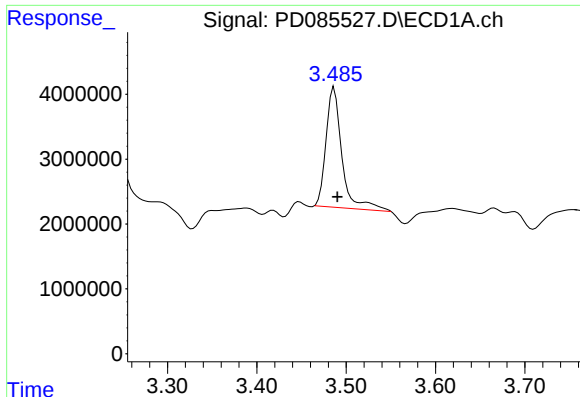


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.003 min
Response: 22853083
Conc: 18.87 ng/ml

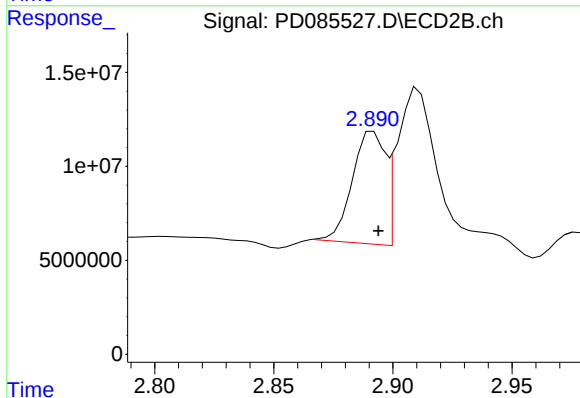


#1 Tetrachloro-m-xylene

R.T.: 2.892 min
Delta R.T.: -0.002 min
Response: 57163671
Conc: 15.12 ng/ml

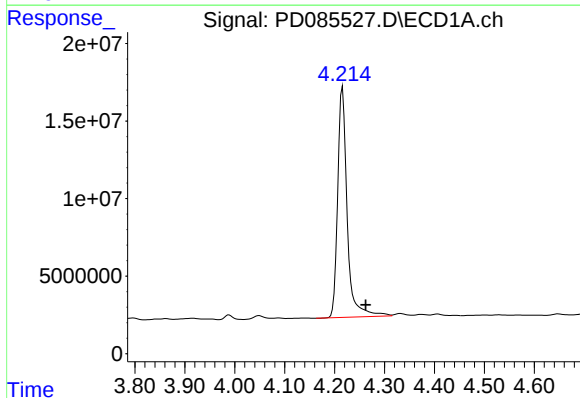


#3 gamma-BHC (Lindane)

R.T.: 4.216 min
Delta R.T.: -0.046 min
Response: 196831136
Conc: 78.67 ng/ml

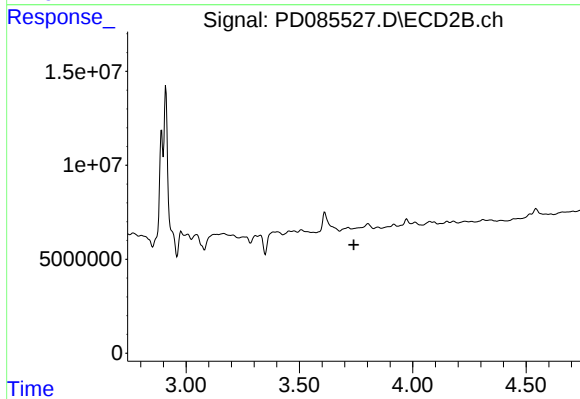


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.739 min
Response: 0
Conc: N.D.

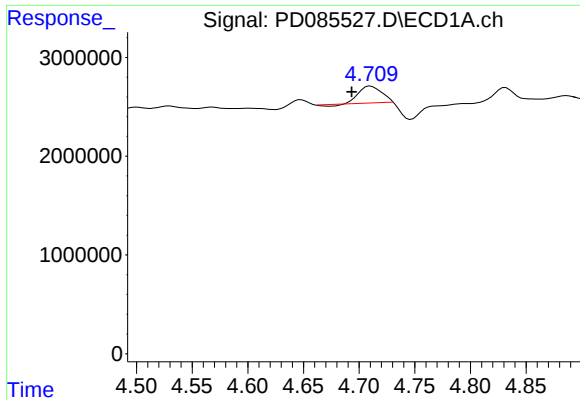


#7 delta-BHC

R.T.: 4.710 min
Delta R.T.: 0.017 min
Response: 2364470
Conc: 1.04 ng/ml

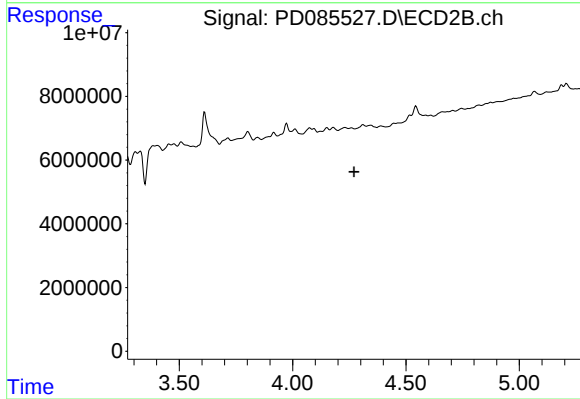


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.271 min
Response: 0
Conc: N.D.

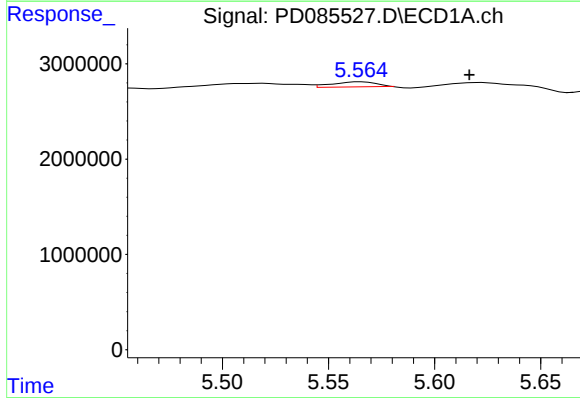


#8 Heptachlor epoxide

R.T.: 5.565 min
Delta R.T.: -0.051 min
Response: 856630
Conc: 0.43 ng/ml

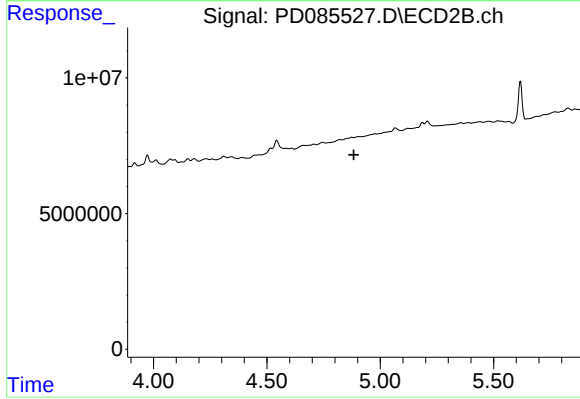


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.883 min
Response: 0
Conc: N.D.

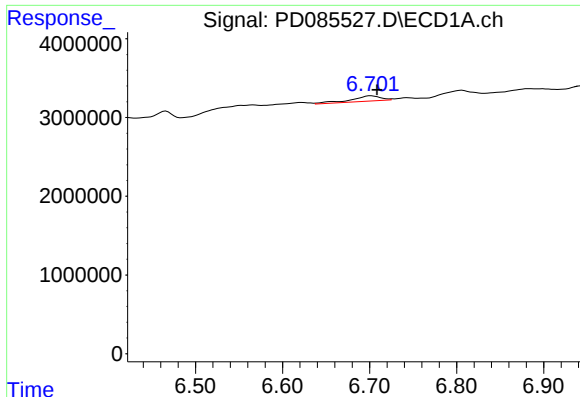


#15 Endosulfan II

R.T.: 6.702 min
Delta R.T.: -0.006 min
Response: 1574102
Conc: 0.86 ng/ml

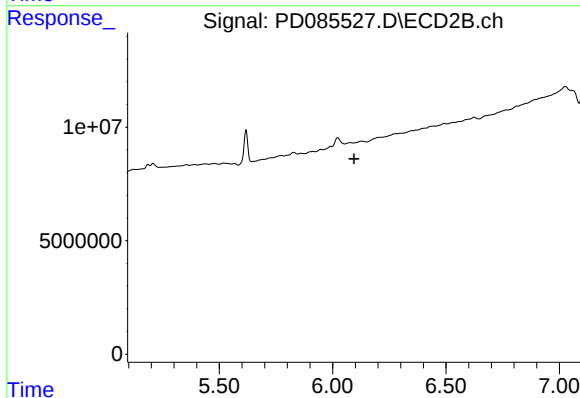


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

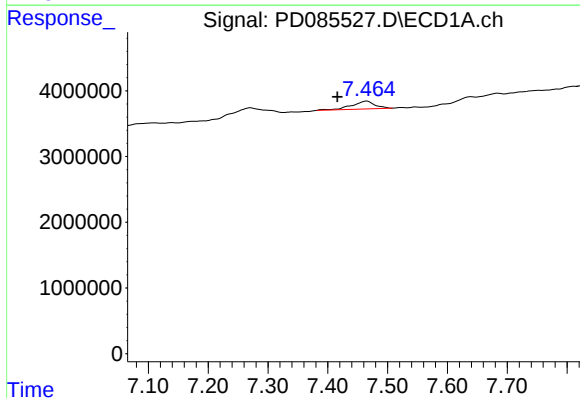


#20 Methoxychlor

R.T.: 7.465 min
Delta R.T.: 0.049 min
Response: 3285287
Conc: 4.49 ng/ml

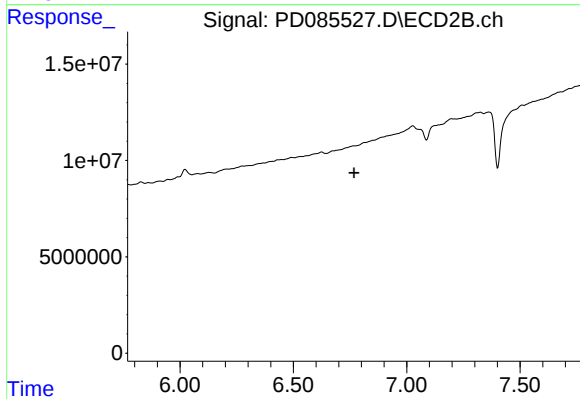


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

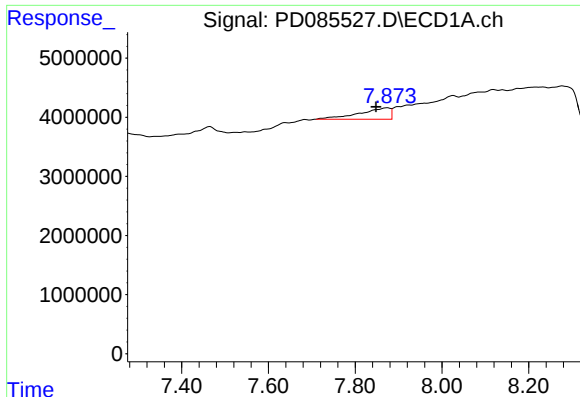


#26 Toxaphene-5

R.T.: 7.874 min
Delta R.T.: 0.026 min
Response: 9409289
Conc: 408.56 ng/ml

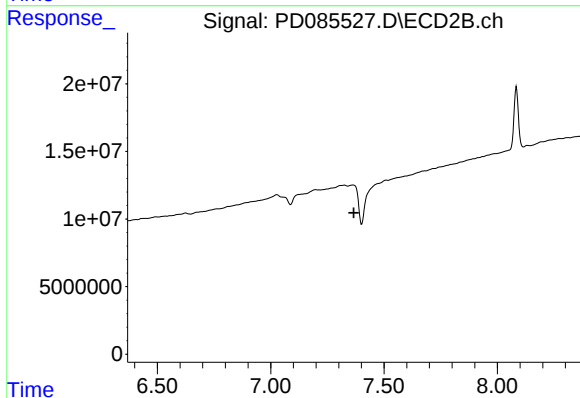


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.367 min
Response: 0
Conc: N.D.

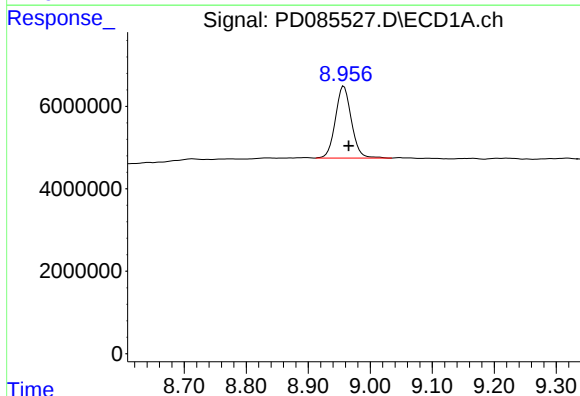

#27 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.008 min
Response: 31281613
Conc: 19.07 ng/ml

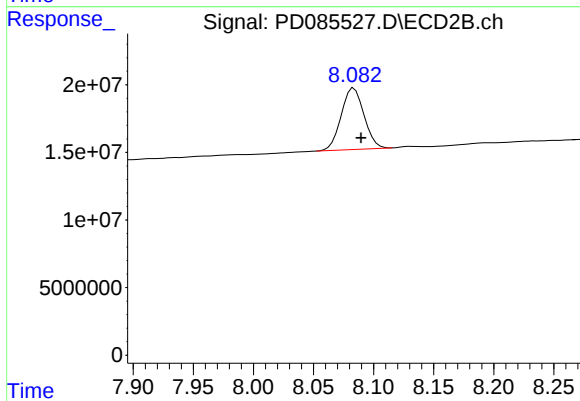

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.006 min
Response: 60149891
Conc: 22.50 ng/ml