

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 12:15
 Operator : AR\AJ
 Sample : P4080-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:33:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	2.891	25586264	82650126	21.129	21.866
27)	SA Decachlor...	8.958	8.085	30094184	59158192	18.345	22.129
Target Compounds							
3)	MA gamma-BHC...	4.216f	0.000	95670455	0	38.240	N.D. #
7)	B delta-BHC	4.708	0.000	3563304	0	1.563	N.D. #
15)	B Endosulfa...	6.691	0.000	1167550	0	0.637	N.D. #
16)	A 4,4'-DDD	6.691f	0.000	1167550	0	0.886	N.D. #
20)	A Methoxychlor	7.465f	0.000	2519153	0	3.443	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 12:15
Operator : AR\AJ
Sample : P4080-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:33:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

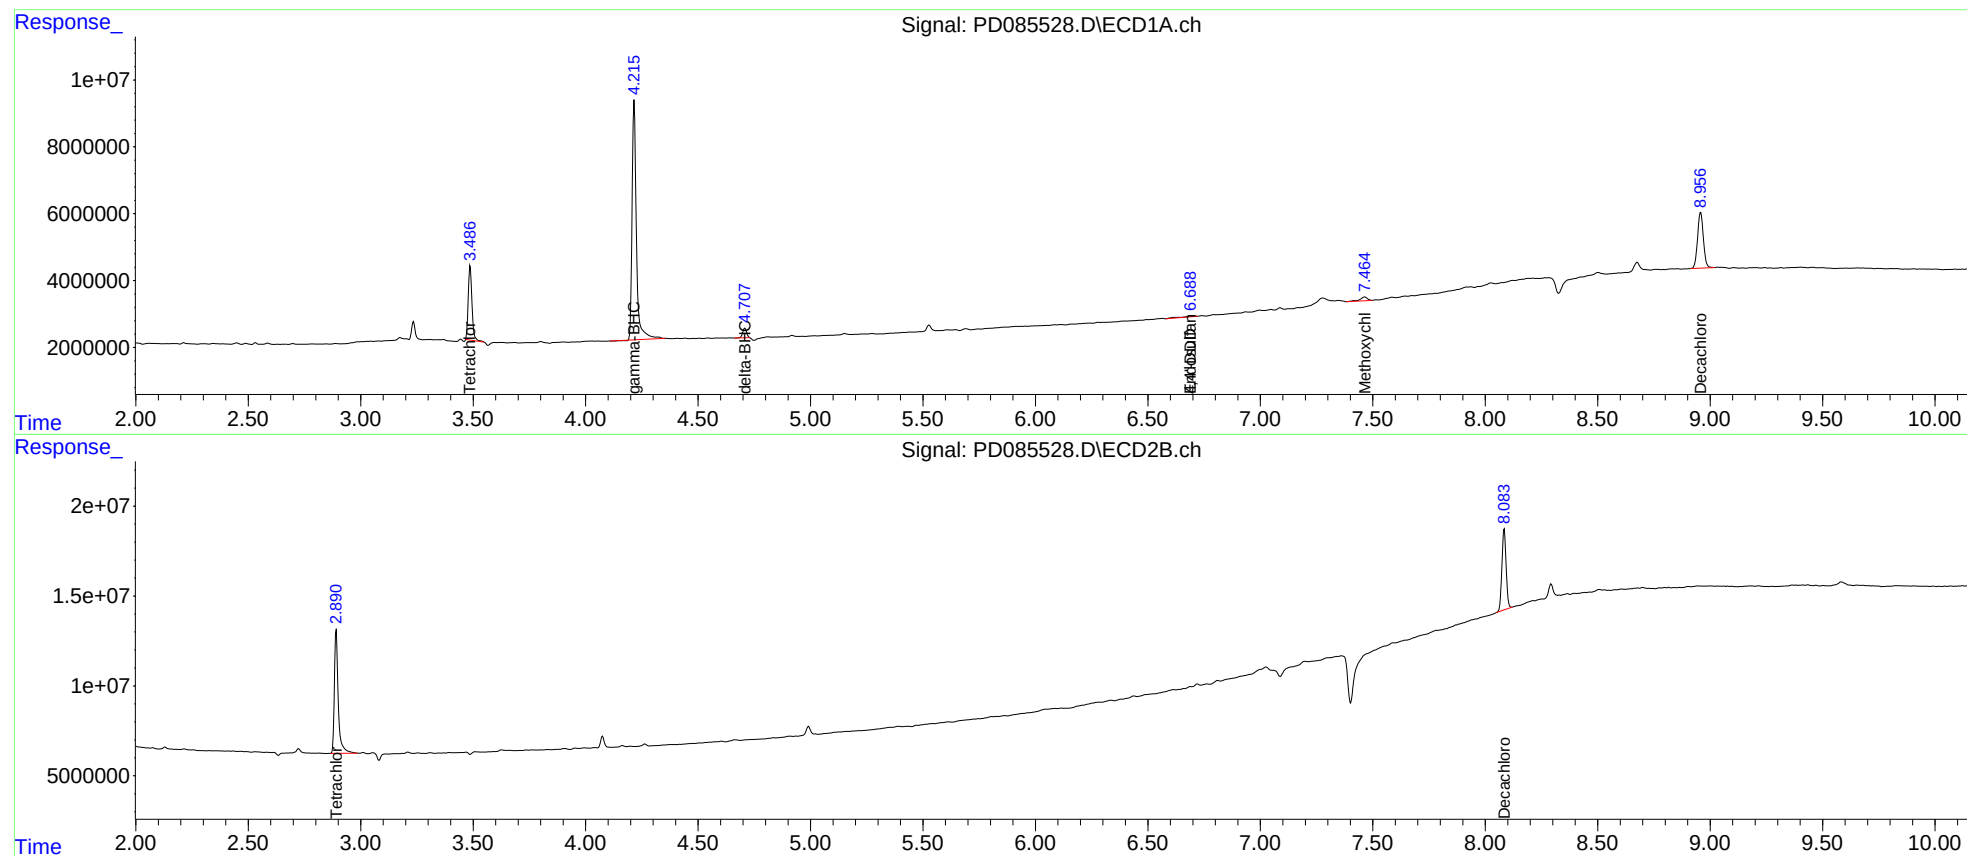

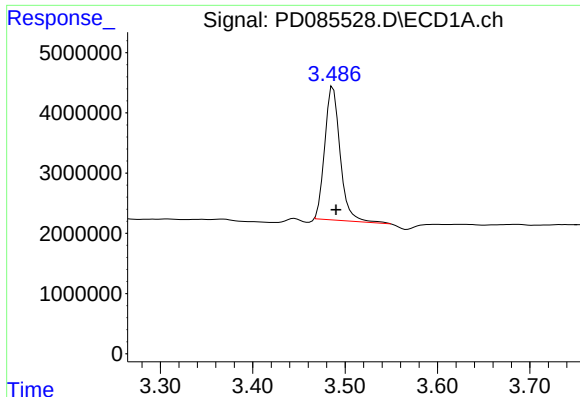


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.003 min
Response: 25586264
Conc: 21.13 ng/ml

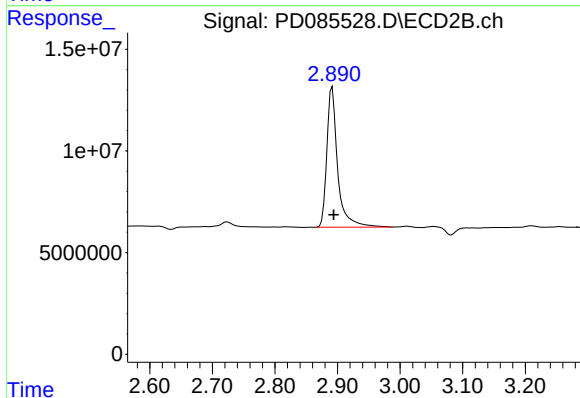


#1 Tetrachloro-m-xylene

R.T.: 2.891 min
Delta R.T.: -0.003 min
Response: 82650126
Conc: 21.87 ng/ml

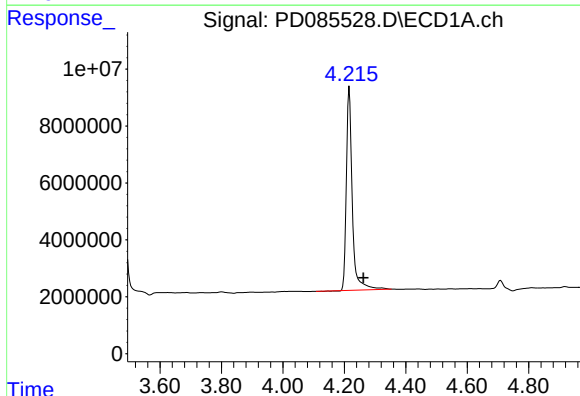


#3 gamma-BHC (Lindane)

R.T.: 4.216 min
Delta R.T.: -0.046 min
Response: 95670455
Conc: 38.24 ng/ml

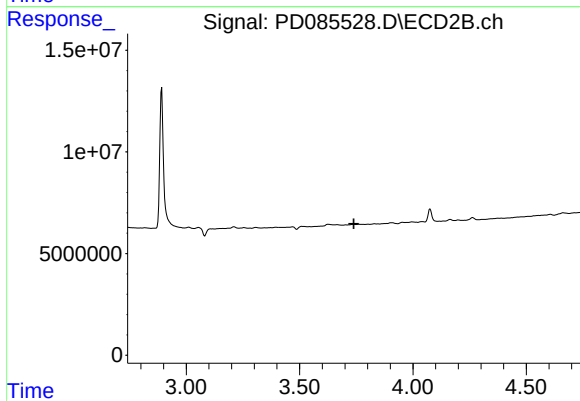


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.739 min
Response: 0
Conc: N.D.

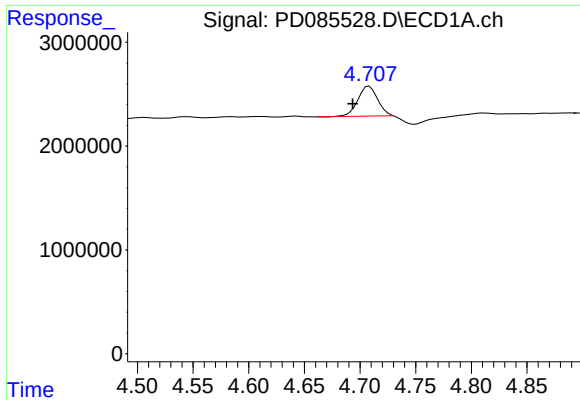


#7 delta-BHC

R.T.: 4.708 min
Delta R.T.: 0.015 min
Response: 3563304
Conc: 1.56 ng/ml

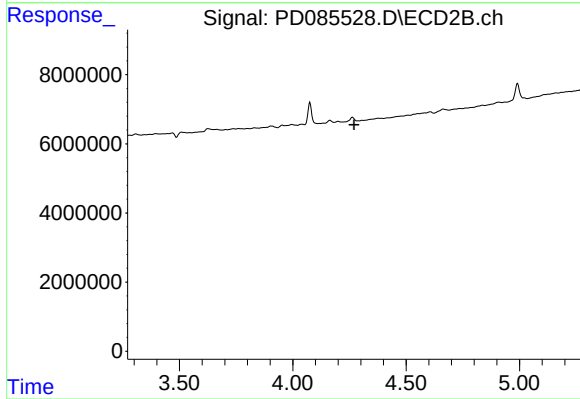


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.271 min
Response: 0
Conc: N.D.

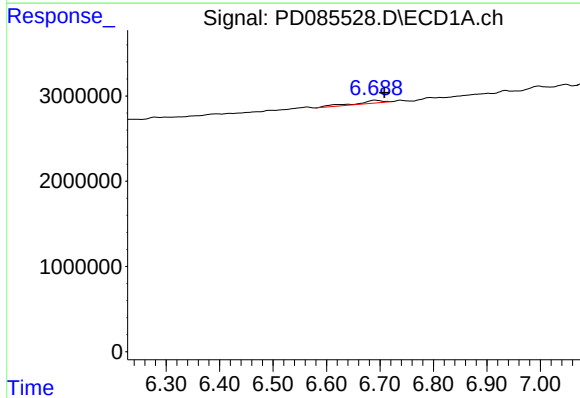


#15 Endosulfan II

R.T.: 6.691 min
Delta R.T.: -0.017 min
Response: 1167550
Conc: 0.64 ng/ml

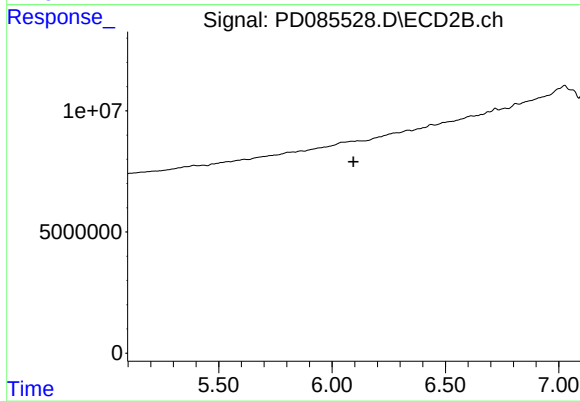


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

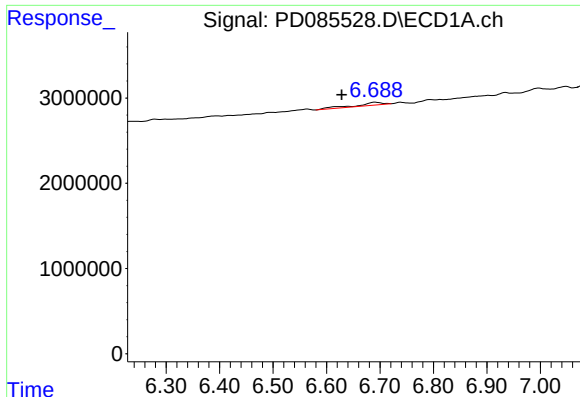


#16 4,4'-DDD

R.T.: 6.691 min
Delta R.T.: 0.062 min
Response: 1167550
Conc: 0.89 ng/ml

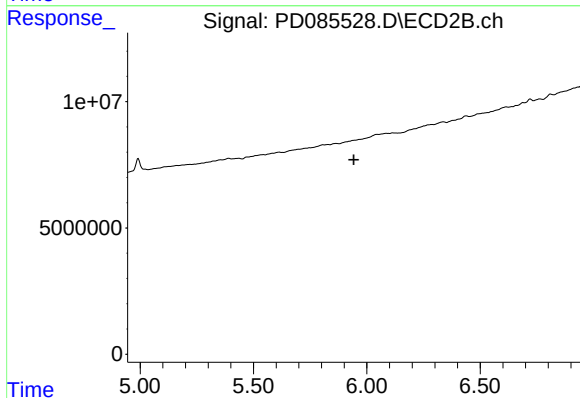


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

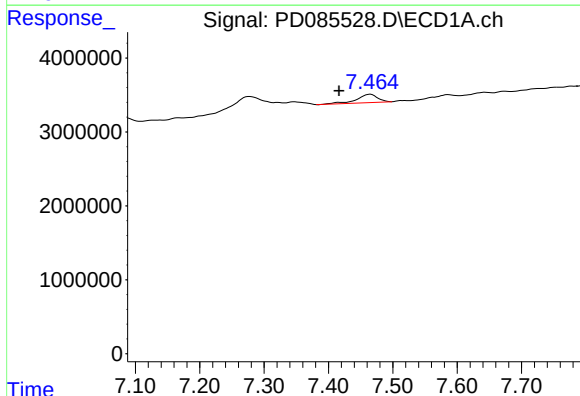


#20 Methoxychlor

R.T.: 7.465 min
Delta R.T.: 0.048 min
Response: 2519153
Conc: 3.44 ng/ml

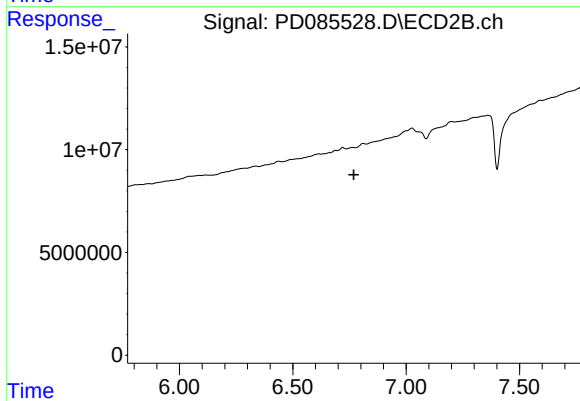


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

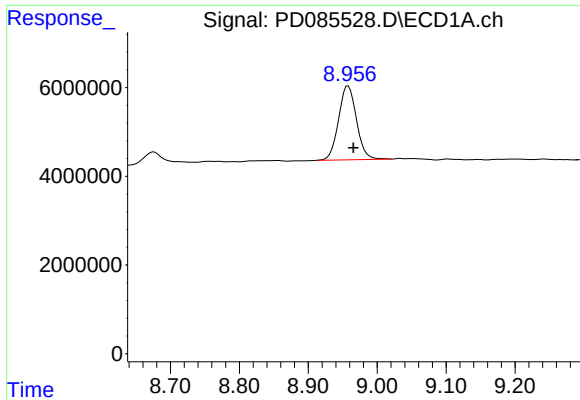

#27 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.008 min
Response: 30094184
Conc: 18.35 ng/ml

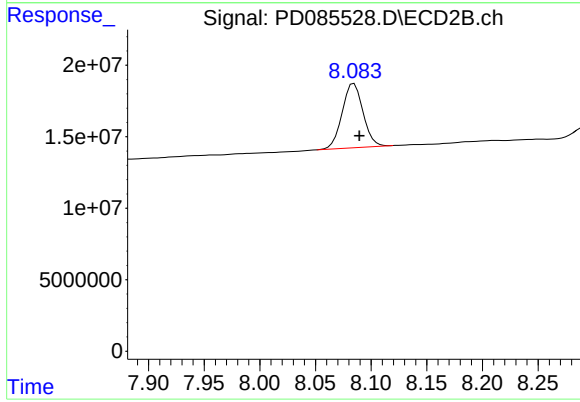

#27 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.005 min
Response: 59158192
Conc: 22.13 ng/ml