

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 12:29
 Operator : AR\AJ
 Sample : P4080-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:33:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	2.892	25134465	85190153	20.755	22.538
27)	SA Decachlor...	8.959	8.084	29560055	57646101	18.019	21.564
Target Compounds							
3)	MA gamma-BHC...	4.216f	0.000	123.3E6	0	49.293	N.D. #
4)	MA Heptachlor	0.000	4.075	0	40791189	N.D.	8.593
6)	B beta-BHC	0.000	4.075f	0	40791189	N.D.	17.541
7)	B delta-BHC	4.710	0.000	18165264	0	7.969	N.D. #
15)	B Endosulfa...	6.697	0.000	777018	0	0.424	N.D. #
16)	A 4,4'-DDD	6.697f	0.000	777018	0	0.590	N.D. #
20)	A Methoxychlor	7.465f	0.000	2264468	0	3.095	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 12:29
Operator : AR\AJ
Sample : P4080-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:33:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

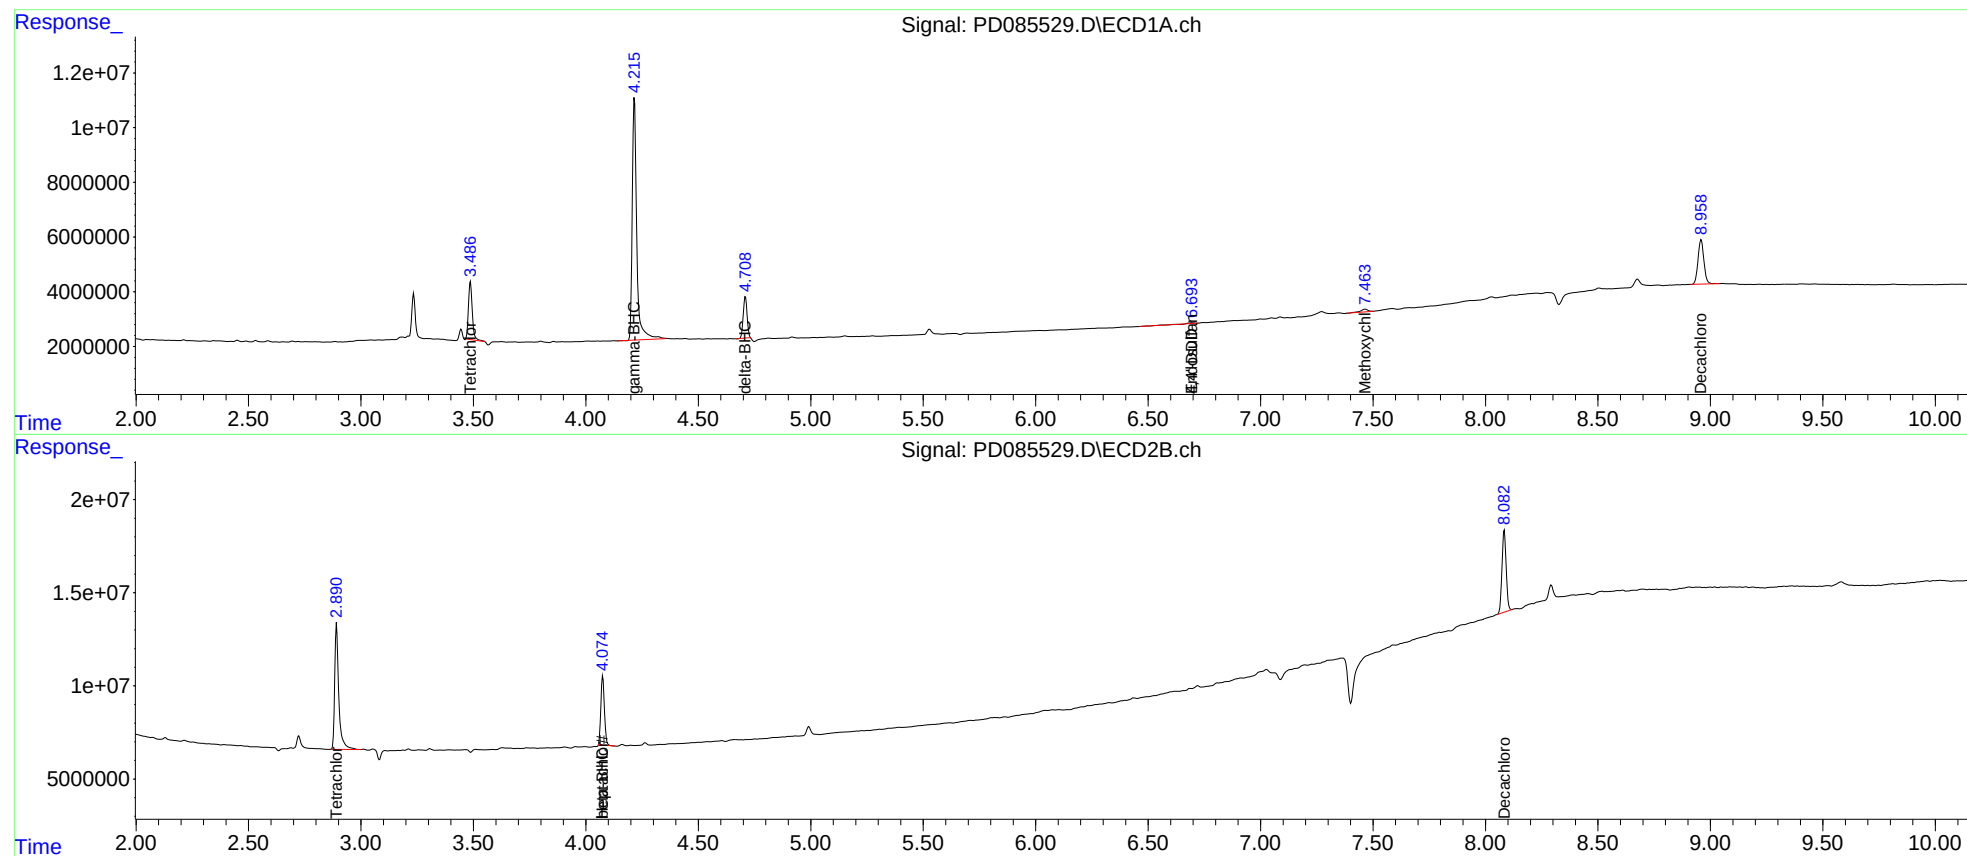

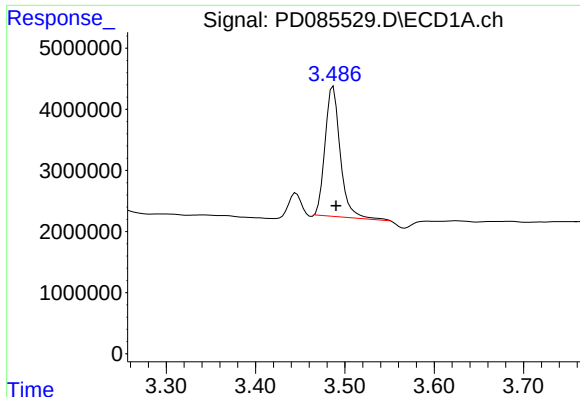


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.003 min
Response: 25134465
Conc: 20.76 ng/ml

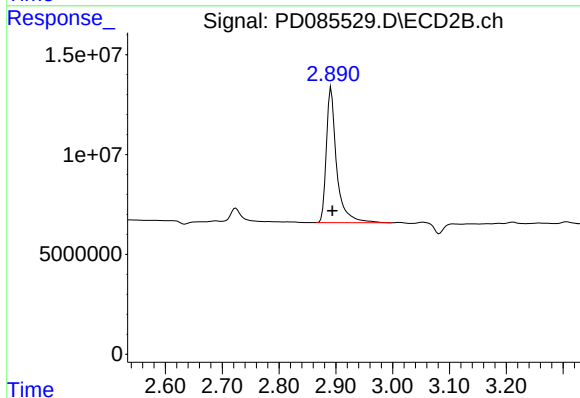


#1 Tetrachloro-m-xylene

R.T.: 2.892 min
Delta R.T.: -0.002 min
Response: 85190153
Conc: 22.54 ng/ml

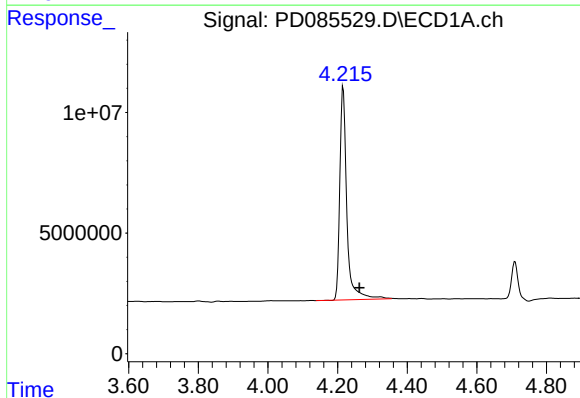


#3 gamma-BHC (Lindane)

R.T.: 4.216 min
Delta R.T.: -0.046 min
Response: 123321816
Conc: 49.29 ng/ml

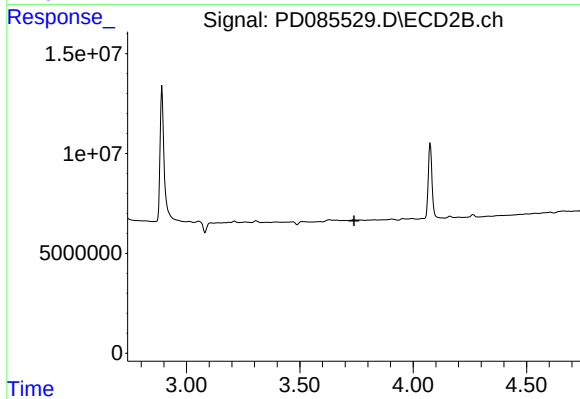


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.739 min
Response: 0
Conc: N.D.

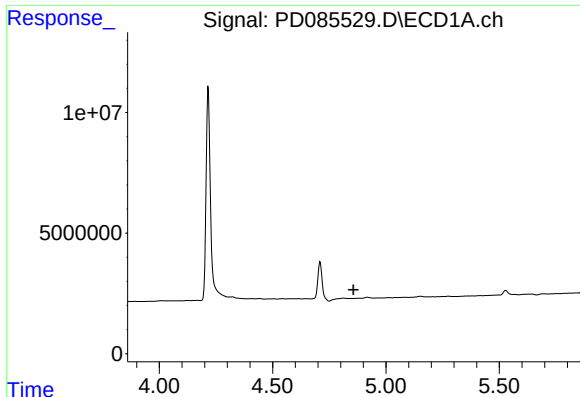


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

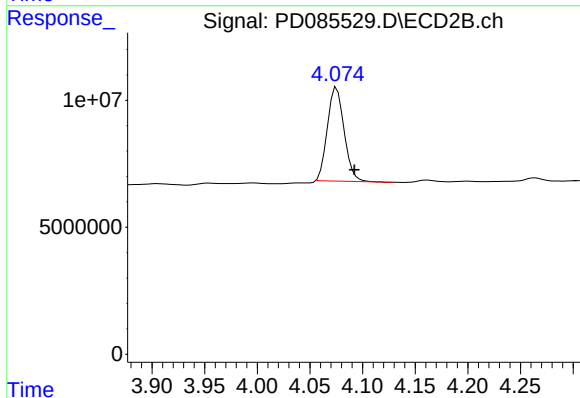


#4 Heptachlor

R.T.: 4.075 min
Delta R.T.: -0.017 min
Response: 40791189
Conc: 8.59 ng/ml

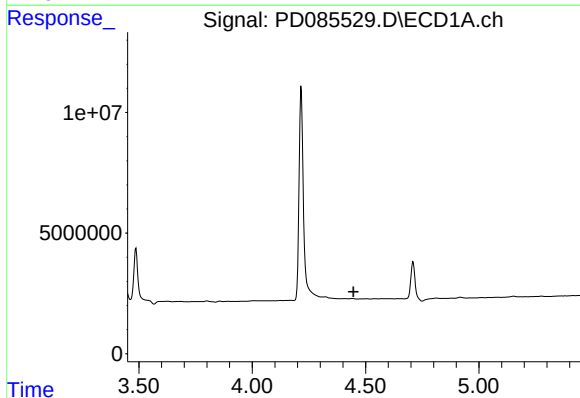


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.447 min
Response: 0
Conc: N.D.

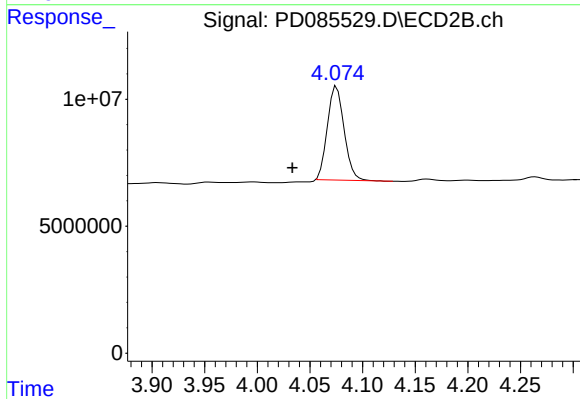


#6 beta-BHC

R.T.: 4.075 min
Delta R.T.: 0.042 min
Response: 40791189
Conc: 17.54 ng/ml

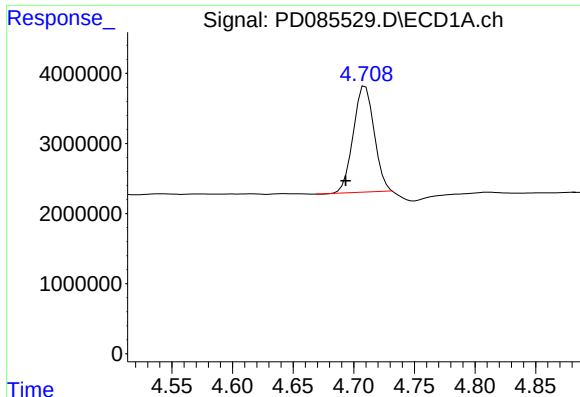


#7 delta-BHC

R.T.: 4.710 min
Delta R.T.: 0.016 min
Response: 18165264
Conc: 7.97 ng/ml

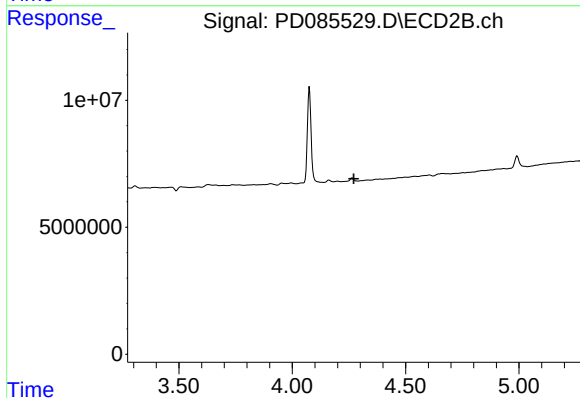


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.271 min
Response: 0
Conc: N.D.

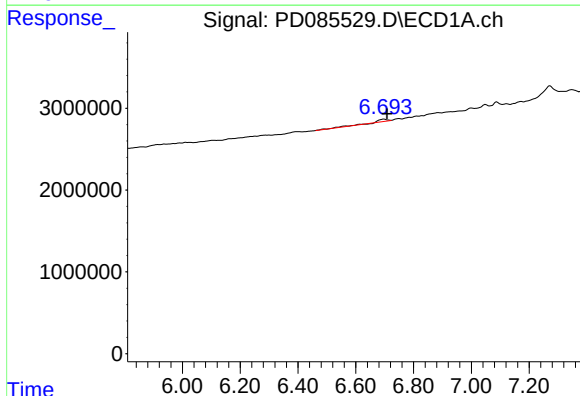


#15 Endosulfan II

R.T.: 6.697 min
Delta R.T.: -0.011 min
Response: 777018
Conc: 0.42 ng/ml

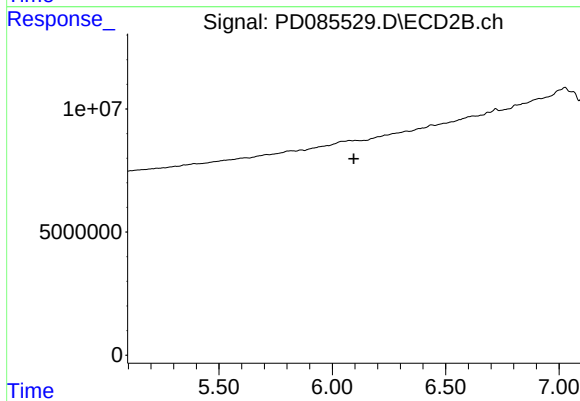


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

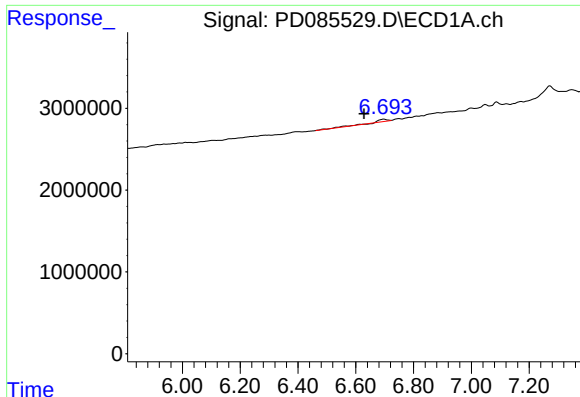


#16 4,4'-DDD

R.T.: 6.697 min
Delta R.T.: 0.069 min
Response: 777018
Conc: 0.59 ng/ml

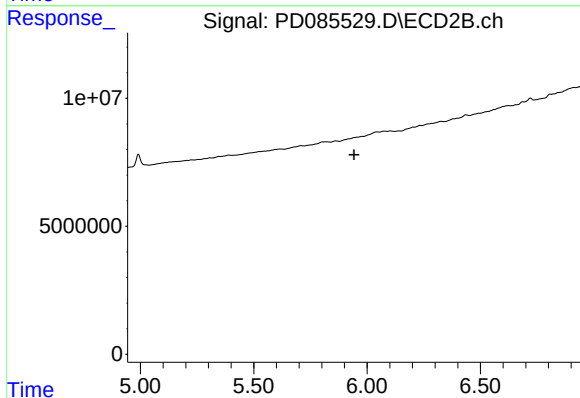


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

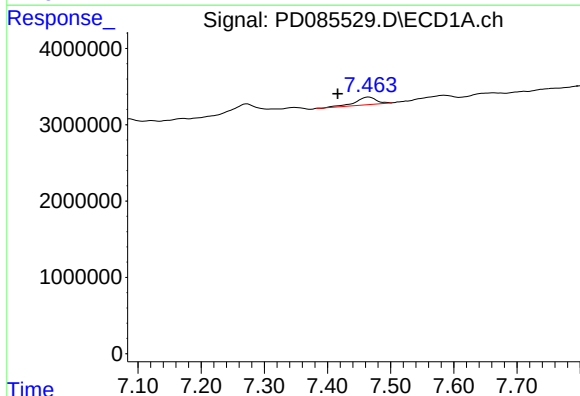


#20 Methoxychlor

R.T.: 7.465 min
Delta R.T.: 0.049 min
Response: 2264468
Conc: 3.10 ng/ml

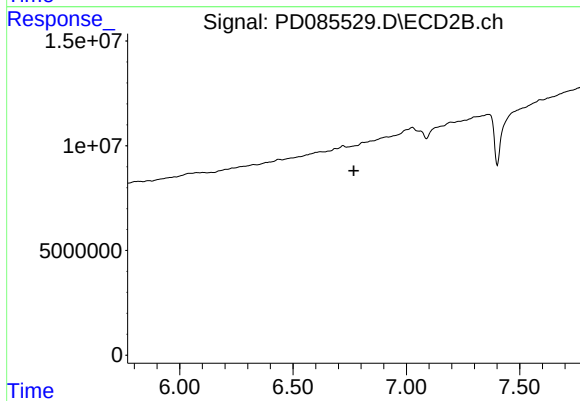


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

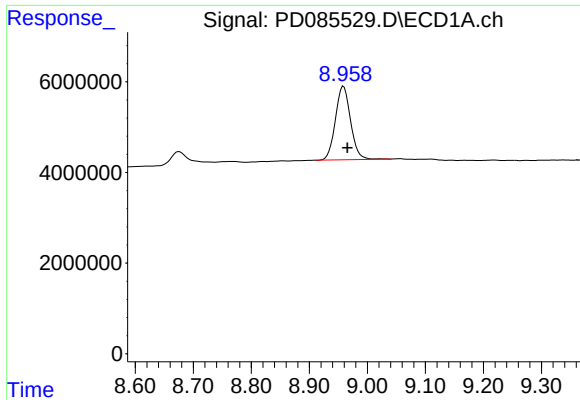

#27 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.006 min
Response: 29560055
Conc: 18.02 ng/ml

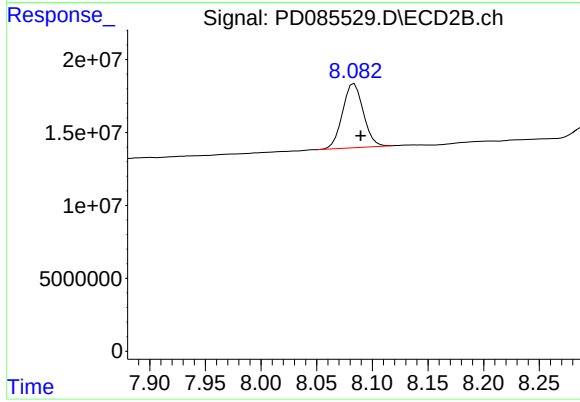

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.006 min
Response: 57646101
Conc: 21.56 ng/ml