

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 12:42
 Operator : AR\AJ
 Sample : P4080-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:33:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	2.892	25590250	81796137	21.132	21.640
27)	SA Decachlor...	8.958	8.085	32231949	59734436	19.648	22.345
Target Compounds							
3)	MA gamma-BHC...	4.216f	0.000	106.8E6	0	42.671	N.D. #
4)	MA Heptachlor	0.000	4.076	0	32889965	N.D.	6.929
6)	B beta-BHC	0.000	4.076f	0	32889965	N.D.	14.143
7)	B delta-BHC	4.709	0.000	14118482	0	6.193	N.D. #
15)	B Endosulfa...	6.694	0.000	349852	0	0.191	N.D. #
16)	A 4,4'-DDD	6.694f	0.000	349852	0	0.266	N.D. #
20)	A Methoxychlor	7.466f	0.000	1904111	0	2.603	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 12:42
Operator : AR\AJ
Sample : P4080-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:33:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

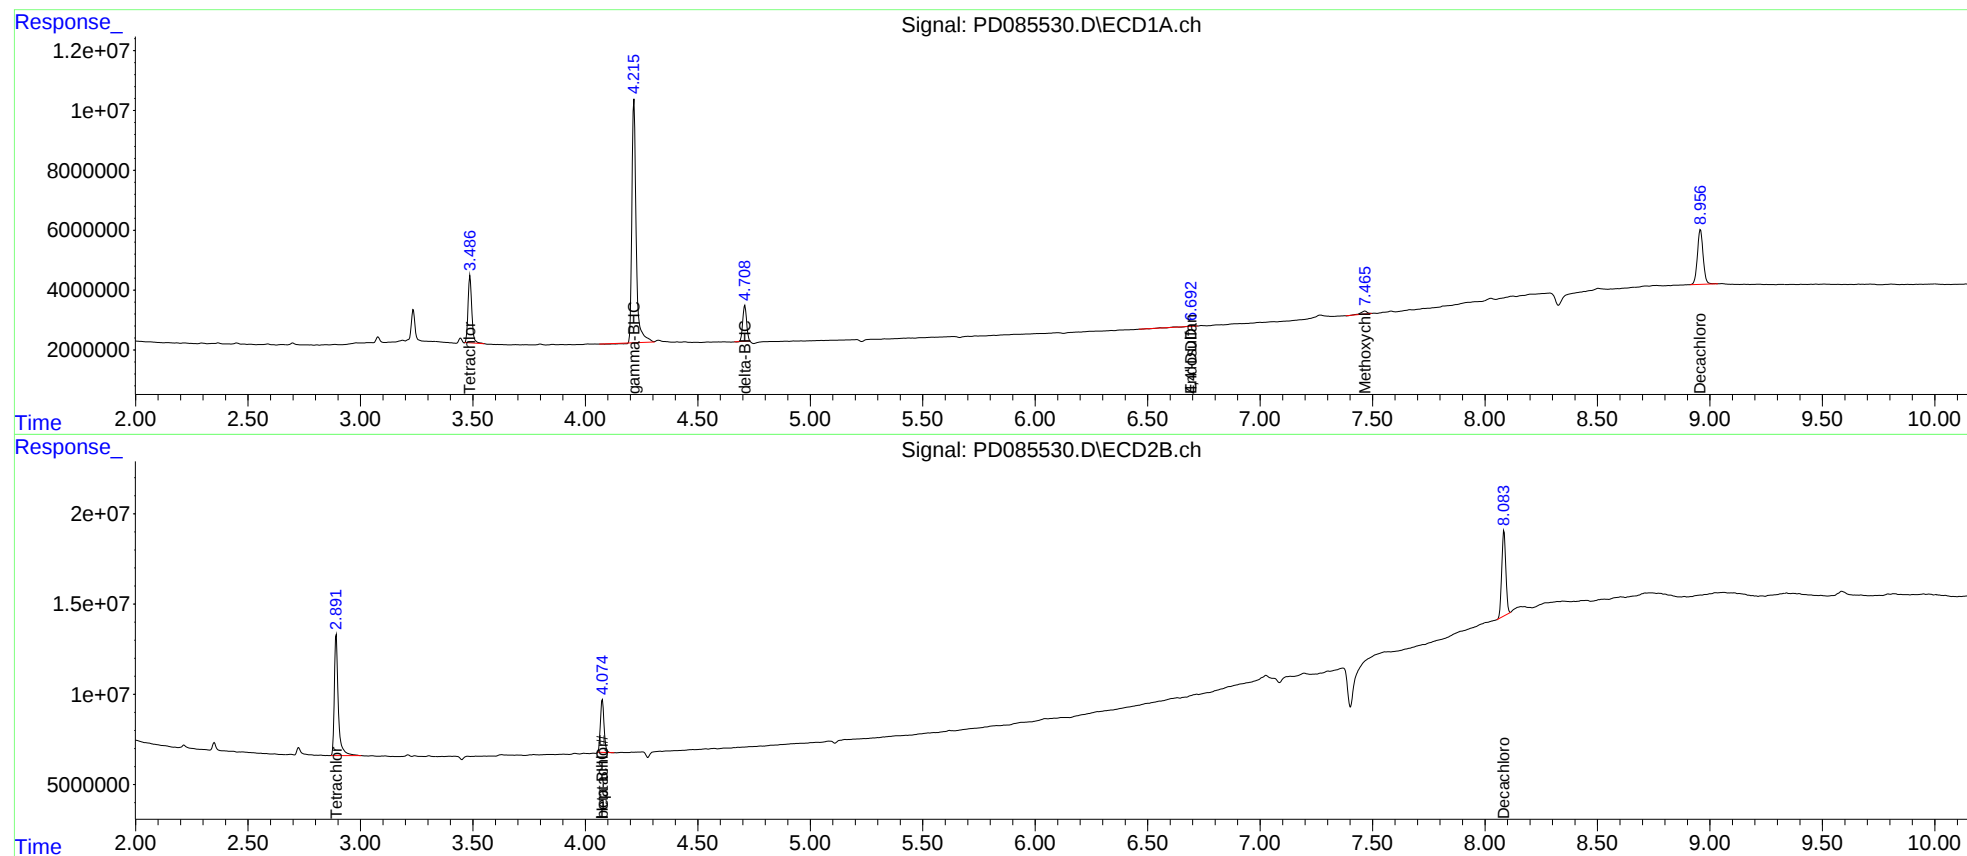

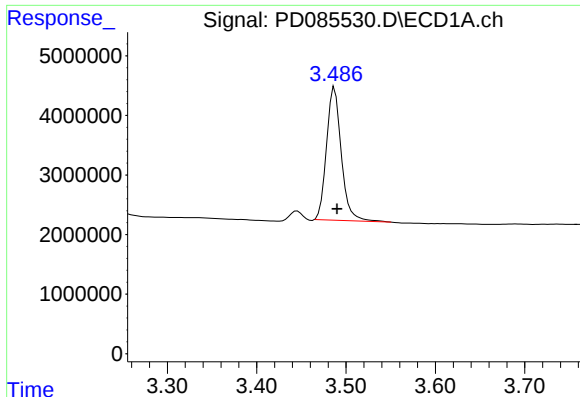


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.003 min
Response: 25590250
Conc: 21.13 ng/ml

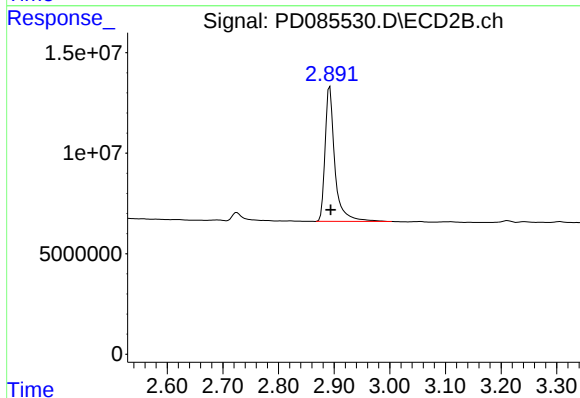


#1 Tetrachloro-m-xylene

R.T.: 2.892 min
Delta R.T.: -0.002 min
Response: 81796137
Conc: 21.64 ng/ml

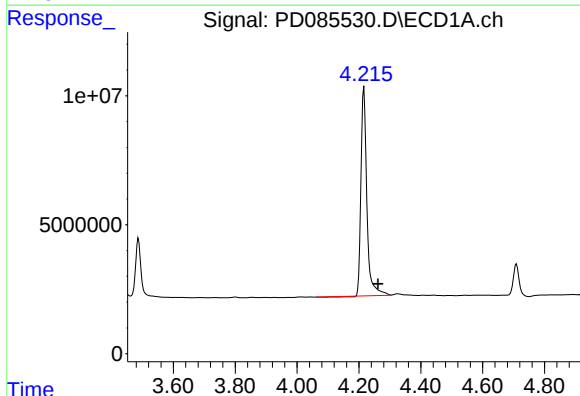


#3 gamma-BHC (Lindane)

R.T.: 4.216 min
Delta R.T.: -0.046 min
Response: 106755548
Conc: 42.67 ng/ml

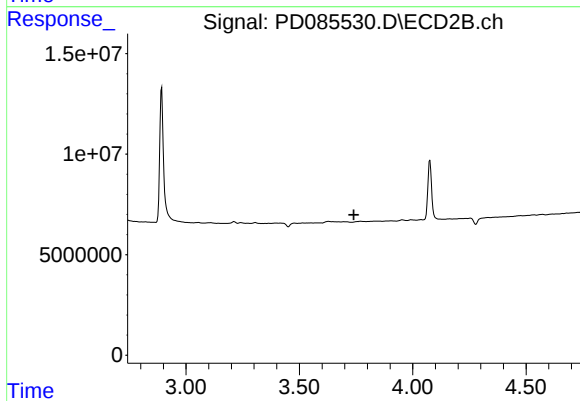


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.739 min
Response: 0
Conc: N.D.

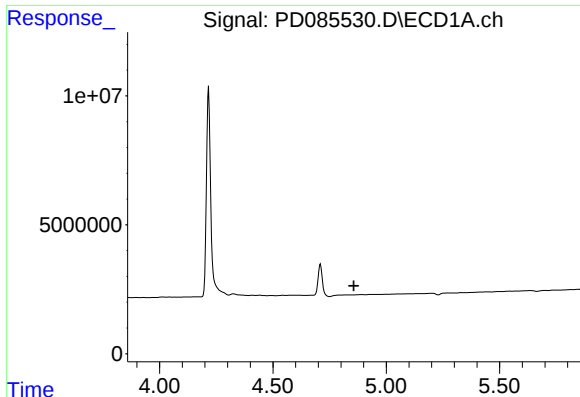


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

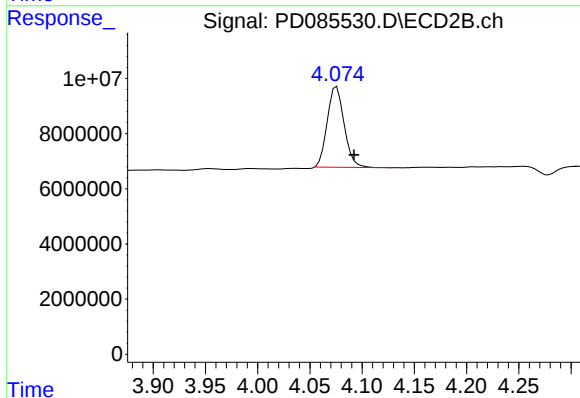


#4 Heptachlor

R.T.: 4.076 min
Delta R.T.: -0.017 min
Response: 32889965
Conc: 6.93 ng/ml

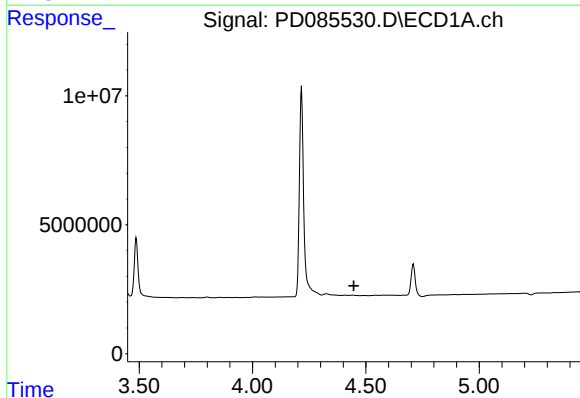


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.447 min
Response: 0
Conc: N.D.

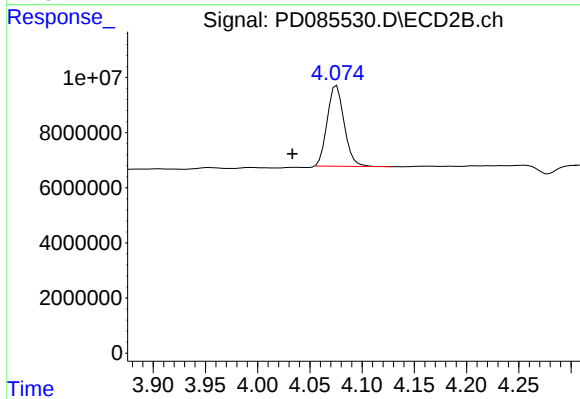


#6 beta-BHC

R.T.: 4.076 min
Delta R.T.: 0.042 min
Response: 32889965
Conc: 14.14 ng/ml

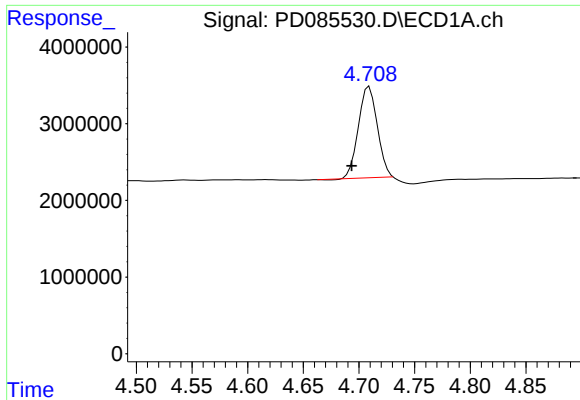


#7 delta-BHC

R.T.: 4.709 min
Delta R.T.: 0.016 min
Response: 14118482
Conc: 6.19 ng/ml

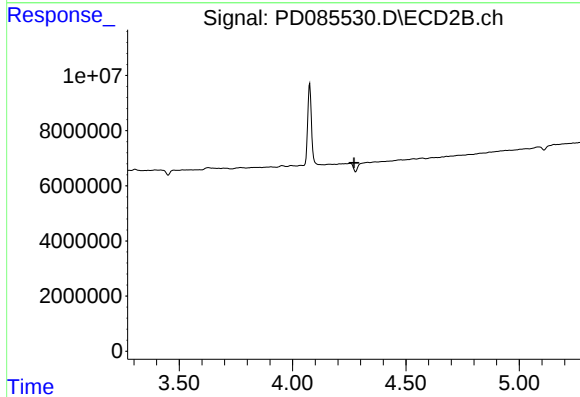


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.271 min
Response: 0
Conc: N.D.

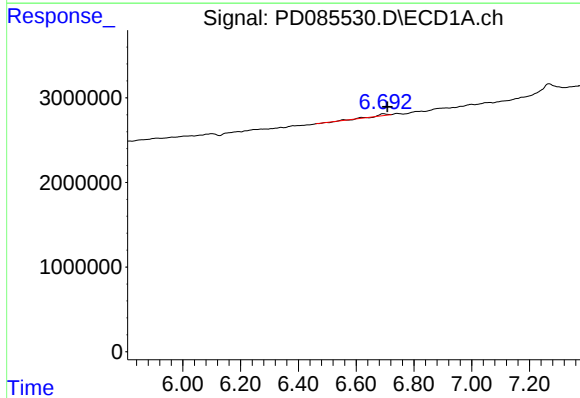


#15 Endosulfan II

R.T.: 6.694 min
Delta R.T.: -0.014 min
Response: 349852
Conc: 0.19 ng/ml

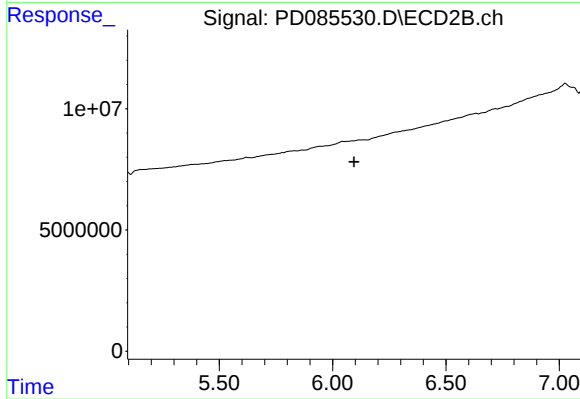


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

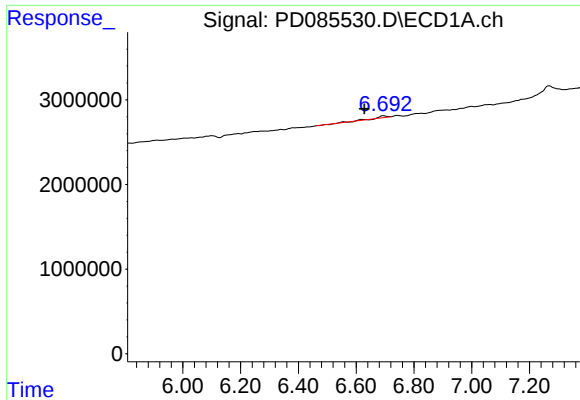


#16 4,4'-DDD

R.T.: 6.694 min
Delta R.T.: 0.065 min
Response: 349852
Conc: 0.27 ng/ml

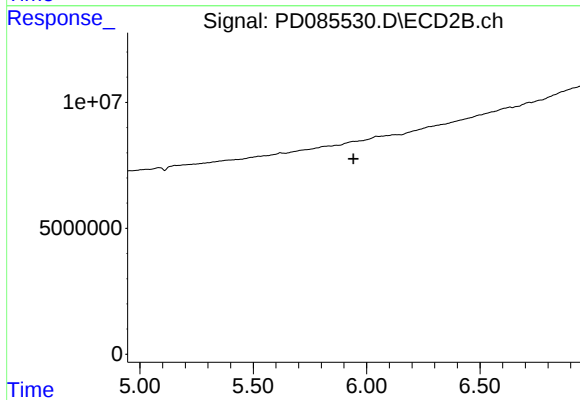


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.942 min
Response: 0
Conc: N.D.

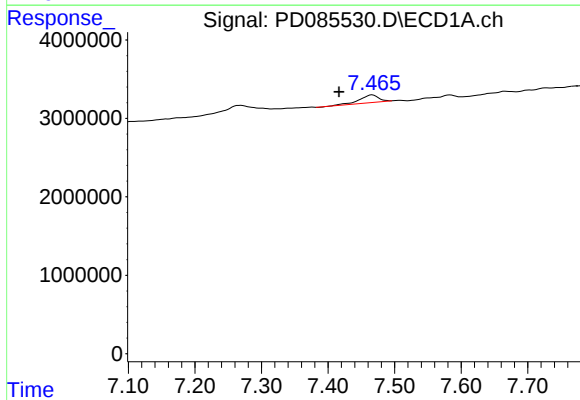


#20 Methoxychlor

R.T.: 7.466 min
Delta R.T.: 0.050 min
Response: 1904111
Conc: 2.60 ng/ml

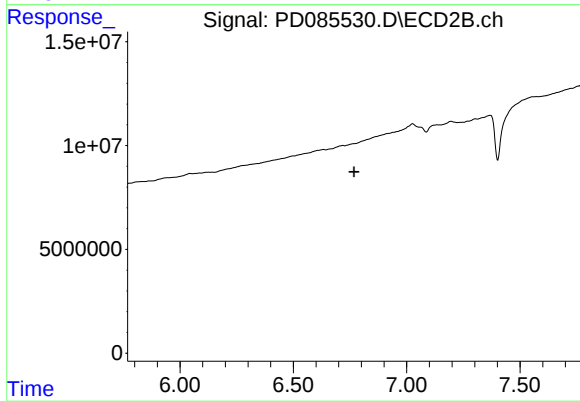


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

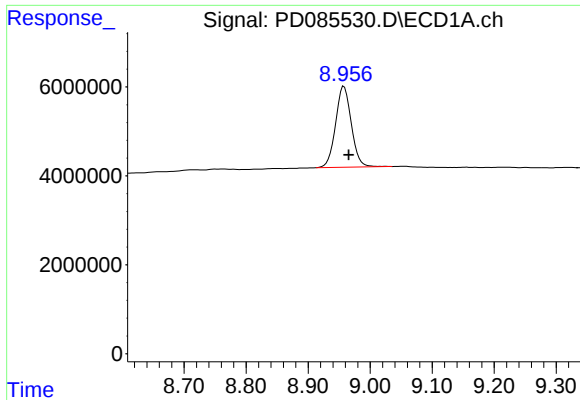

#27 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.008 min
Response: 32231949
Conc: 19.65 ng/ml

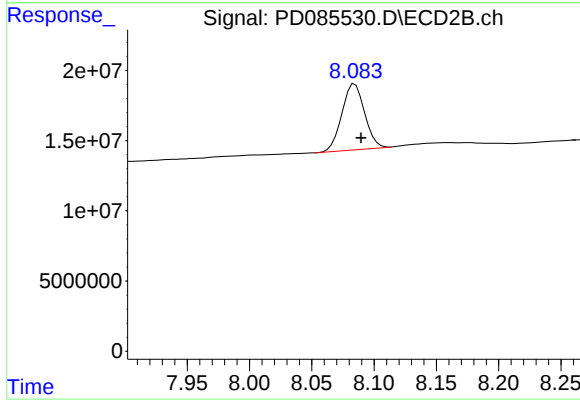

#27 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.005 min
Response: 59734436
Conc: 22.34 ng/ml