

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 17:56
 Operator : AR\AJ
 Sample : PIBLK152
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:38:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.488	2.906	24091397	83051304	19.894	21.972
27)	SA Decachlor...	8.959	8.098	42777596	75658298	26.077	28.301
Target Compounds							
3)	MA gamma-BHC...	4.217f	0.000	214.3E6	0	85.676	N.D. #
7)	B delta-BHC	4.709	0.000	1339348	0	0.588	N.D. #
15)	B Endosulfa...	6.689	6.053f	16136204	12298688	8.801	3.324 #
16)	A 4,4'-DDD	6.689f	0.000	16136204	0	12.247	N.D. #
20)	A Methoxychlor	7.466f	0.000	1719704	0	2.350	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 17:56
Operator : AR\AJ
Sample : PIBLK152
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:38:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

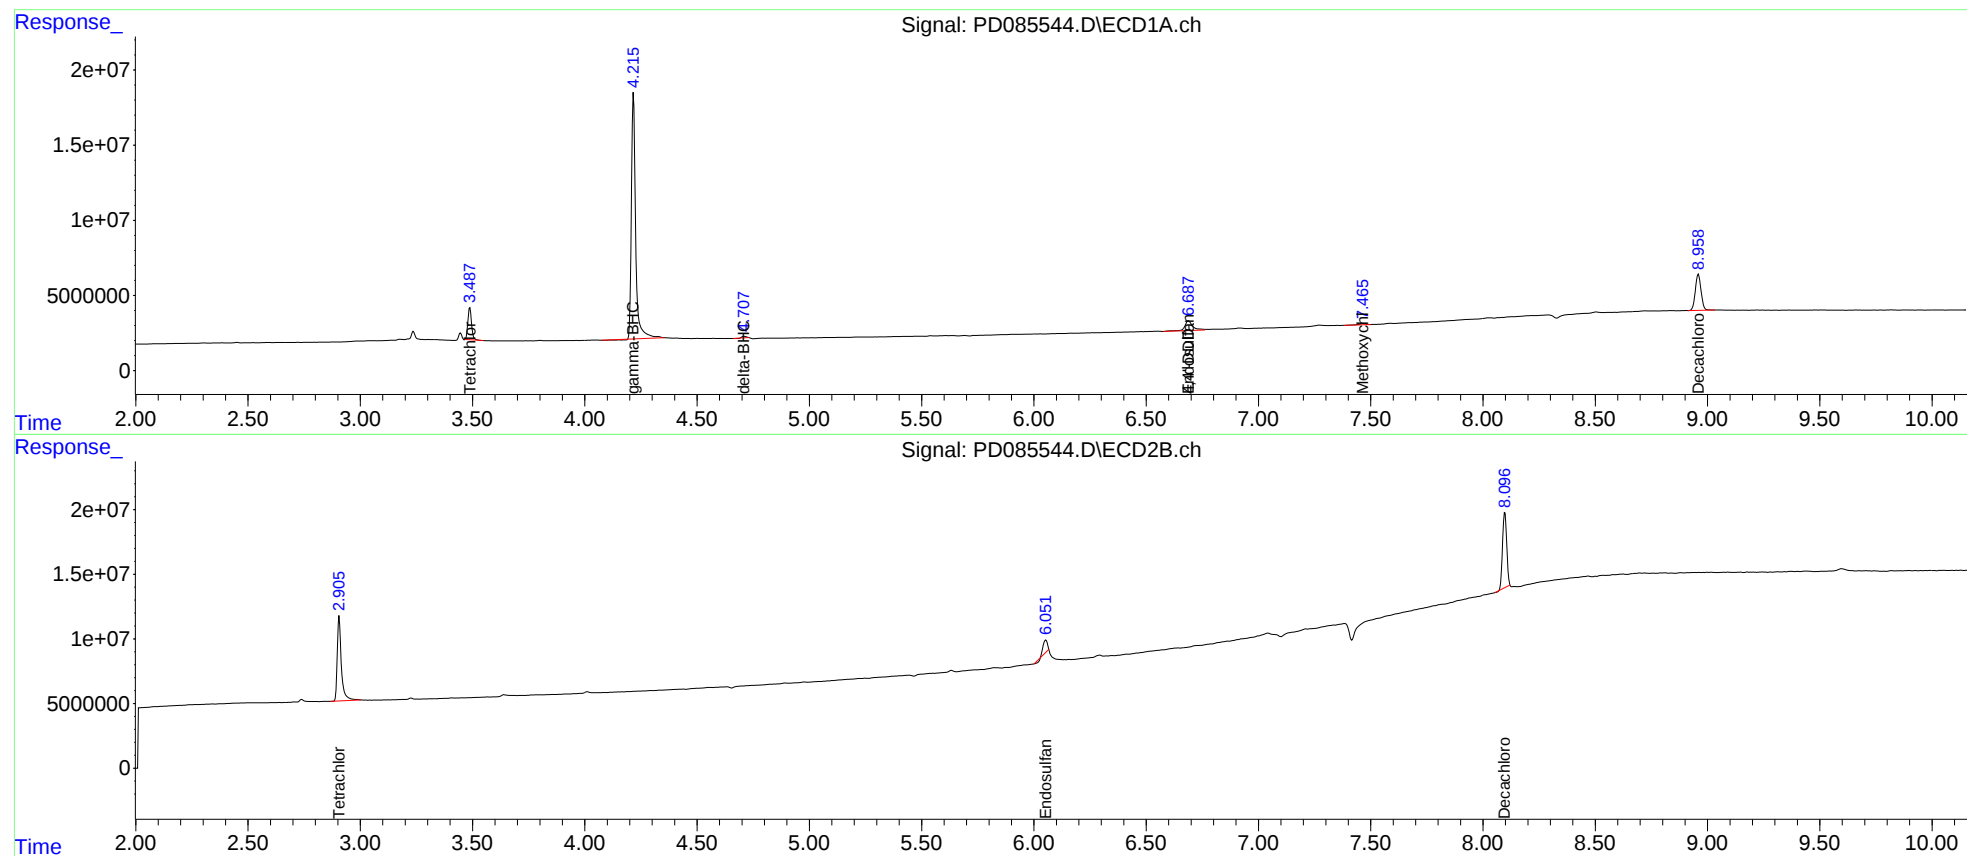

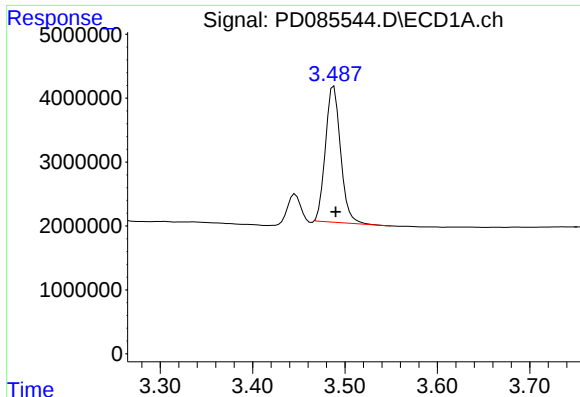


#1 Tetrachloro-m-xylene

R.T.: 3.488 min
Delta R.T.: -0.002 min
Response: 24091397
Conc: 19.89 ng/ml

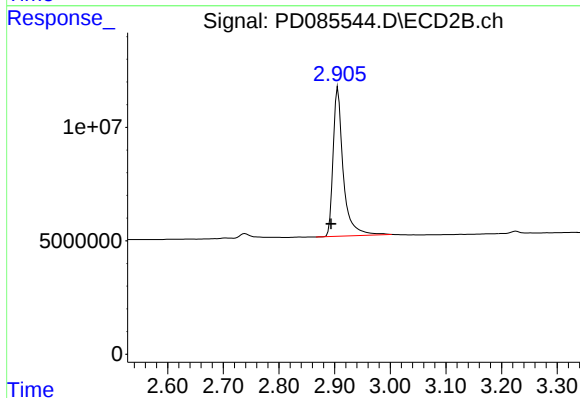


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.012 min
Response: 83051304
Conc: 21.97 ng/ml

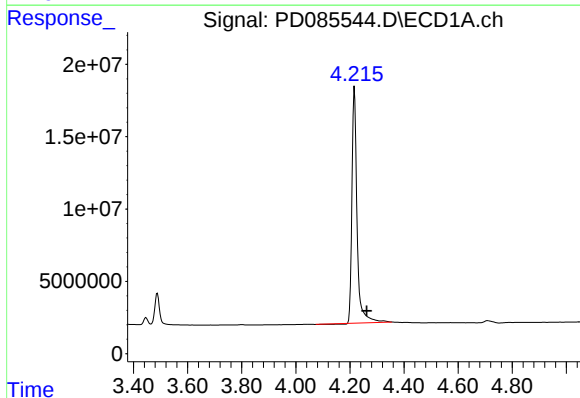


#3 gamma-BHC (Lindane)

R.T.: 4.217 min
Delta R.T.: -0.046 min
Response: 214346302
Conc: 85.68 ng/ml

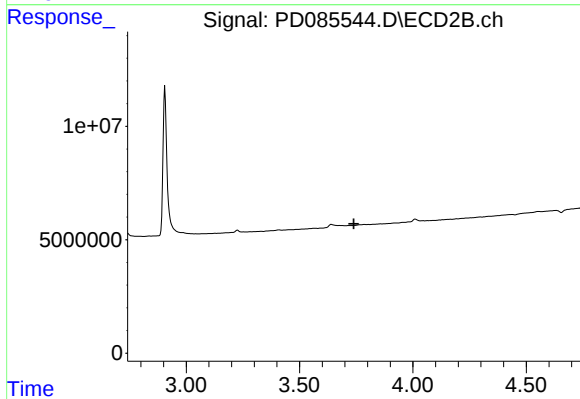


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.739 min
Response: 0
Conc: N.D.

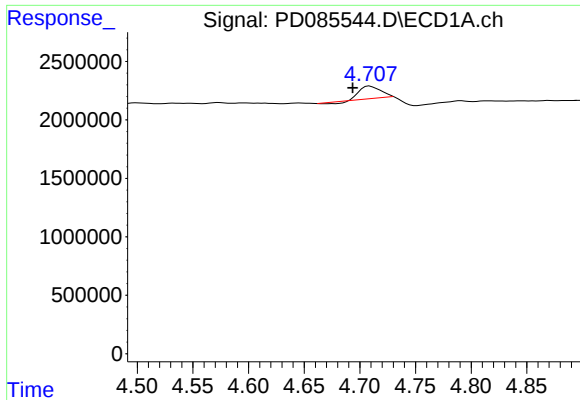


#7 delta-BHC

R.T.: 4.709 min
Delta R.T.: 0.016 min
Response: 1339348
Conc: 0.59 ng/ml

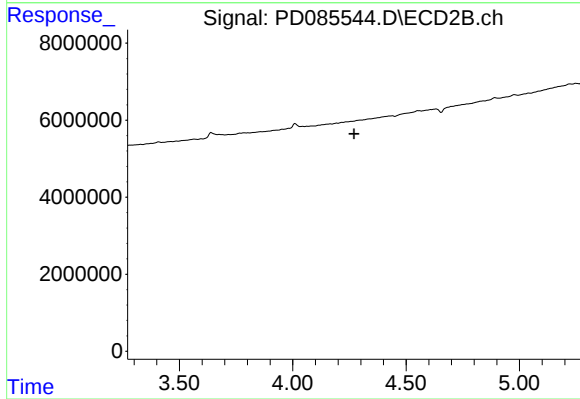


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.271 min
Response: 0
Conc: N.D.

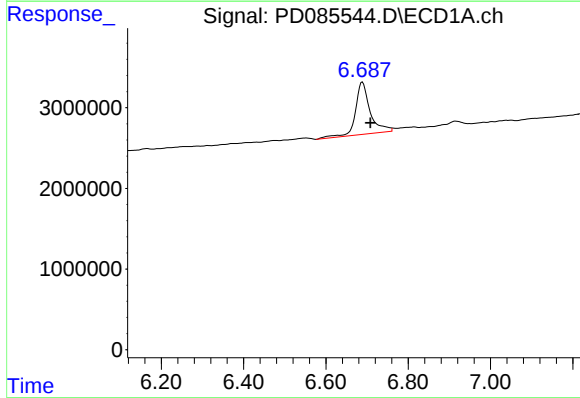


#15 Endosulfan II

R.T.: 6.689 min
Delta R.T.: -0.020 min
Response: 16136204
Conc: 8.80 ng/ml

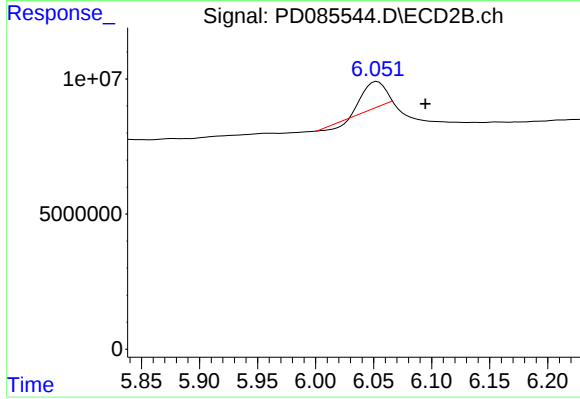


#15 Endosulfan II

R.T.: 6.053 min
Delta R.T.: -0.042 min
Response: 12298688
Conc: 3.32 ng/ml

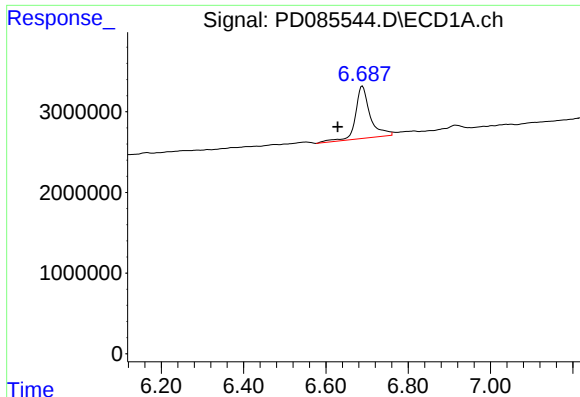


#16 4,4'-DDD

R.T.: 6.689 min
Delta R.T.: 0.060 min
Response: 16136204
Conc: 12.25 ng/ml

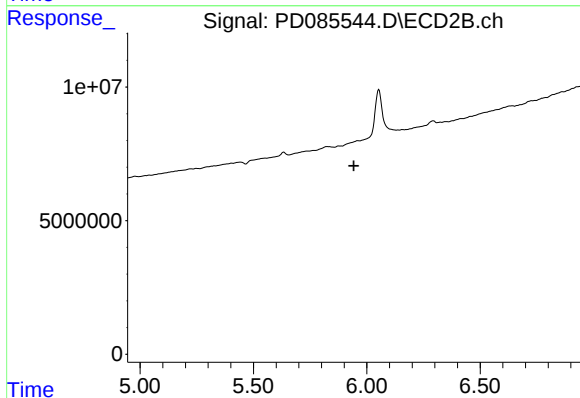


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.942 min
Response: 0
Conc: N.D.

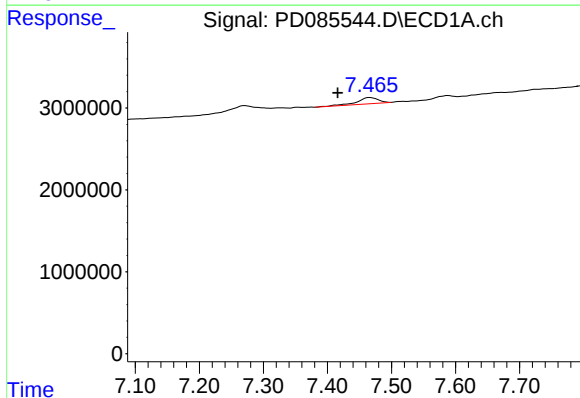


#20 Methoxychlor

R.T.: 7.466 min
Delta R.T.: 0.050 min
Response: 1719704
Conc: 2.35 ng/ml

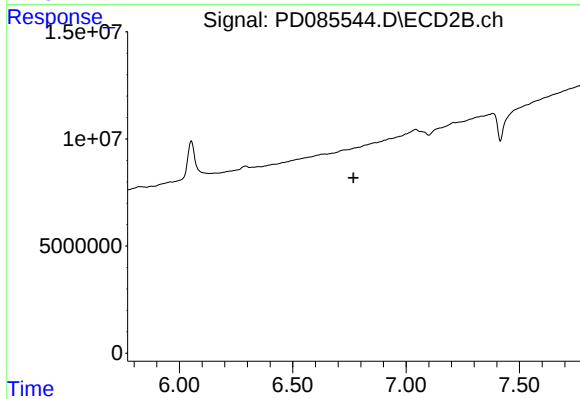


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

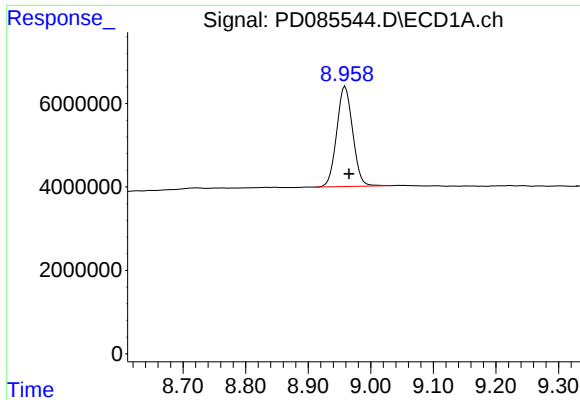

#27 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.006 min
Response: 42777596
Conc: 26.08 ng/ml

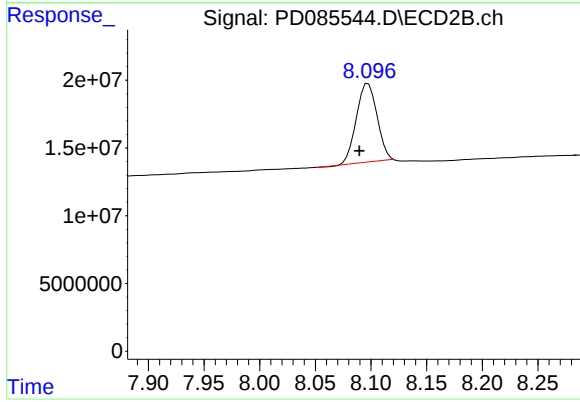

#27 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: 0.008 min
Response: 75658298
Conc: 28.30 ng/ml