

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 20:28
 Operator : AR\AJ
 Sample : P4017-05RE
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC44RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/25/2024
 Supervised By : Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:41:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.488	2.893	14205996	60165804	11.731	15.917m#
2) SA Decachlor...	8.959	8.083	32191179	41396801	19.623m	15.485m
Target Compounds						
2) A alpha-BHC	3.931	3.402	17755644	35096748	7.515	6.356
7) B delta-BHC	4.708	4.267	285.7E6	49945913	125.319m	9.482m#
8) B Heptachlo...	5.614	4.873	8998030	35609419	4.505m	7.671m#
16) A 4,4'-DDD	6.623	5.938	15088582	15952445	11.452m	4.764m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 20:28
Operator : AR\AJ
Sample : P4017-05RE
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:41:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

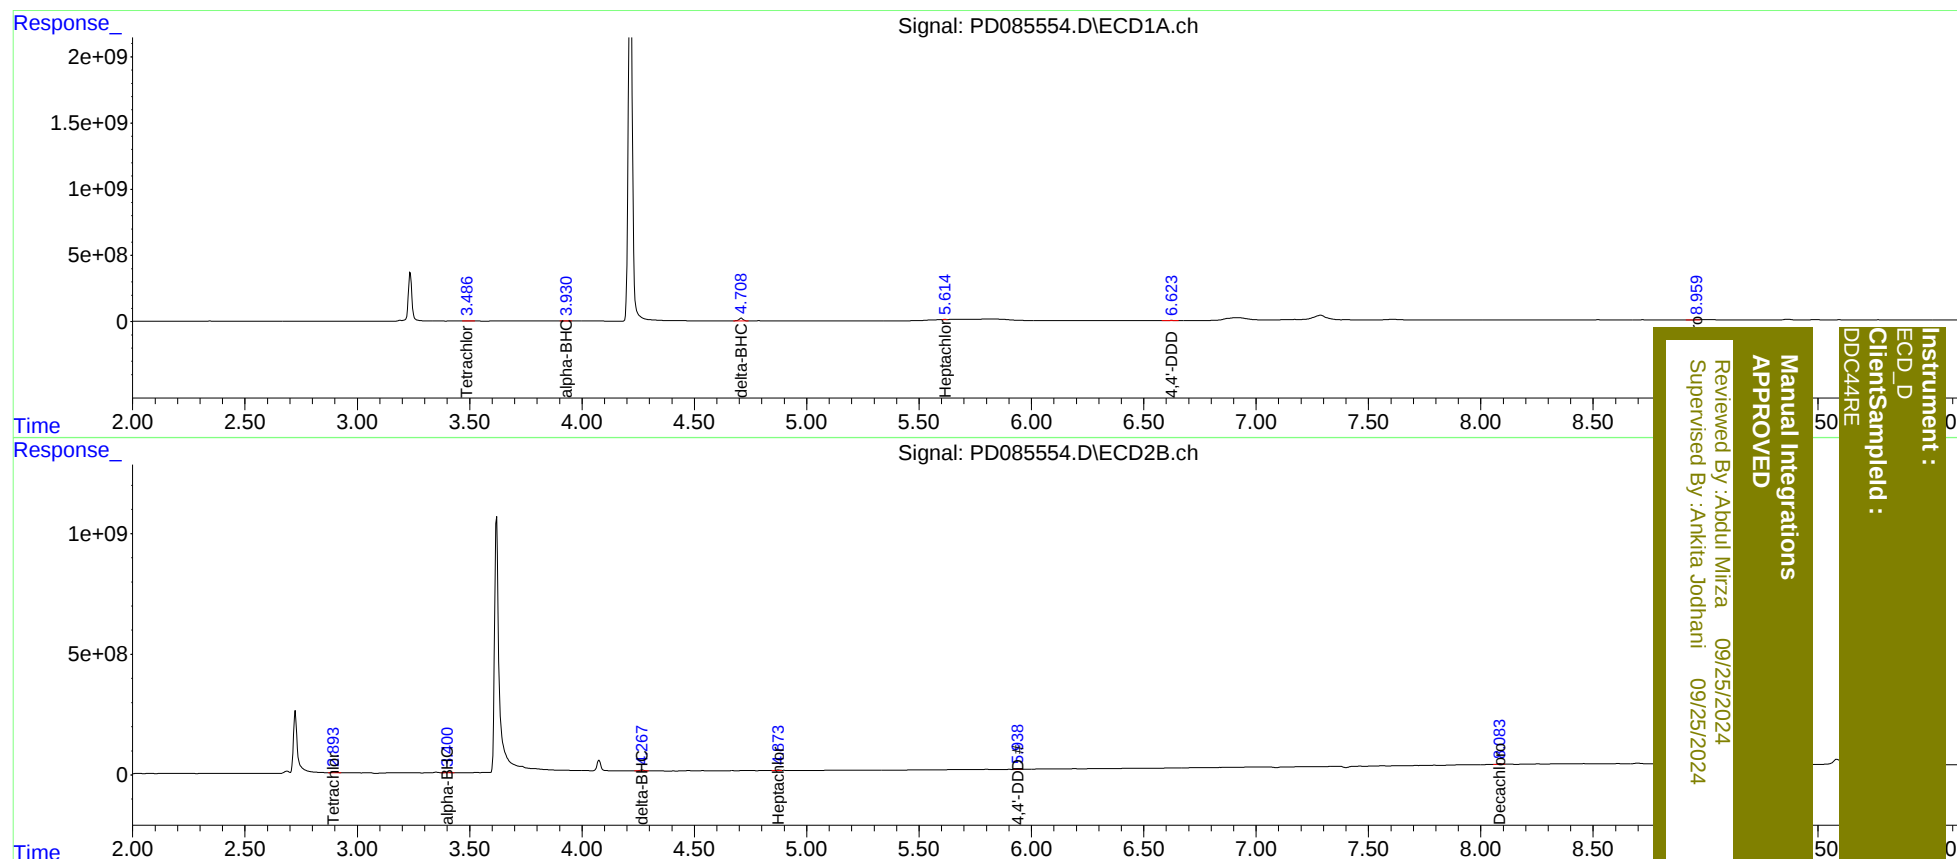

Instrument :
ECD_D
ClientSampled :
DDC4ARE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/25/2024
Supervised By :Ankita Jodhani 09/25/2024