

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 04:04
 Operator : AR\AJ
 Sample : P4018-17MS
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCE2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2024
 Supervised By : Ankita Jodhani 10/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 05:16:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	2.903	19538081	876.8E6	16.134m	231.976m#
27)	SA Decachlor...	8.962	8.084	47079012	57934037	28.699	21.671
Target Compounds							
2)	A alpha-BHC	3.932	3.402	123.5E6	255.6E6	52.267	46.286
3)	MA gamma-BHC...	4.201f	3.728	60440.7E6	178.4E6	24158.562m	34.233m#
4)	MA Heptachlor	4.854	4.079	115.7E6	521.5E6	54.798	109.867 #
5)	MB Aldrin	5.193	4.375	117.9E6	226.4E6	54.321	44.656
6)	B beta-BHC	4.442	4.028	47148834	66791290	49.441m	28.721 #
7)	B delta-BHC	4.692	4.269	127.8E6	284.1E6	56.045	53.942
8)	B Heptachlo...	5.612	4.878	133.7E6	264.2E6	66.911	56.917
9)	A Endosulfan I	5.994	5.254	102.4E6	187.9E6	57.797	45.723
10)	B trans-Chl...	5.866	5.132	126.8E6	199.4E6	66.602	44.064 #
11)	B cis-Chlor...	5.947	5.197	102.0E6	218.1E6	50.903	47.006
12)	B 4,4'-DDE	6.117	5.381	207.1E6	408.7E6	118.495	95.392
13)	MA Dieldrin	6.266	5.521	233.6E6	428.0E6	120.811	91.953
14)	MA Endrin	6.492	5.796	191.5E6	390.5E6	119.110	94.154m
15)	B Endosulfa...	6.704	6.090	165.4E6	352.4E6	90.225	95.234
16)	A 4,4'-DDD	6.623	5.938	179.0E6	341.6E6	135.894m	101.991
17)	MA 4,4'-DDT	6.938	6.192	145.0E6	317.0E6	118.986m	100.080
18)	B Endrin al...	6.831	6.269	126.7E6	267.2E6	106.972m	96.645
19)	B Endosulfa...	7.066	6.493	164.2E6	337.3E6	108.761	98.198
20)	A Methoxychlor	7.412	6.764	368.6E6	705.0E6	503.770	434.378
21)	B Endrin ke...	7.545	7.004	198.1E6	406.1E6	123.936	87.435 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 04:04
Operator : AR\AJ
Sample : P4018-17MS
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 05:16:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

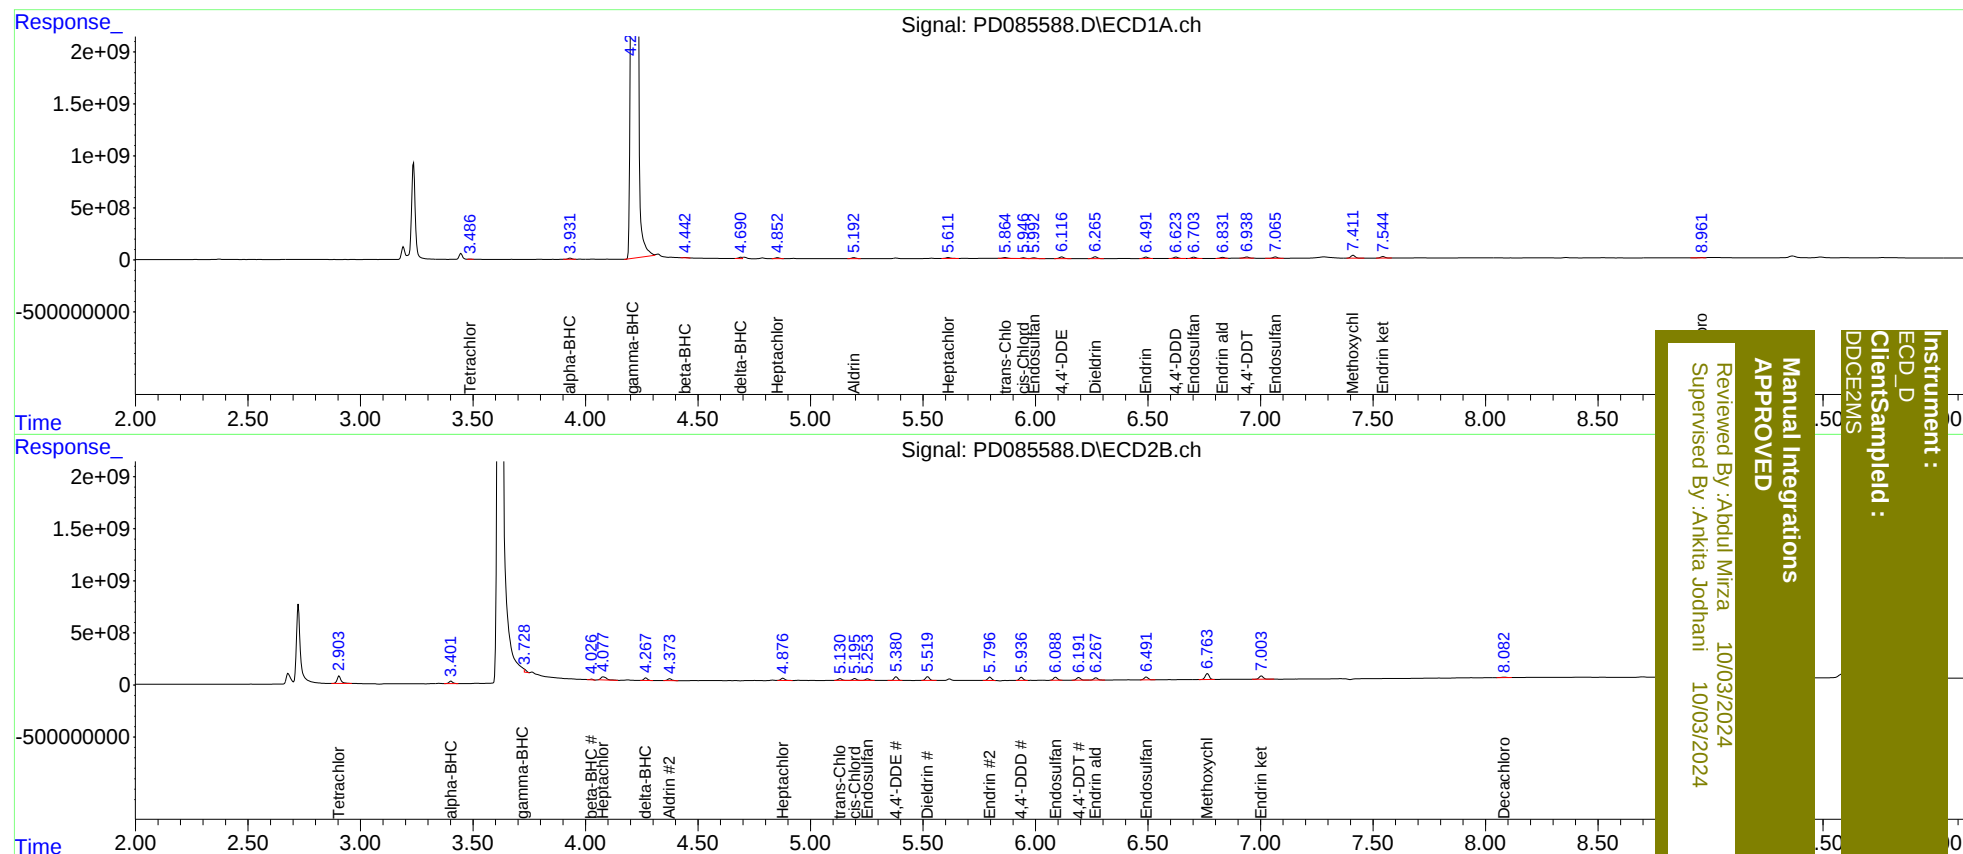

Reviewed By: Abdul Mirza 10/03/2024
Supervised By: Ankita Jodhani 10/03/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DCEZMS