

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 21:08
 Operator : AR\AJ
 Sample : P4017-08MS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC70MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/25/2024
 Supervised By :Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:42:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.481	2.905	30307841	387.6E6	25.028m	102.537m#
2) SA Decachlor...	8.956	8.082	26542451	32494805	16.180m	12.155m
Target Compounds						
2) A alpha-BHC	3.933	3.403	1726.8E6	2438.5E6	730.852	441.588 #
3) MA gamma-BHC...	4.200f	3.735	108568.1E6	1765.4E6	43395.400m	338.769m#
4) MA Heptachlor	4.854	4.085	166.2E6	163.5E6	78.690m	34.434m#
5) MB Aldrin	5.194	4.368	117.5E6	216.1E6	54.149m	42.637m
6) B beta-BHC	4.441	4.028	228.9E6	296.5E6	240.058m	127.501m#
7) B delta-BHC	4.691	4.269	2408.2E6	3231.1E6	1056.399	613.393 #
8) B Heptachlo...	5.612	4.875	102.9E6	806.6E6	51.530m	173.754m#
9) A Endosulfan I	5.993	5.255	190.5E6	172.9E6	107.490m	42.068m#
10) B trans-Chl...	5.845	5.132	548.4E6	224.6E6	288.129m	49.623m#
11) B cis-Chlor...	5.941	5.199	146.1E6	252.5E6	72.860m	54.427 #
12) B 4,4'-DDE	6.118	5.380	211.0E6	241.2E6	120.724	56.306m#
13) MA Dieldrin	6.265	5.521	320.4E6	329.2E6	165.731m	70.716 #
14) MA Endrin	6.491	5.798	152.6E6	431.5E6	94.909m	104.022m
15) B Endosulfa...	6.703	6.089	137.5E6	455.2E6	74.997m	123.024m#
16) A 4,4'-DDD	6.625	5.939	1493.7E6	2224.0E6	1133.676	664.098 #
17) MA 4,4'-DDT	6.933	6.191	670.0E6	539.3E6	549.643m	170.258m#
18) B Endrin al...	6.848	6.268	464.3E6	205.5E6	392.038m	74.306m#
19) B Endosulfa...	7.064	6.494	207.1E6	274.5E6	137.160m	79.925 #
20) A Methoxychlor	7.410	6.762	503.2E6	905.9E6	687.735m	558.214m
21) B Endrin ke...	7.544	7.003	81199851	353.2E6	50.790m	76.050m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 21:08
Operator : AR\AJ
Sample : P4017-08MS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:42:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

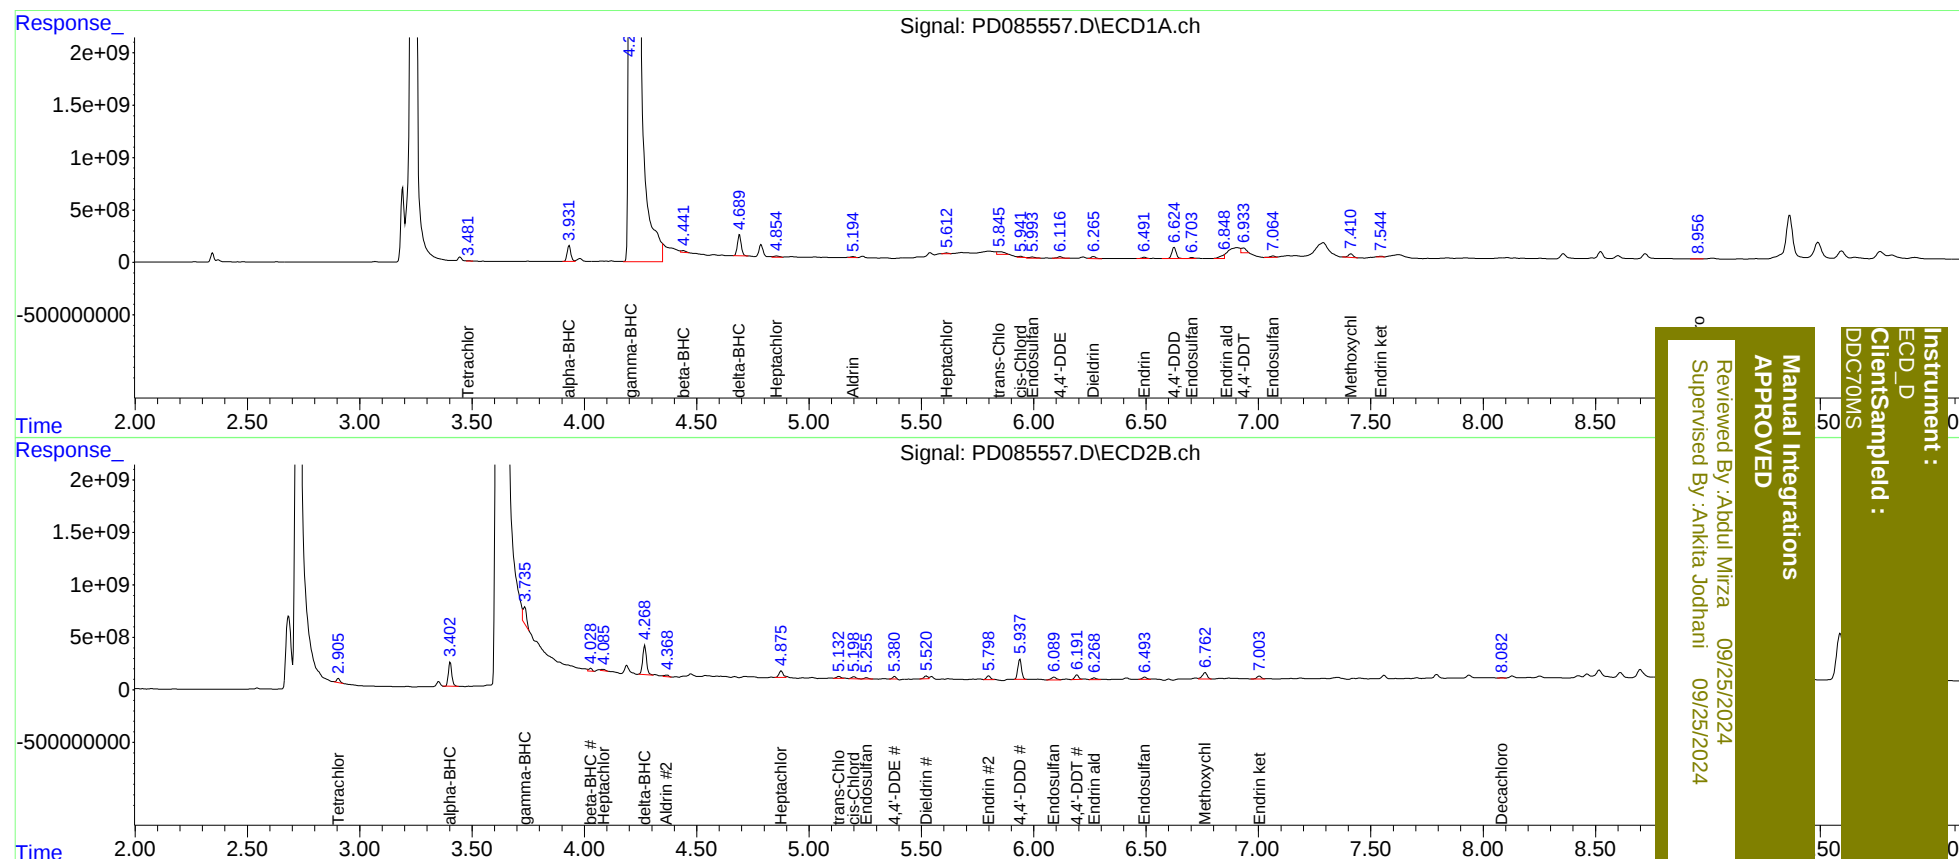

Reviewed By: Abdul Miza 09/25/2024
Supervised By: Ankita Jodhani 09/25/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC70MS