

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 21:35
 Operator : AR\AJ
 Sample : P4017-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC85

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/25/2024
 Supervised By : Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:42:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.485	2.904	27117282	1074.7E6	22.393m	284.316m#
27) SA Decachlor...	8.959	8.082	27894838	32982321	17.004m	12.338m#
Target Compounds						
2) A alpha-BHC	3.932	3.403	104.9E6	161.5E6	44.415	29.255 #
7) B delta-BHC	4.689	4.267	200.7E6	367.6E6	88.037m	69.778m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 21:35
Operator : AR\AJ
Sample : P4017-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:42:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

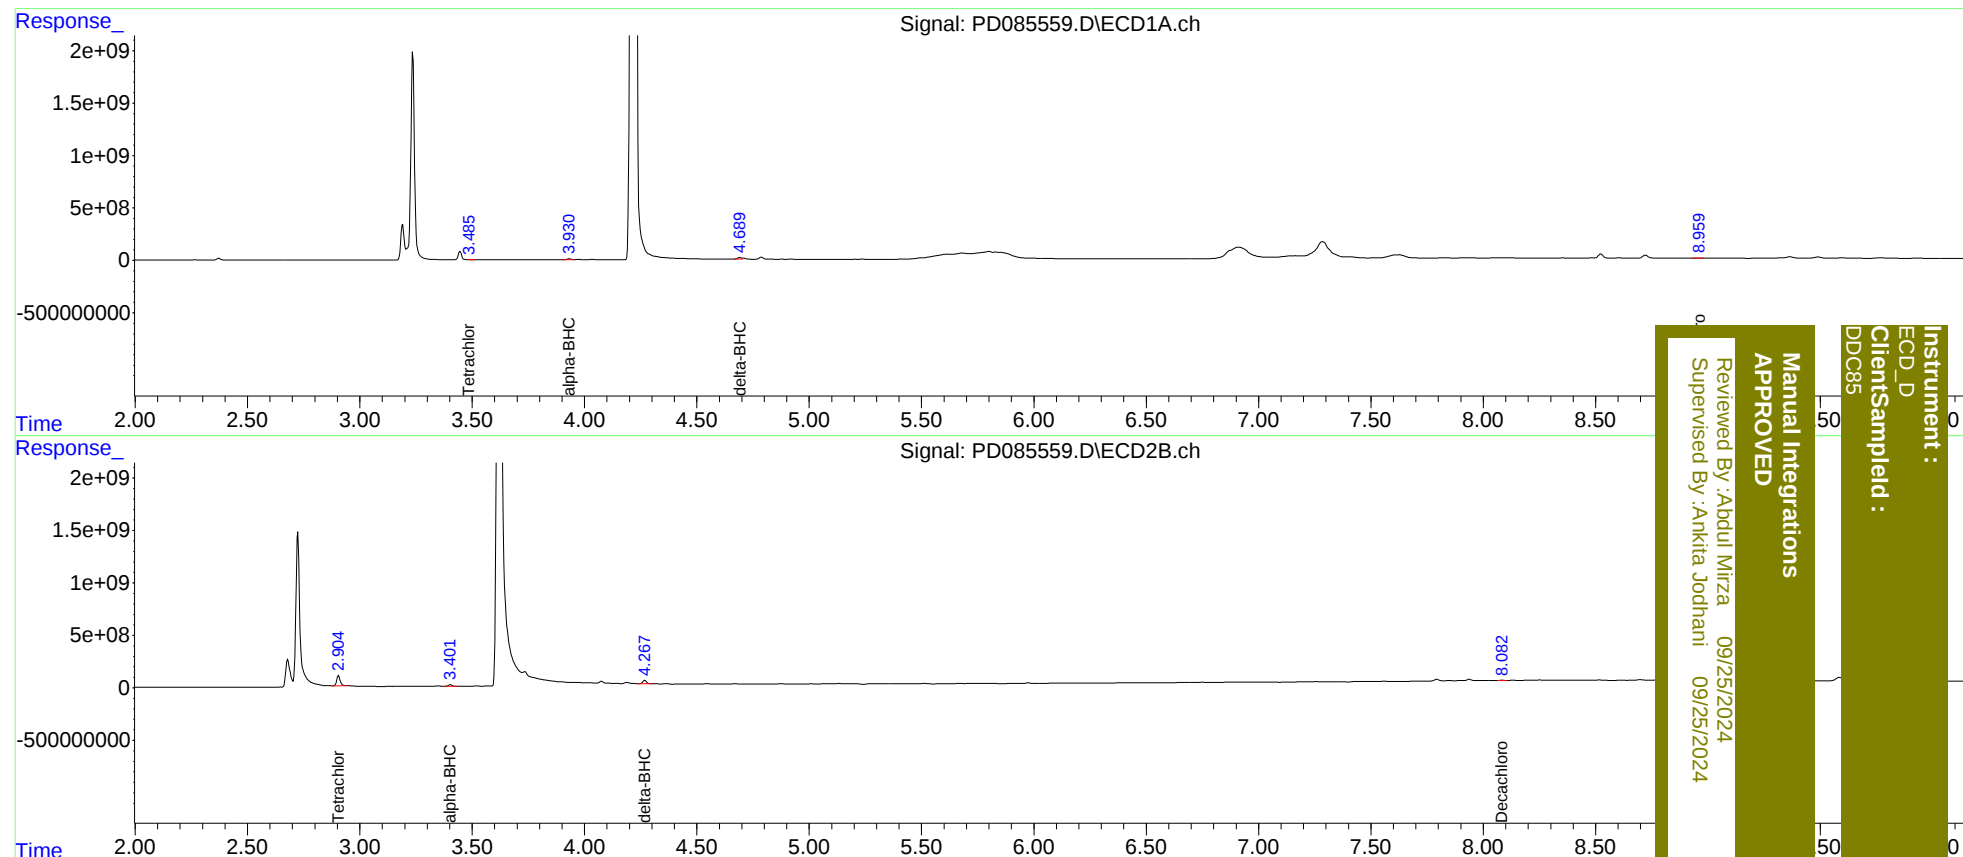

Reviewed By: Abdul Mirza 09/25/2024
Supervised By: Ankita Jodhani 09/25/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDC85