

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
 Data File : PD085575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 01:09
 Operator : AR\AJ
 Sample : P4018-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCA2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/03/2024
 Supervised By :Ankita Jodhani 10/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 05:11:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.489	2.903	21023784	128.7E6	17.361m	34.058m#
2) SA Decachlor...	8.961	8.083	20387420	8452865	12.428m	3.162 #
Target Compounds						
2) A alpha-BHC	3.931	3.401	32044915	138.8E6	13.563	25.141 #
7) B delta-BHC	4.707	4.271	195.9E6	116.3E6	85.944m	22.075 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092324\
Data File : PD085575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 01:09
Operator : AR\AJ
Sample : P4018-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 05:11:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

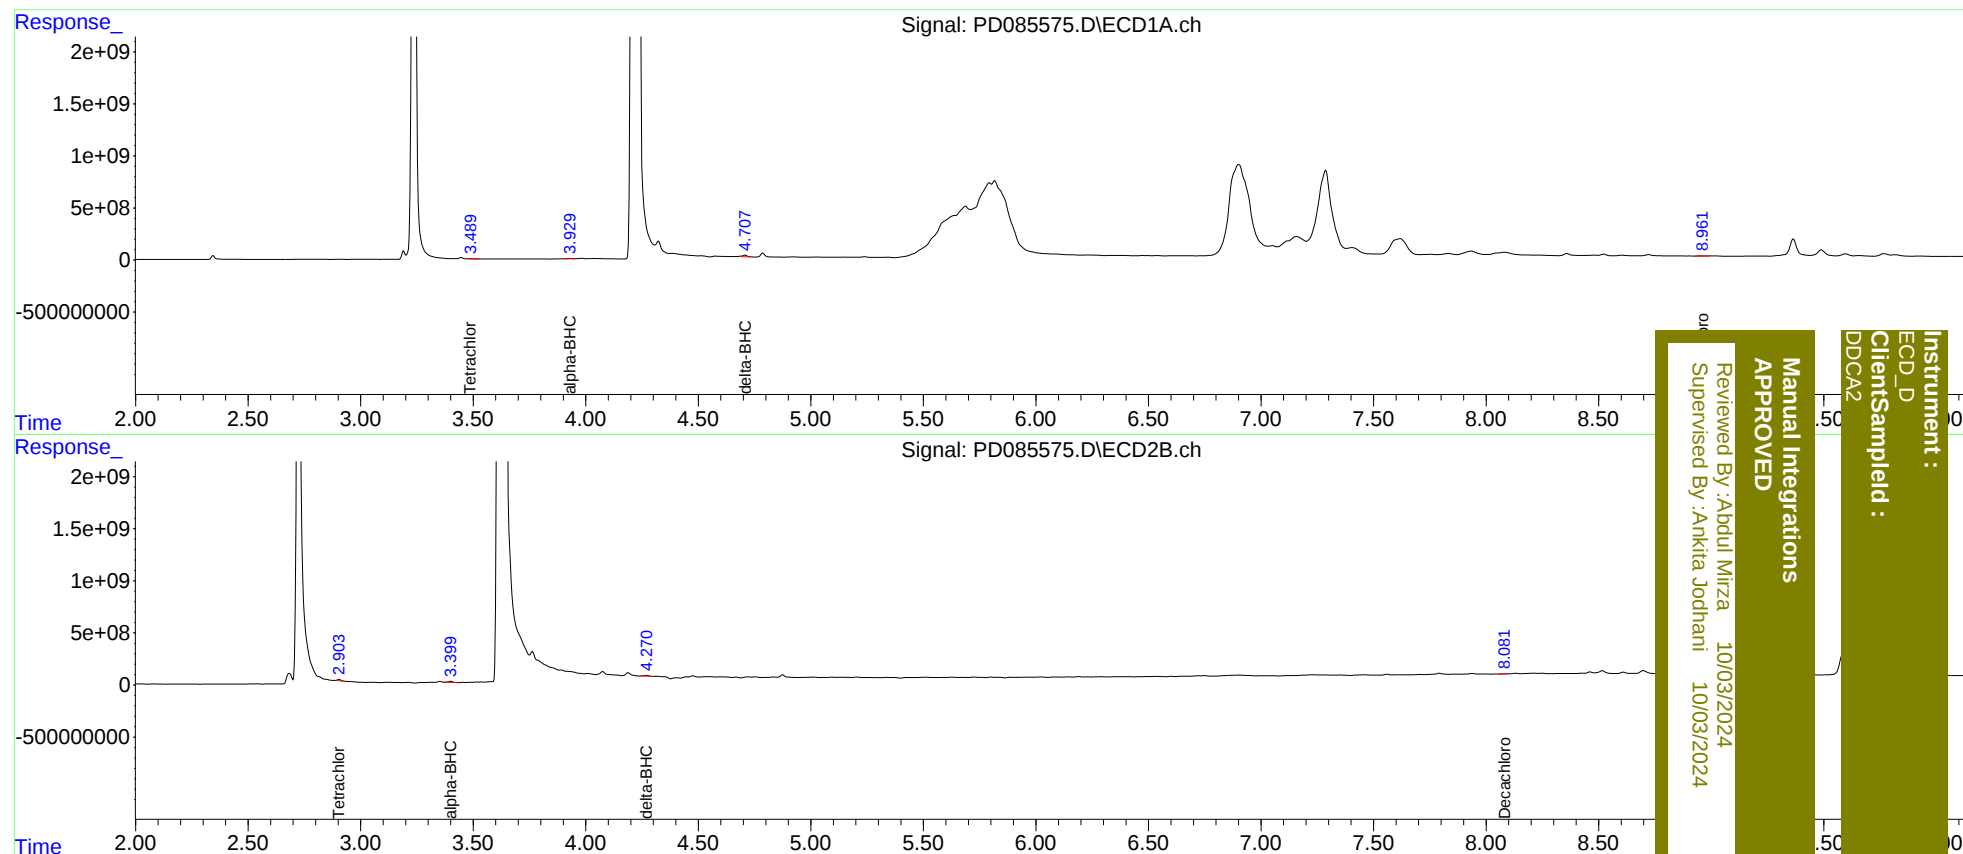

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/03/2024
Supervised By: Ankita Jodhani 10/03/2024

Instrument :
ECD_D
ClientSampled :
DDCA2