

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092419\
 Data File : PD054893.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2019 8:34
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 06:58:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	3.961f	0.000	1097480	0	1.024	N.D.	#
9) A	Endosulfan I	0.000	6.150	0	4949705	N.D.	3.923	
11) B	cis-Chlor...	0.000	6.150	0	4949705	N.D.	3.758	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092419\
Data File : PD054893.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 8:34
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 06:58:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

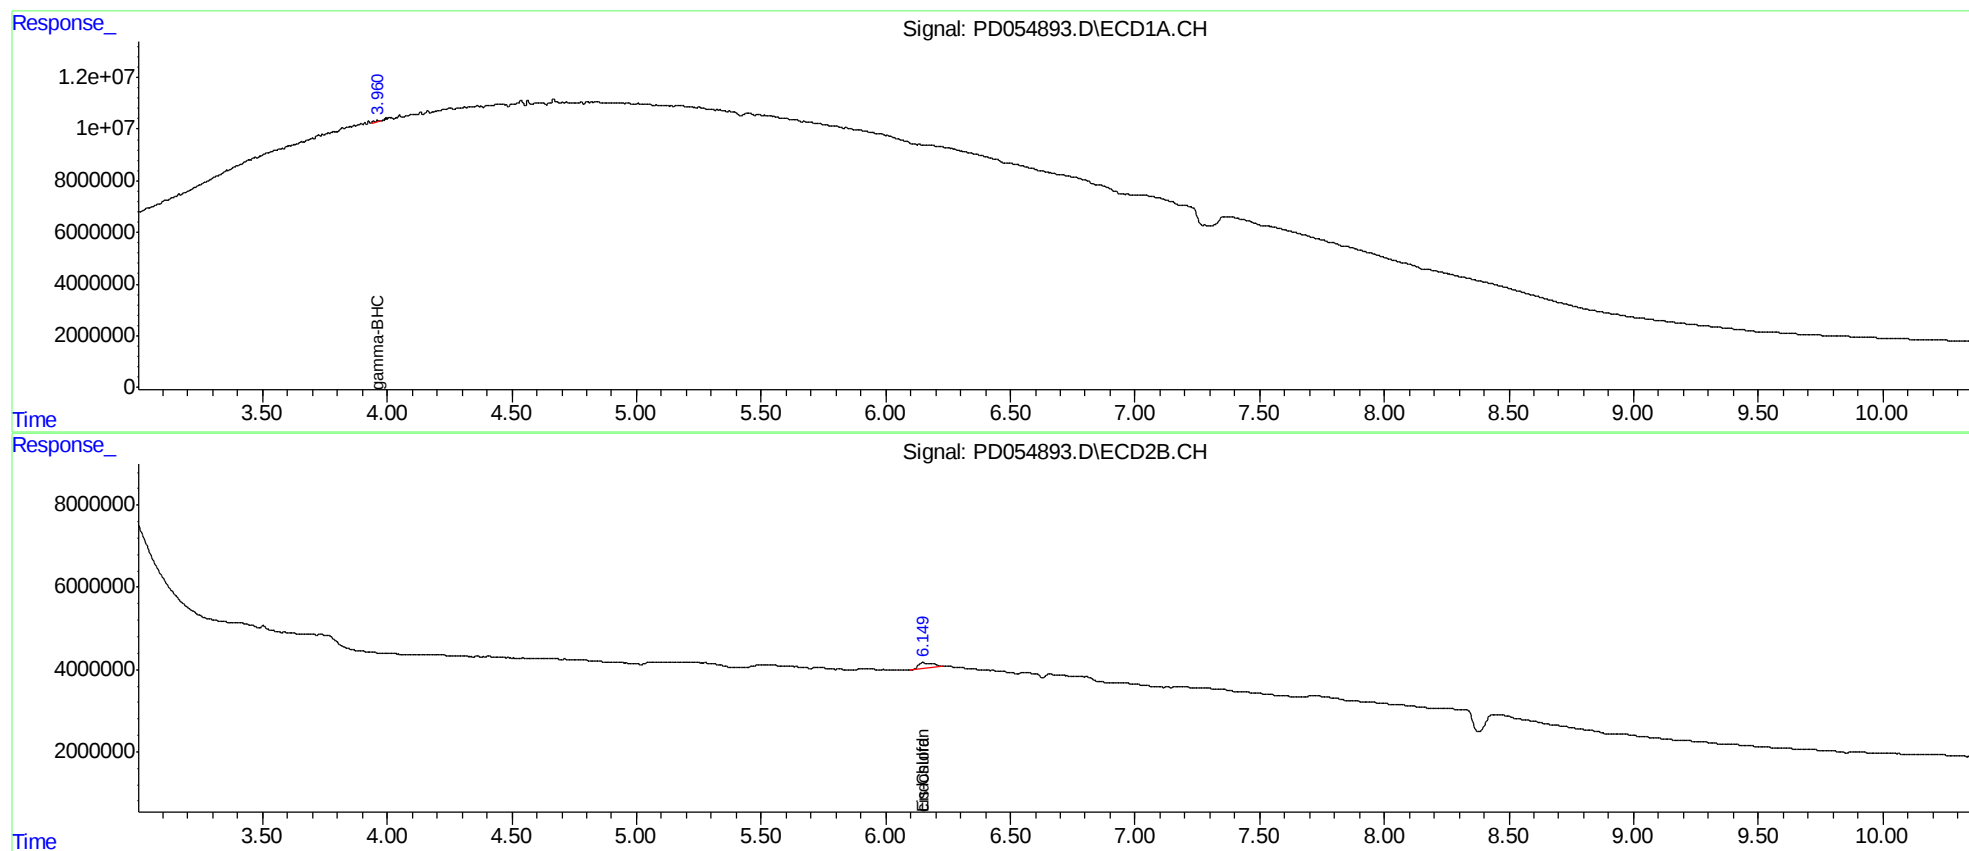


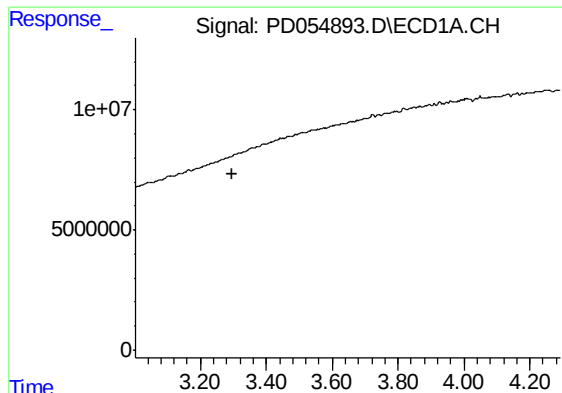

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

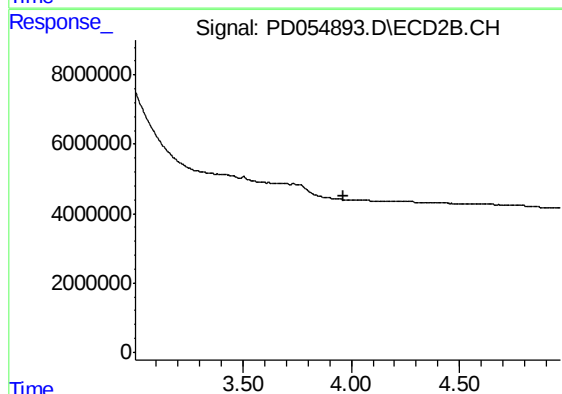


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

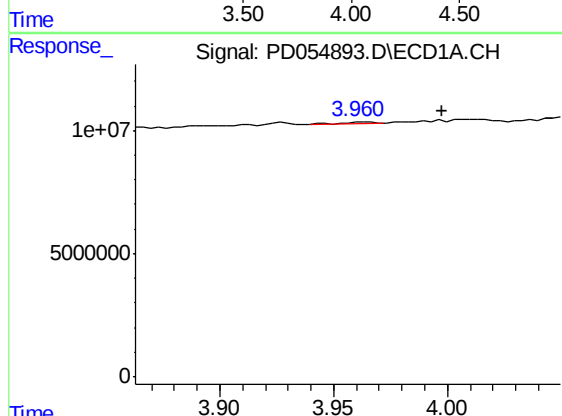


#3 gamma-BHC (Lindane)

R.T.: 3.961 min
Delta R.T.: -0.036 min
Response: 1097480
Conc: 1.02 ng/ml

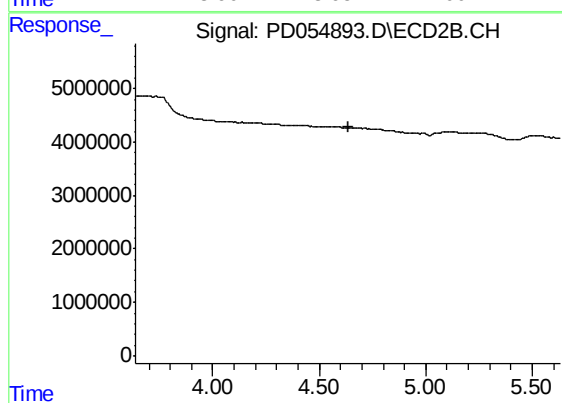

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.635 min
Response: 0
Conc: N.D.

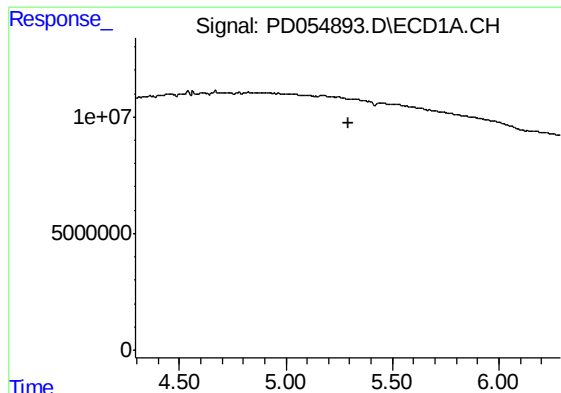

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

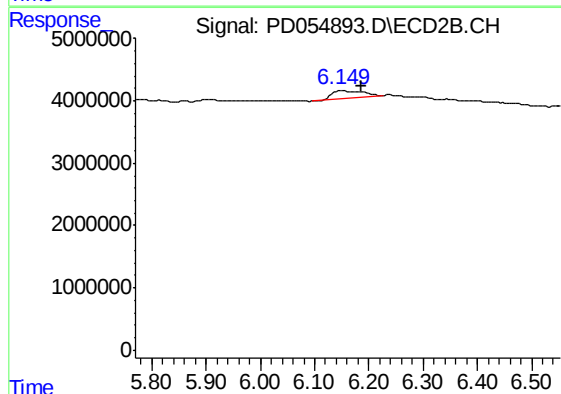


#9 Endosulfan I

R.T.: 6.150 min
Delta R.T.: -0.035 min
Response: 4949705
Conc: 3.92 ng/ml

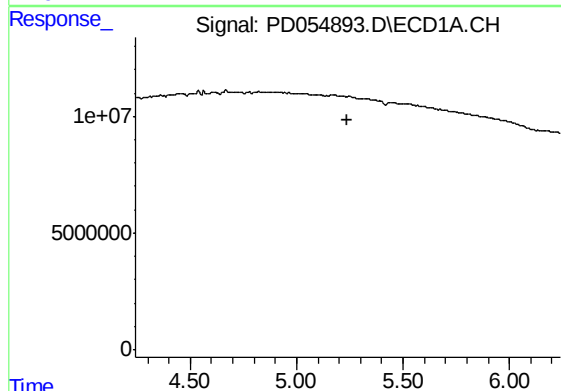


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.241 min
Response: 0
Conc: N.D.

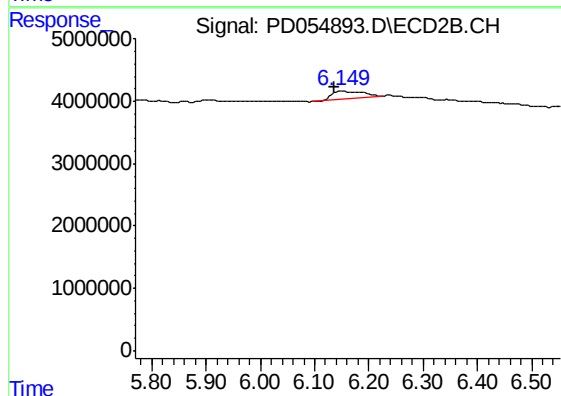

#11 cis-Chlordane


R.T.: 6.150 min
Delta R.T.: 0.014 min
Response: 4949705
Conc: 3.76 ng/ml

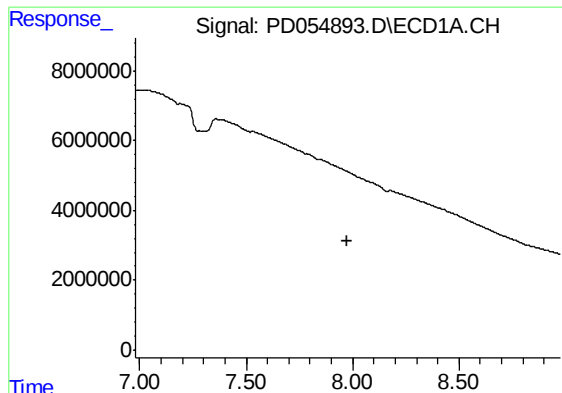

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.977 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

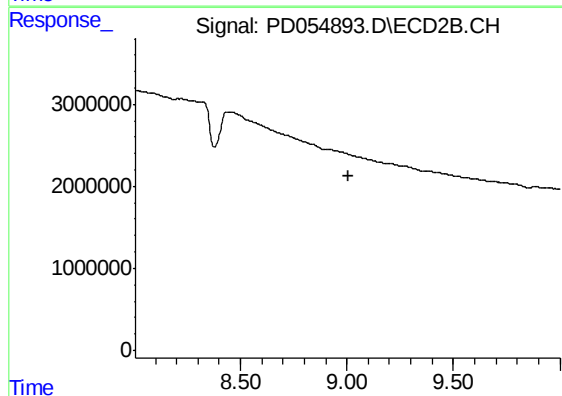

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.005 min
Response: 0
Conc: N.D.