

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092419\
 Data File : PD054900.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2019 10:41
 Operator : SG\AJ
 Sample : K4932-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFDG4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 07:00:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.295	3.966	15771484	20132832	20.731	19.619
27) SA	Decachlor...	7.976	9.003	30667785	42648751	36.397	36.606
Target Compounds							
3) MA	gamma-BHC...	4.004	4.616	2673398	1737062	2.493	1.241 #
8) B	Heptachlo...	5.027f	0.000	2489313	0	2.713	N.D. #
9) A	Endosulfan I	0.000	6.222f	0	1133838	N.D.	0.899
19) B	Endosulfa...	0.000	7.240	0	3329033	N.D.	2.803


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092419\
Data File : PD054900.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 10:41
Operator : SG\AJ
Sample : K4932-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFDG4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 07:00:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

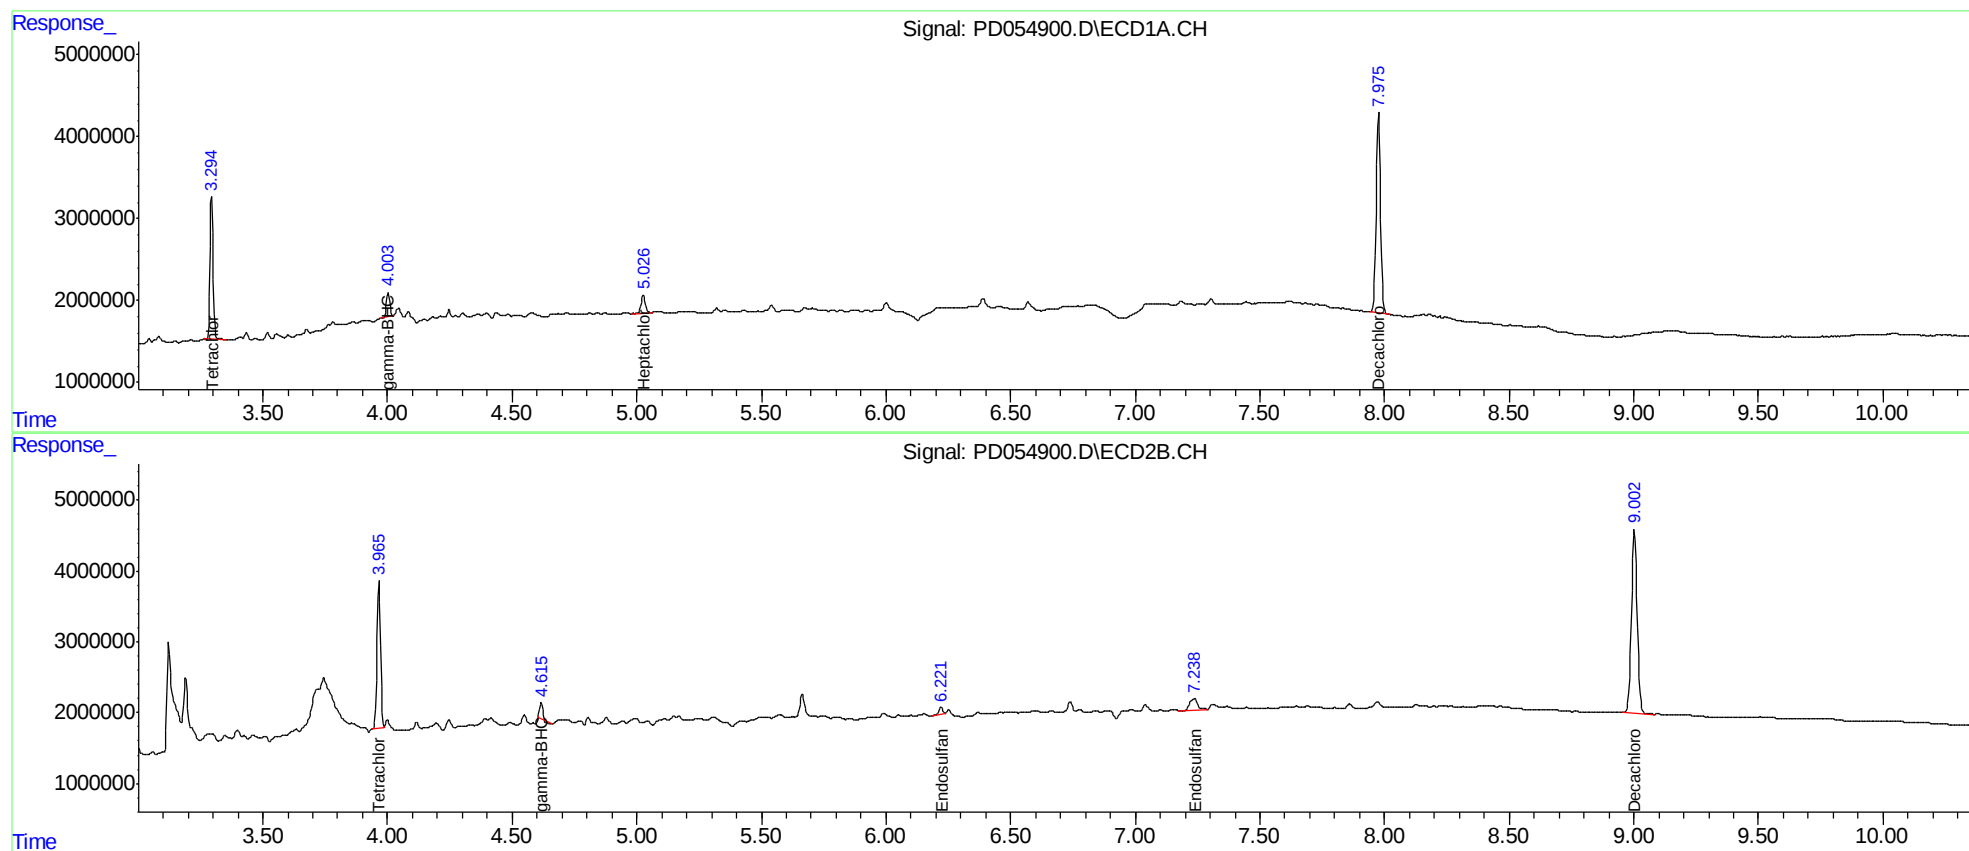


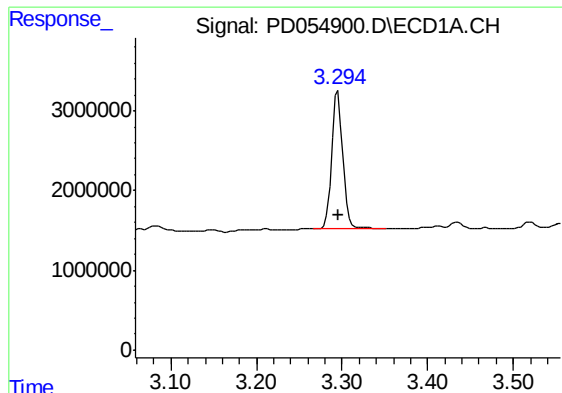

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 15771484
Conc: 20.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFDG4

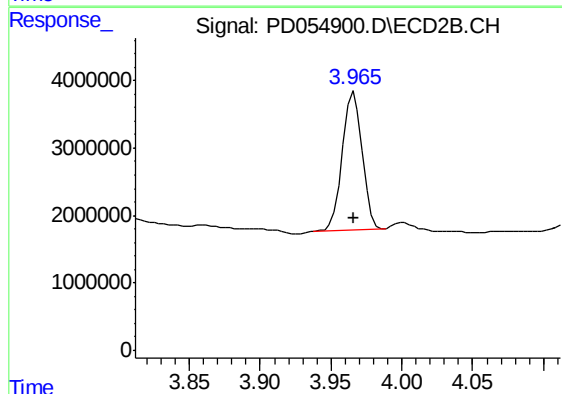


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 20132832
Conc: 19.62 ng/ml

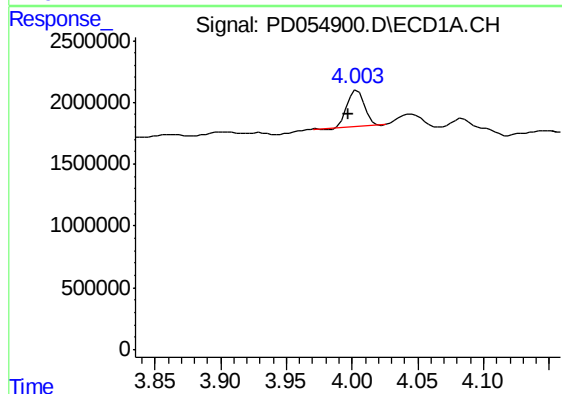


#3 gamma-BHC (Lindane)

R.T.: 4.004 min
Delta R.T.: 0.007 min
Response: 2673398
Conc: 2.49 ng/ml

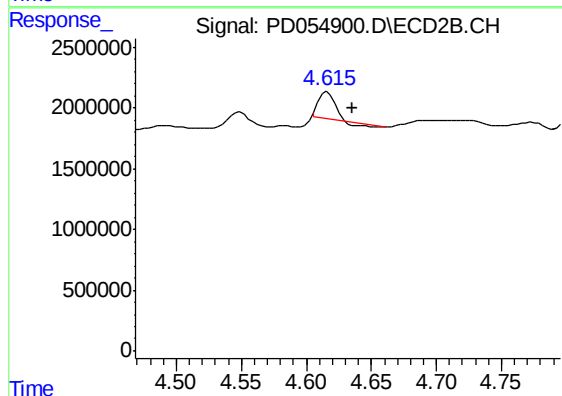

#3 gamma-BHC (Lindane)


R.T.: 4.616 min
Delta R.T.: -0.019 min
Response: 1737062
Conc: 1.24 ng/ml

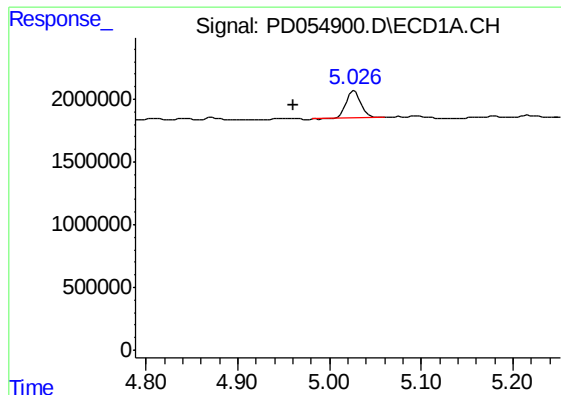

#8 Heptachlor epoxide


R.T.: 5.027 min
Delta R.T.: 0.066 min
Response: 2489313
Conc: 2.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFDG4

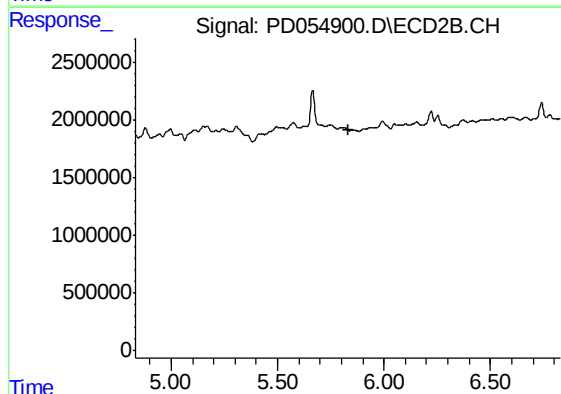


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.831 min
Response: 0
Conc: N.D.

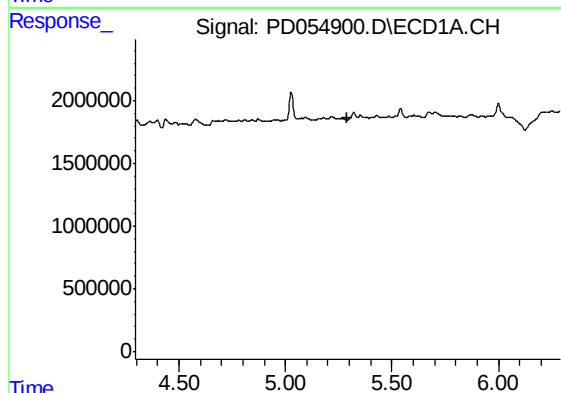


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.292 min
Response: 0
Conc: N.D.

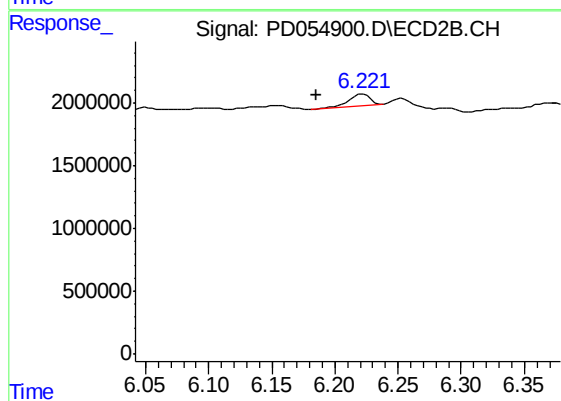

#9 Endosulfan I


R.T.: 6.222 min
Delta R.T.: 0.037 min
Response: 1133838
Conc: 0.90 ng/ml

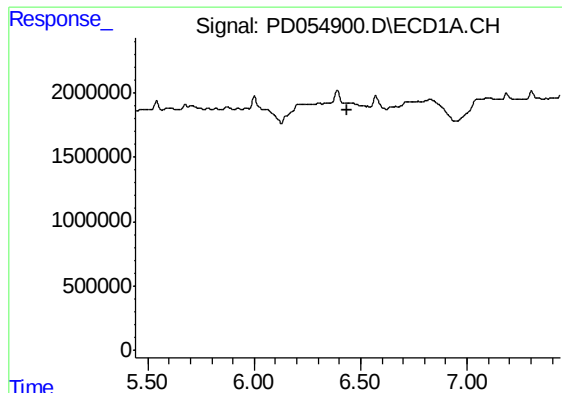

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFDG4

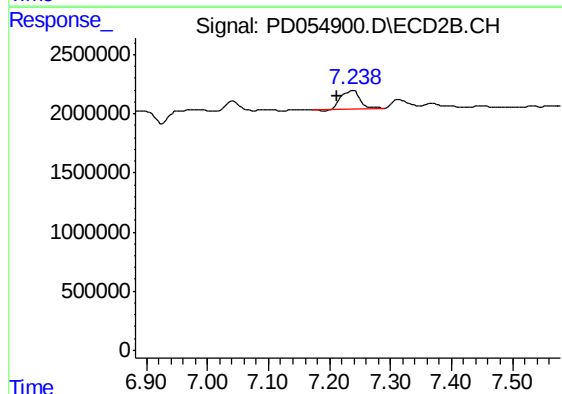


#19 Endosulfan Sulfate

R.T.: 7.240 min
Delta R.T.: 0.027 min
Response: 3329033
Conc: 2.80 ng/ml

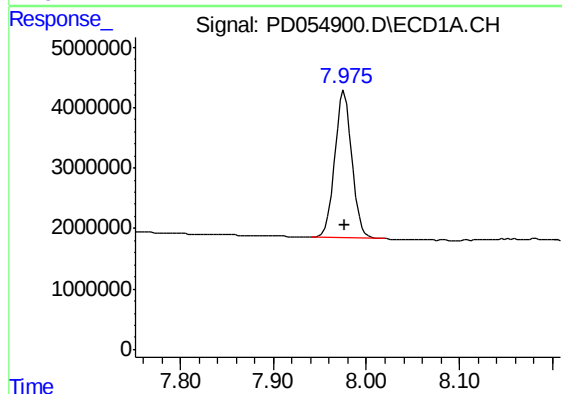

#27 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: 0.000 min
Response: 30667785
Conc: 36.40 ng/ml

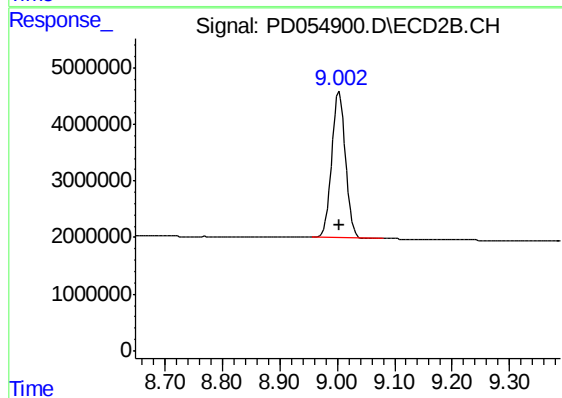

#27 Decachlorobiphenyl

R.T.: 9.003 min
Delta R.T.: -0.002 min
Response: 42648751
Conc: 36.61 ng/ml