

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
 Data File : PD059308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 22:01
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 04:48:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 04:46:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.025	6383160	7868145	4.935	4.543
27)	SA Decachlor...	8.326	9.109	9613790	11605202	11.245	10.004
Target Compounds							
2)	A alpha-BHC	3.956	4.416	8678529	11646871	4.807	4.695
3)	MA gamma-BHC...	4.243	4.702	11856830	10519964	6.557	4.623 #
4)	MA Heptachlor	4.553	5.214	8346209	11062866	4.906	5.112
9)	A Endosulfan I	5.596	6.265	6604533	8066750	5.004	4.764
13)	MA Dieldrin	5.842	6.522	13181237	16817195	9.489	9.331
14)	MA Endrin	6.101	6.740	10014811	12545926	9.894	9.742
16)	A 4,4'-DDD	6.227	6.859	10506802	12721890	9.857	9.261
17)	MA 4,4'-DDT	6.472	7.159	10263409	10414463	9.489	9.330
20)	A Methoxychlor	7.023	7.615	26009176	30155127	51.737	48.340


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 22:01
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 04:48:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 04:46:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

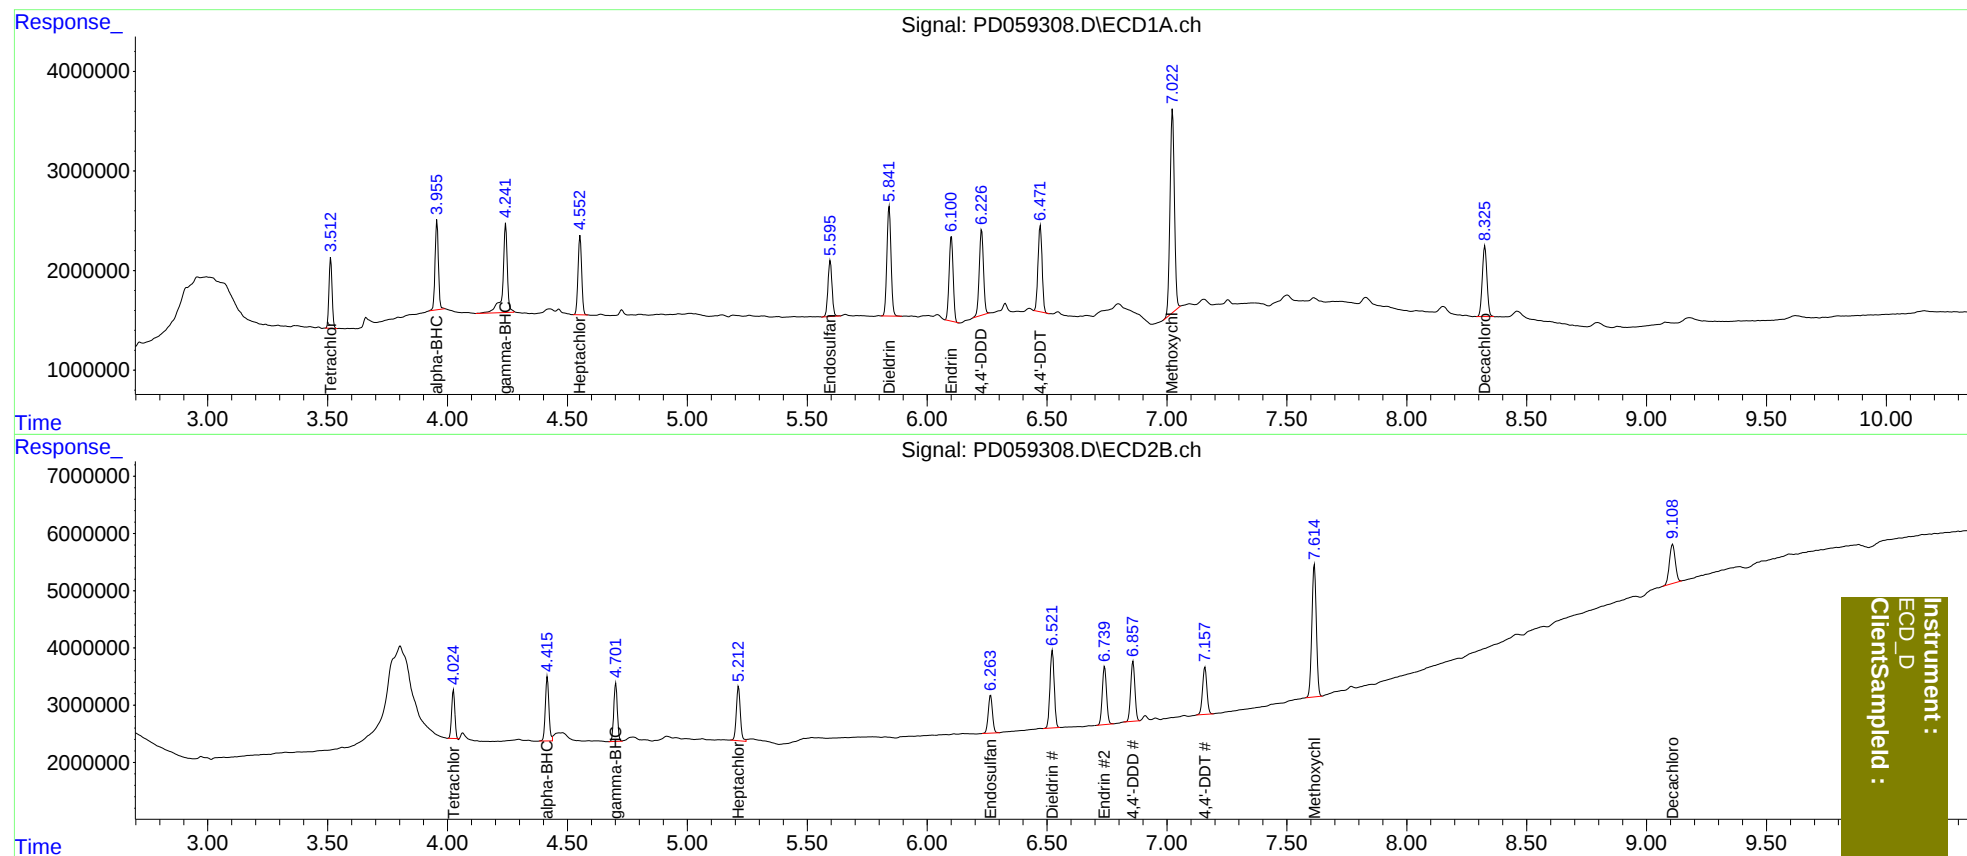


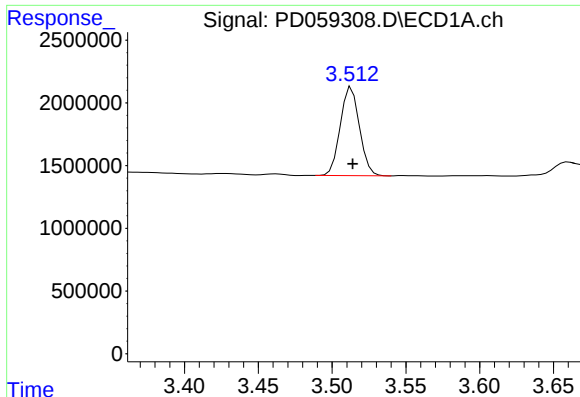

#1 Tetrachloro-m-xylene


R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 6383160
Conc: 4.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

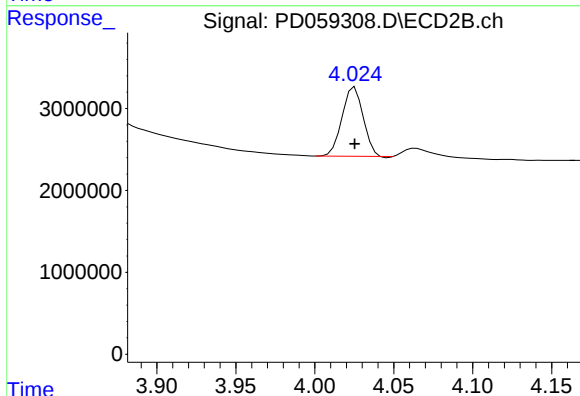


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 7868145
Conc: 4.54 ng/ml

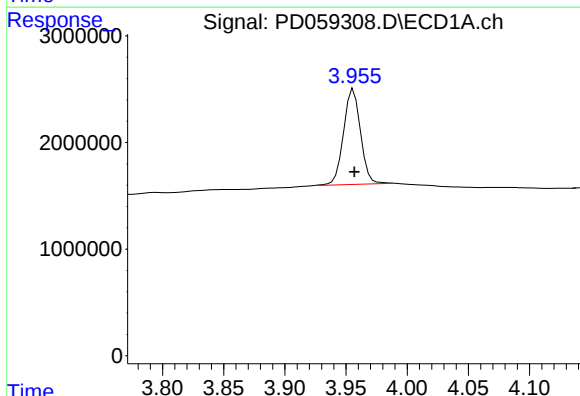


#2 alpha-BHC

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 8678529
Conc: 4.81 ng/ml

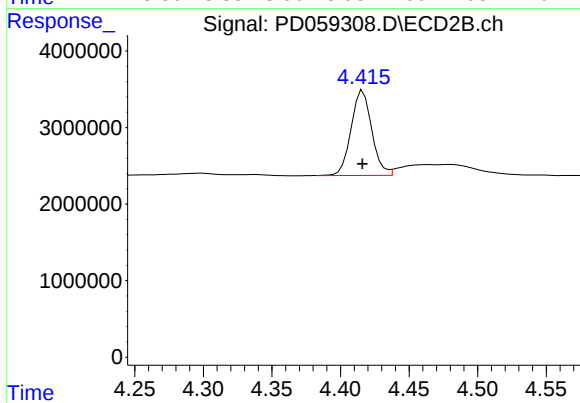

#2 alpha-BHC


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 11646871
Conc: 4.69 ng/ml

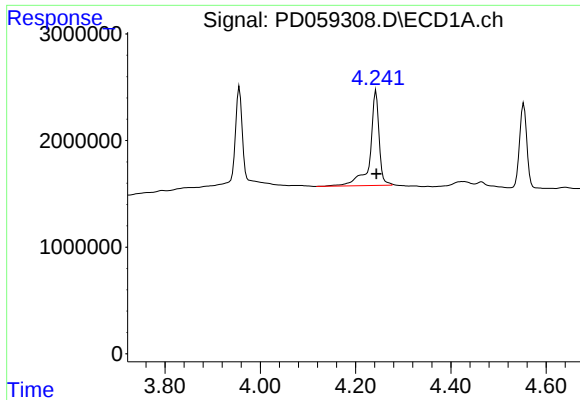

#3 gamma-BHC (Lindane)


R.T.: 4.243 min
Delta R.T.: 0.000 min
Response: 11856830
Conc: 6.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

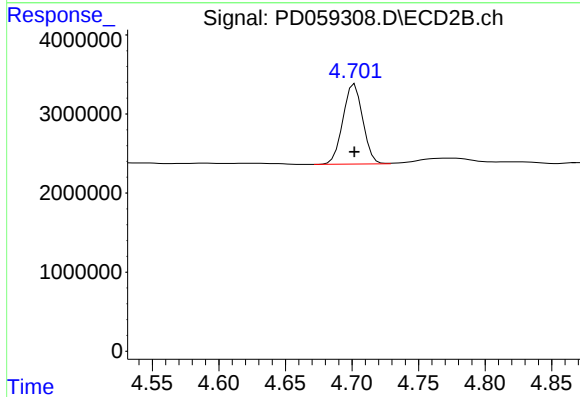


#3 gamma-BHC (Lindane)

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 10519964
Conc: 4.62 ng/ml

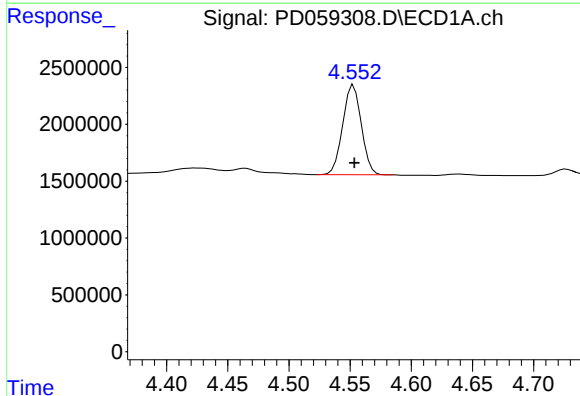


#4 Heptachlor

R.T.: 4.553 min
Delta R.T.: 0.000 min
Response: 8346209
Conc: 4.91 ng/ml

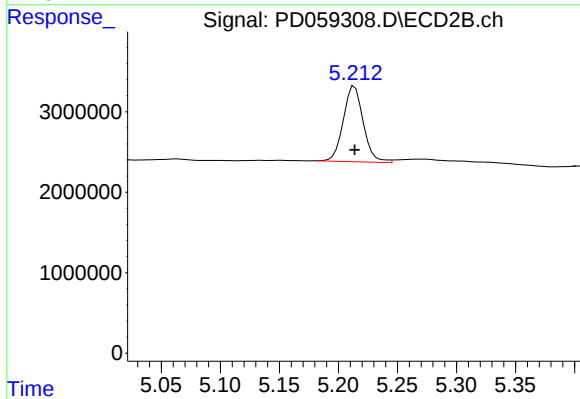

#4 Heptachlor


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 11062866
Conc: 5.11 ng/ml

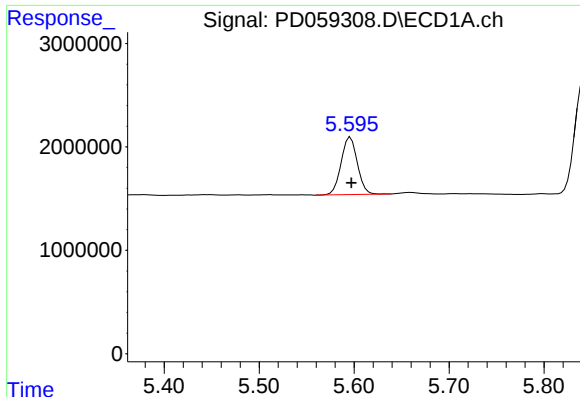

#9 Endosulfan I


R.T.: 5.596 min
Delta R.T.: -0.001 min
Response: 6604533
Conc: 5.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

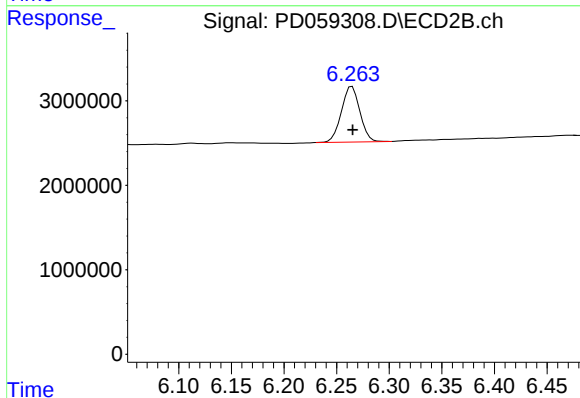


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 8066750
Conc: 4.76 ng/ml

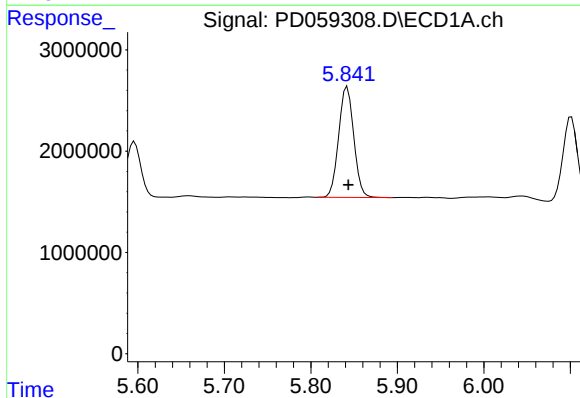


#13 Dieldrin

R.T.: 5.842 min
Delta R.T.: -0.001 min
Response: 13181237
Conc: 9.49 ng/ml

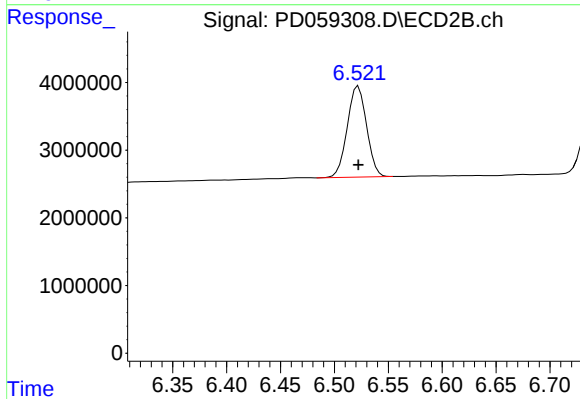

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 16817195
Conc: 9.33 ng/ml

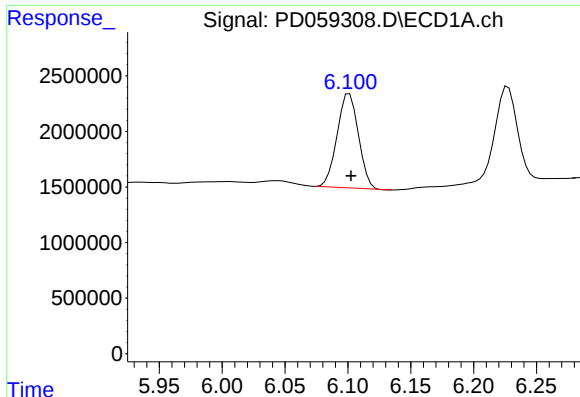

#14 Endrin


R.T.: 6.101 min
Delta R.T.: -0.001 min
Response: 10014811
Conc: 9.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

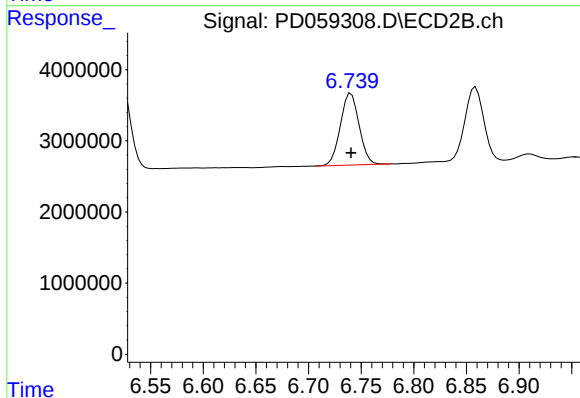


#14 Endrin

R.T.: 6.740 min
Delta R.T.: 0.000 min
Response: 12545926
Conc: 9.74 ng/ml

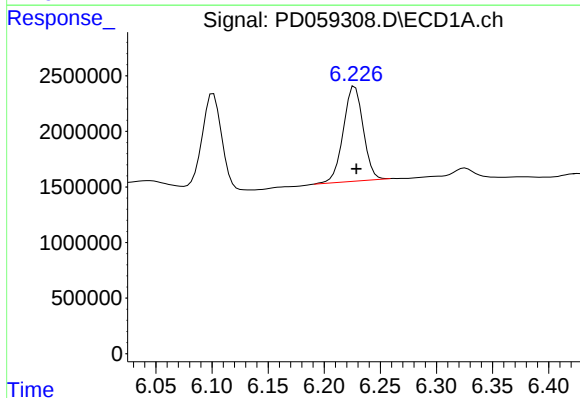


#16 4,4'-DDD

R.T.: 6.227 min
Delta R.T.: -0.001 min
Response: 10506802
Conc: 9.86 ng/ml

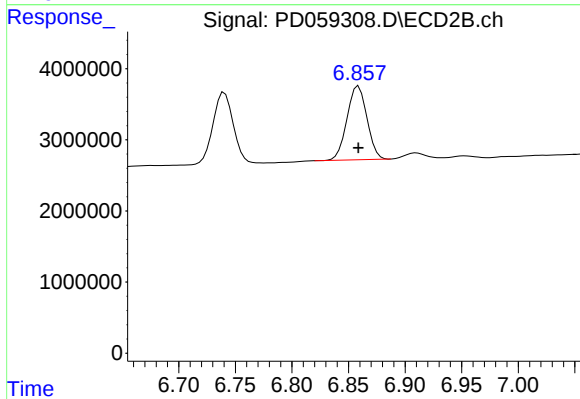

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 12721890
Conc: 9.26 ng/ml

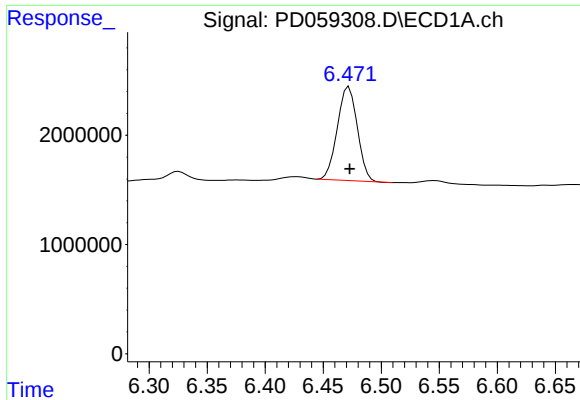

#17 4,4'-DDT


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 10263409
Conc: 9.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

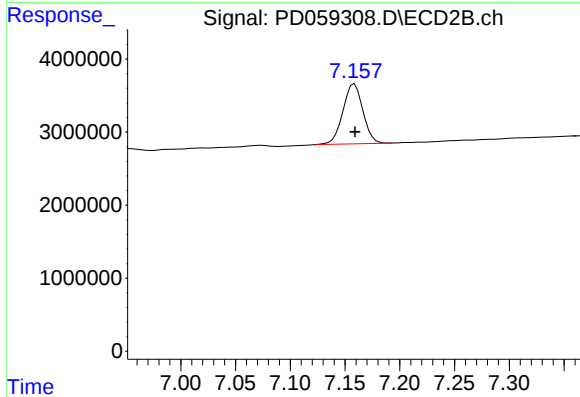


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 10414463
Conc: 9.33 ng/ml

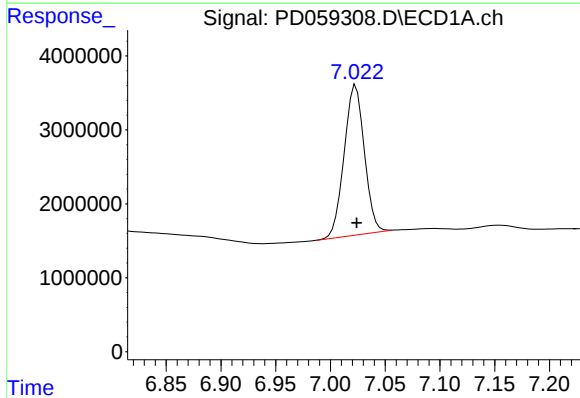


#20 Methoxychlor

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 26009176
Conc: 51.74 ng/ml

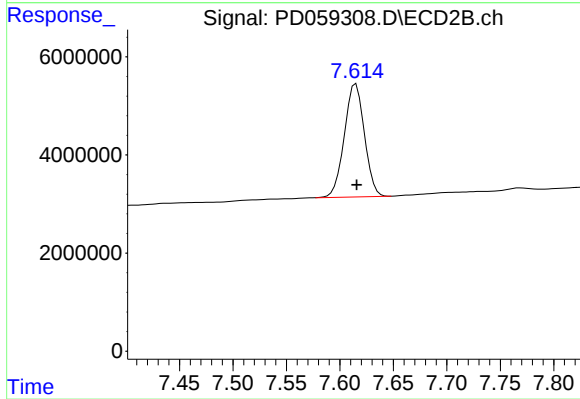

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 30155127
Conc: 48.34 ng/ml

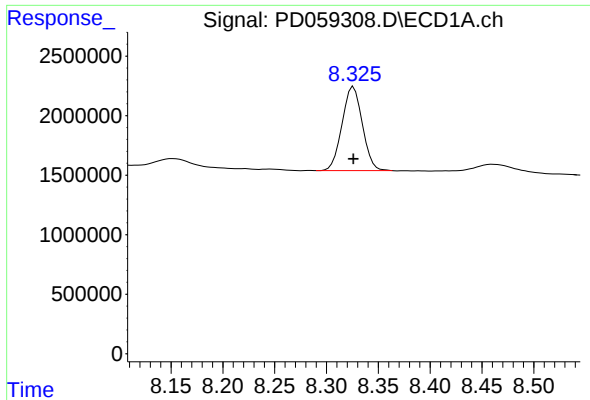

#27 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 9613790
Conc: 11.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

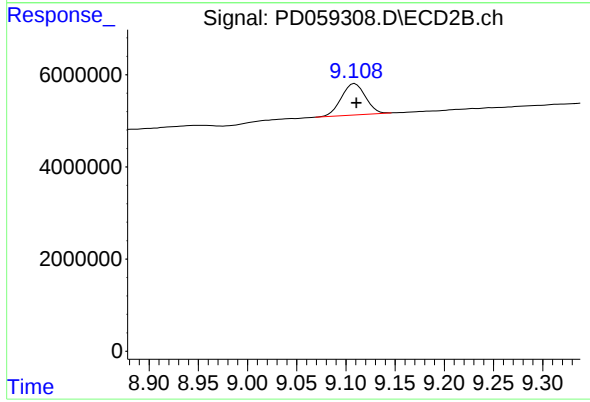

#27 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.002 min
Response: 11605202
Conc: 10.00 ng/ml