

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
 Data File : PD059310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 22:30
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 04:48:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 04:46:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.514	4.025	13073916	17436541	10.108	10.067
27)	SA Decachlor...	8.326	9.109	18090207	23426343	21.159	20.193
Target Compounds							
2)	A alpha-BHC	3.956	4.416	17535094	24450705	9.713	9.856
3)	MA gamma-BHC...	4.244	4.701	21359344	22427170	11.812	9.855
4)	MA Heptachlor	4.553	5.213	16641707	21691738	9.782	10.023
9)	A Endosulfan I	5.596	6.264	13221751	16793801	10.017	9.918
13)	MA Dieldrin	5.843	6.522	26621724	35468464	19.165	19.680
14)	MA Endrin	6.102	6.741	19666348	25432148	19.430	19.749
16)	A 4,4'-DDD	6.227	6.859	20778854	26892077	19.493	19.576
17)	MA 4,4'-DDT	6.472	7.159	21006630	21410094	19.421	19.182
20)	A Methoxychlor	7.024	7.615	50167279	61282432	99.792	98.239


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 22:30
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 04:48:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 04:46:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

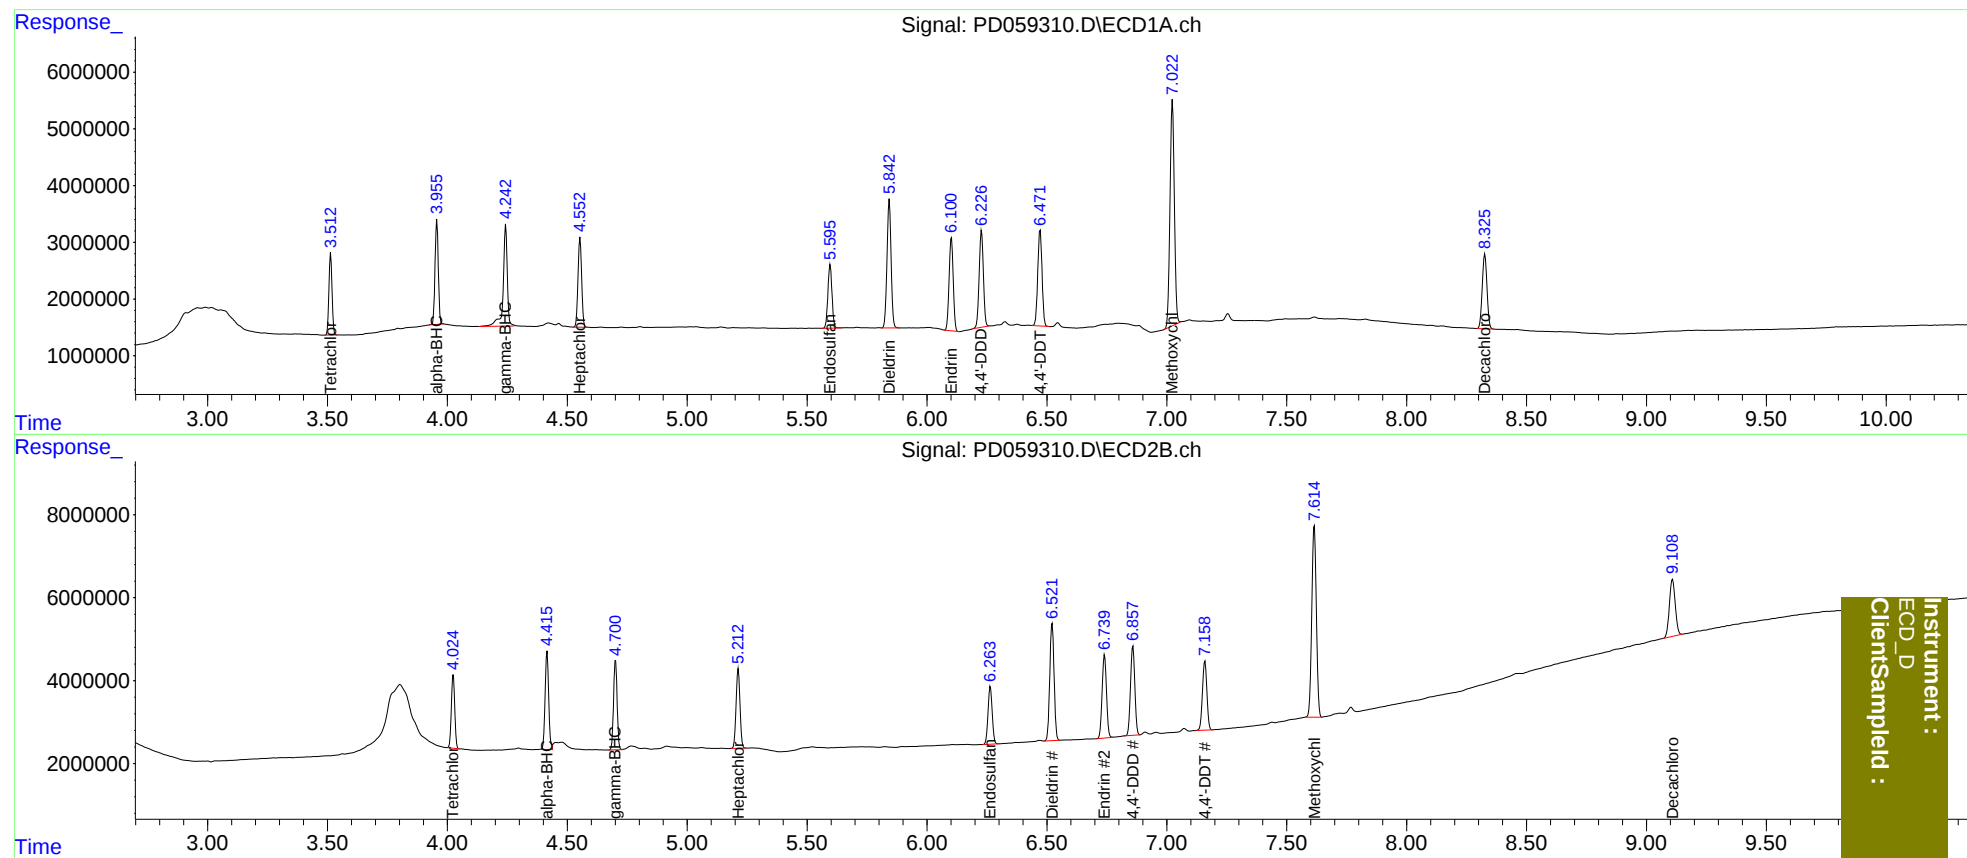


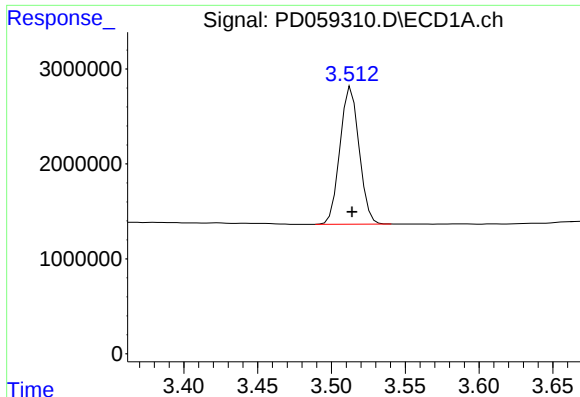

#1 Tetrachloro-m-xylene


R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 13073916
Conc: 10.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

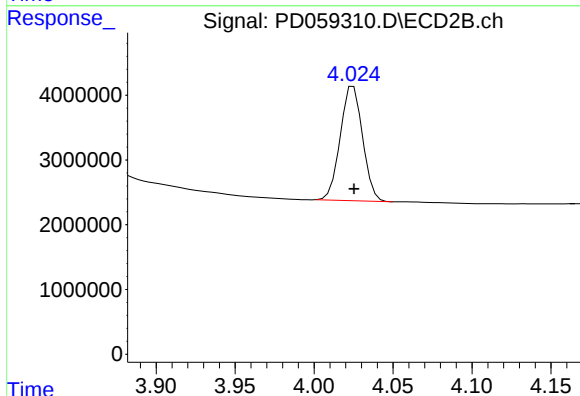


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 17436541
Conc: 10.07 ng/ml

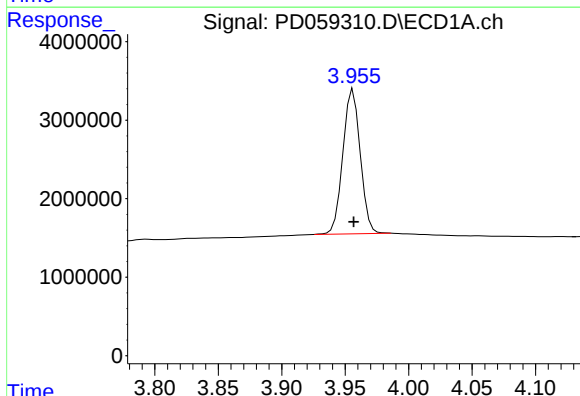


#2 alpha-BHC

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 17535094
Conc: 9.71 ng/ml

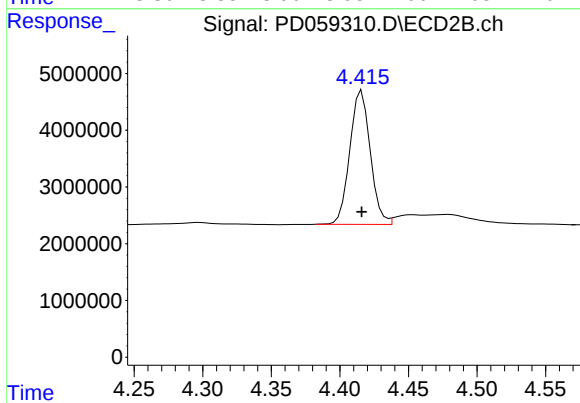

#2 alpha-BHC


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 24450705
Conc: 9.86 ng/ml

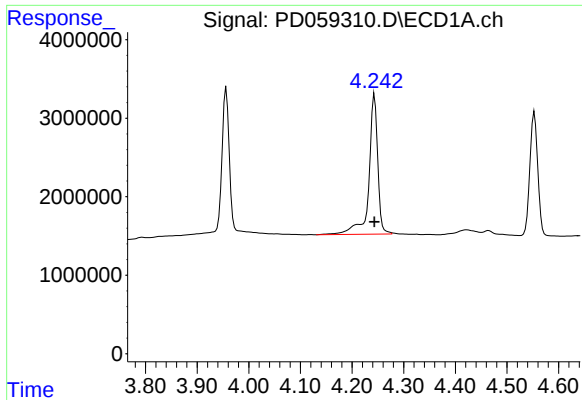

#3 gamma-BHC (Lindane)


R.T.: 4.244 min
Delta R.T.: 0.000 min
Response: 21359344
Conc: 11.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

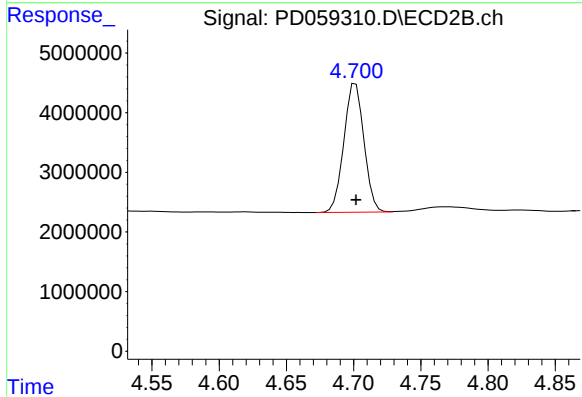


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 22427170
Conc: 9.85 ng/ml

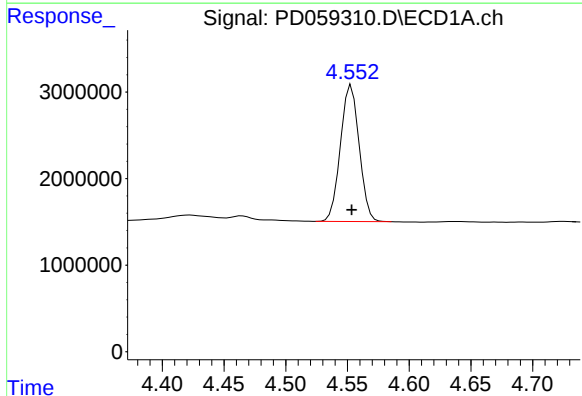


#4 Heptachlor

R.T.: 4.553 min
Delta R.T.: 0.000 min
Response: 16641707
Conc: 9.78 ng/ml

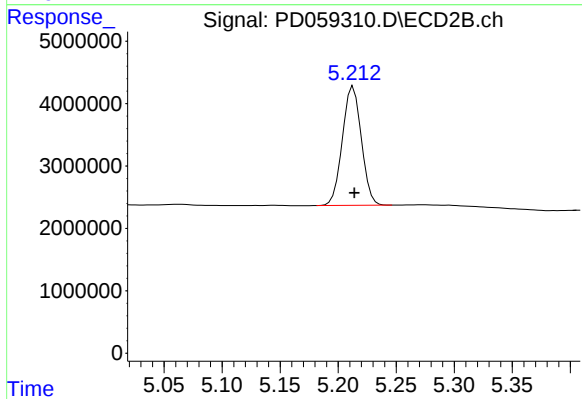

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 21691738
Conc: 10.02 ng/ml

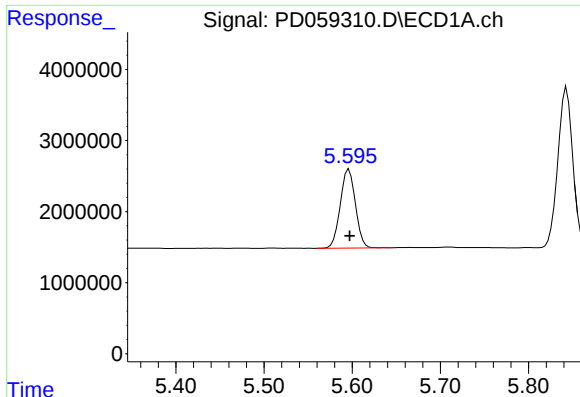

#9 Endosulfan I


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 13221751
Conc: 10.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

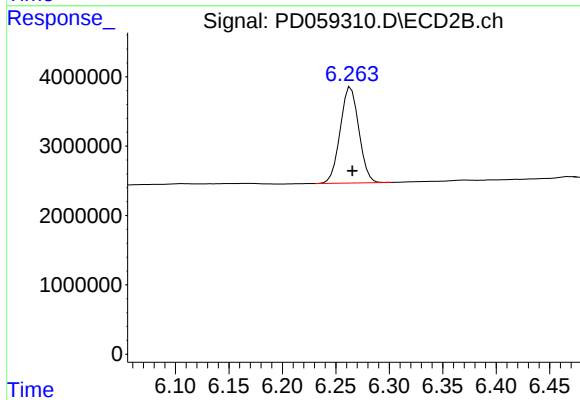


#9 Endosulfan I

R.T.: 6.264 min
Delta R.T.: -0.001 min
Response: 16793801
Conc: 9.92 ng/ml

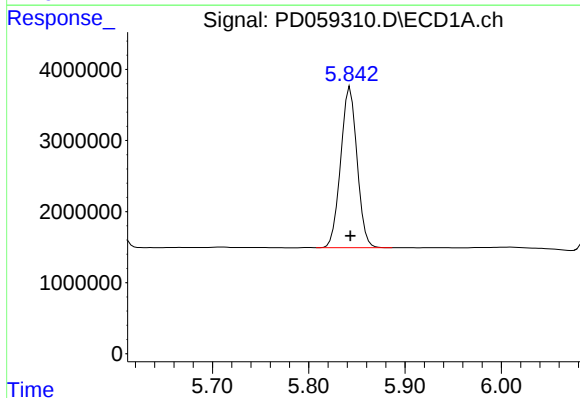


#13 Dieldrin

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 26621724
Conc: 19.17 ng/ml

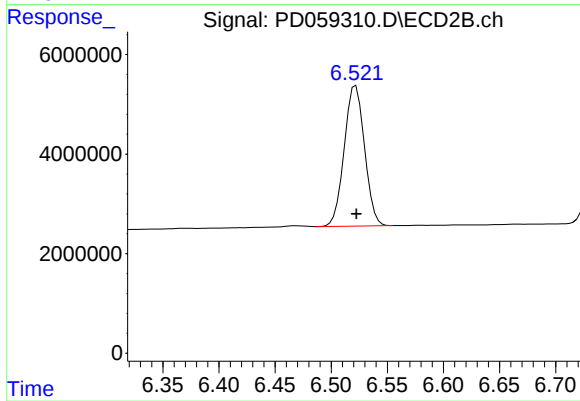

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 35468464
Conc: 19.68 ng/ml

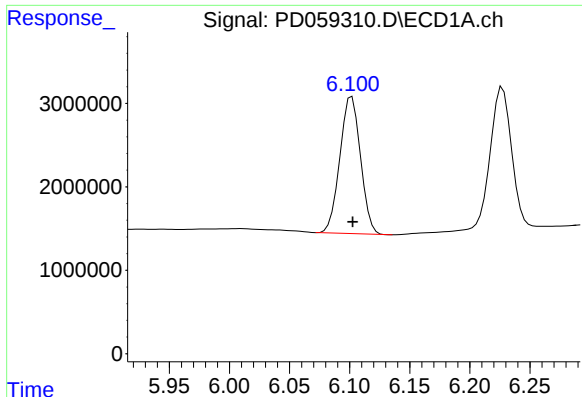

#14 Endrin


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 19666348
Conc: 19.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

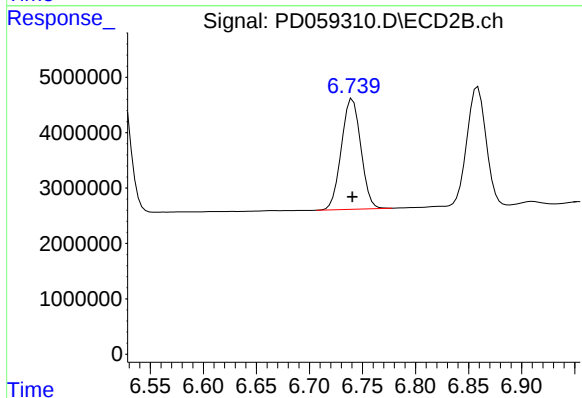


#14 Endrin

R.T.: 6.741 min
Delta R.T.: 0.000 min
Response: 25432148
Conc: 19.75 ng/ml

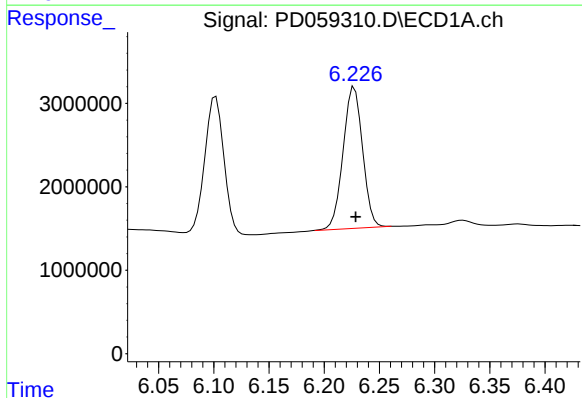


#16 4,4'-DDD

R.T.: 6.227 min
Delta R.T.: -0.001 min
Response: 20778854
Conc: 19.49 ng/ml

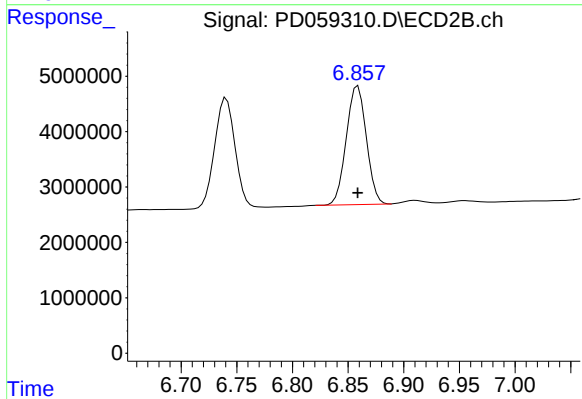

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 26892077
Conc: 19.58 ng/ml

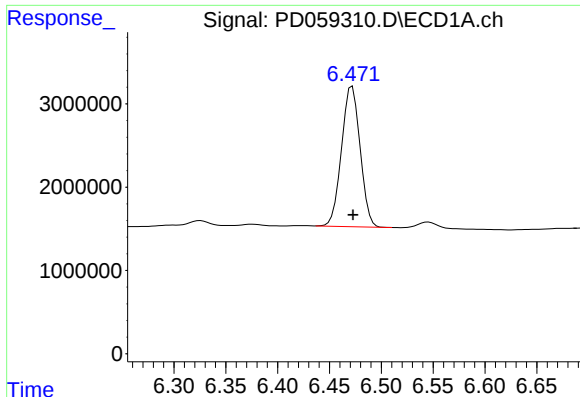

#17 4,4'-DDT


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 21006630
Conc: 19.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

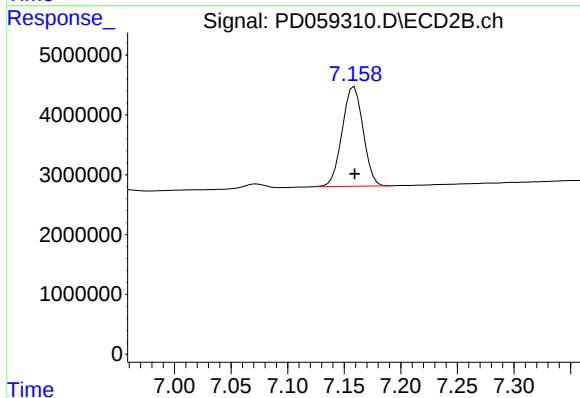


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 21410094
Conc: 19.18 ng/ml

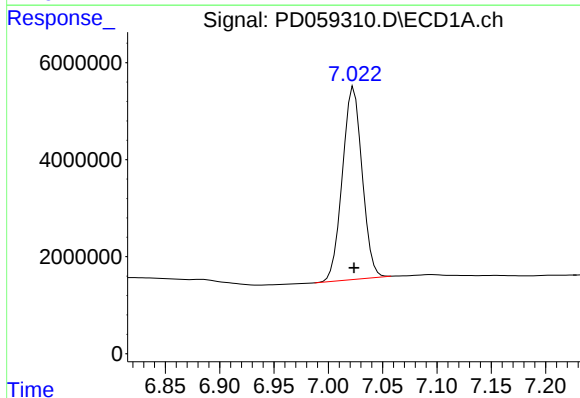


#20 Methoxychlor

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 50167279
Conc: 99.79 ng/ml

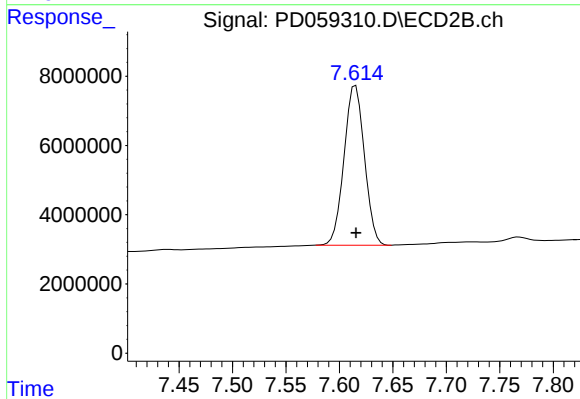

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 61282432
Conc: 98.24 ng/ml

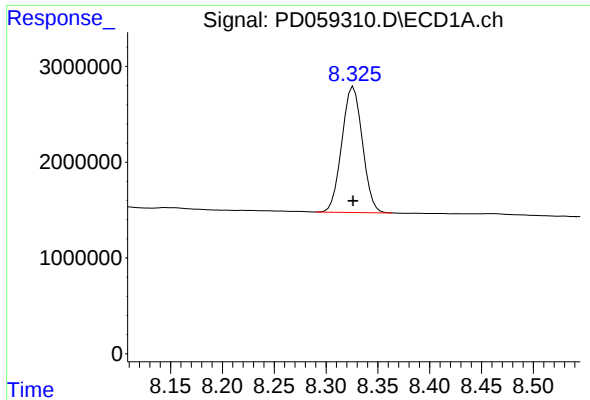

#27 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 18090207
Conc: 21.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

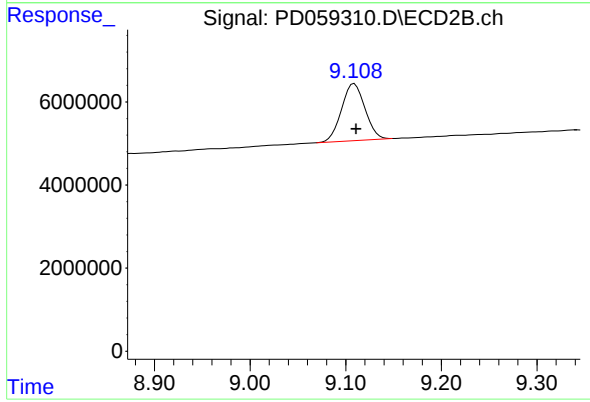

#27 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.002 min
Response: 23426343
Conc: 20.19 ng/ml