

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
 Data File : PD059312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 22:58
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 04:48:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 04:46:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.514	4.025	25868455	34639867	20.000	20.000
27)	SA Decachlor...	8.326	9.111	34198147	46404563	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.957	4.416	36107976	49615191	20.000	20.000
3)	MA gamma-BHC...	4.244	4.702	36164672	45515810	20.000	20.000
4)	MA Heptachlor	4.553	5.214	34025881	43281775	20.000	20.000
9)	A Endosulfan I	5.597	6.265	26397518	33866179	20.000	20.000
13)	MA Dieldrin	5.843	6.522	55562255	72090318	40.000	40.000
14)	MA Endrin	6.103	6.740	40486761	51510369	40.000	40.000
16)	A 4,4'-DDD	6.229	6.859	42638929	54949044	40.000	40.000
17)	MA 4,4'-DDT	6.473	7.159	43265979	44647293	40.000	40.000
20)	A Methoxychlor	7.024	7.616	100.5E6	124.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 22:58
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 04:48:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 04:46:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

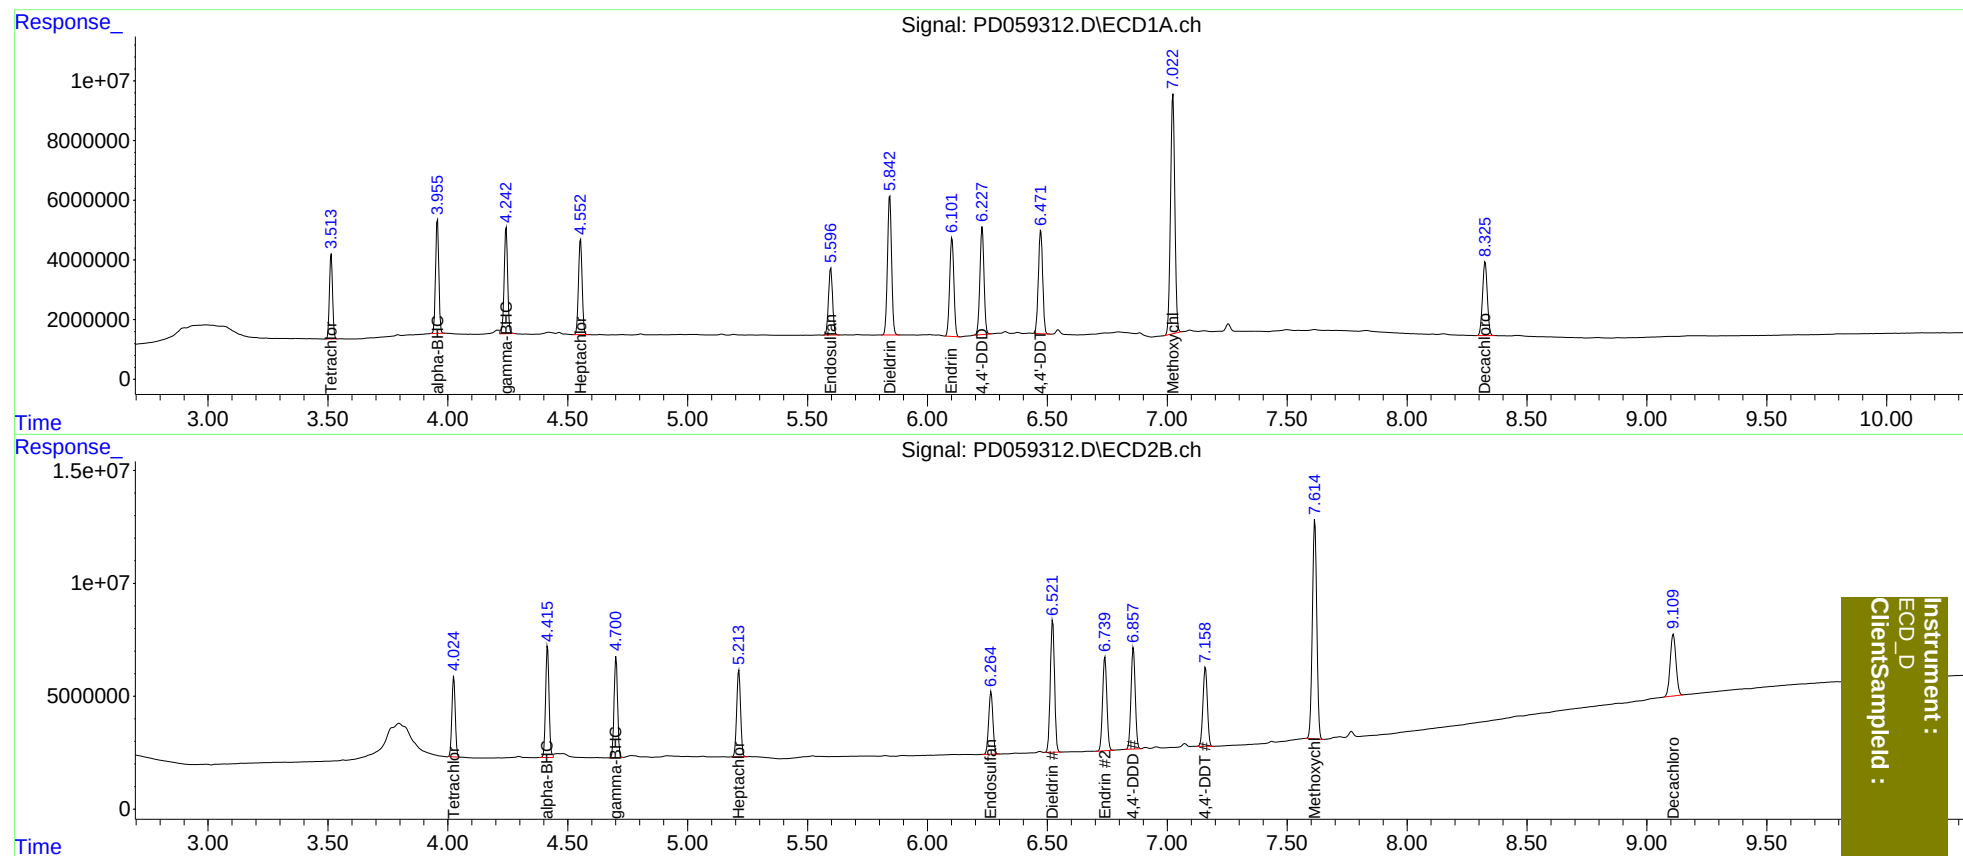


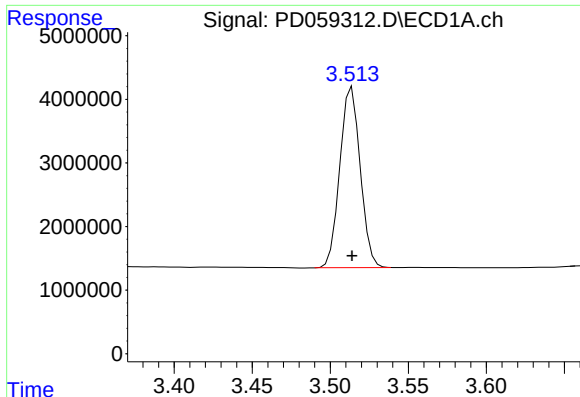

#1 Tetrachloro-m-xylene


R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 25868455
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

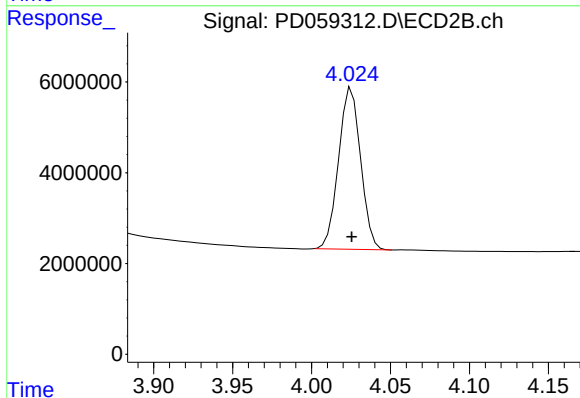


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 34639867
Conc: 20.00 ng/ml

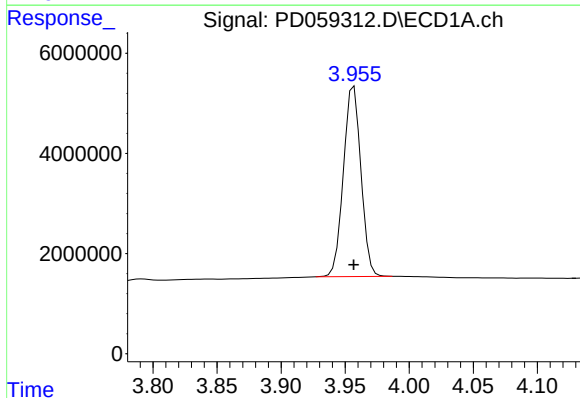


#2 alpha-BHC

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 36107976
Conc: 20.00 ng/ml

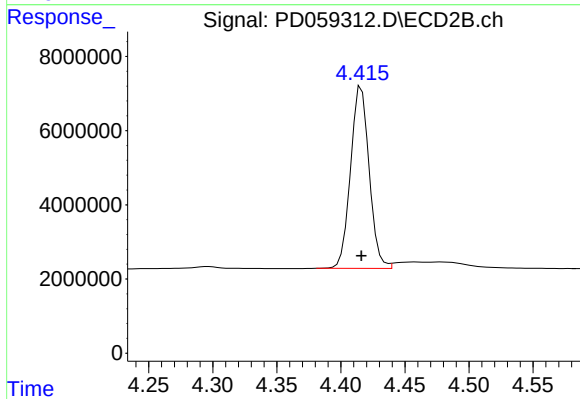

#2 alpha-BHC


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 49615191
Conc: 20.00 ng/ml

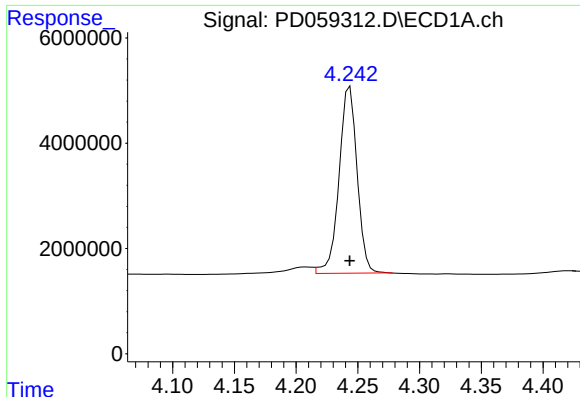

#3 gamma-BHC (Lindane)


R.T.: 4.244 min
Delta R.T.: 0.000 min
Response: 36164672
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

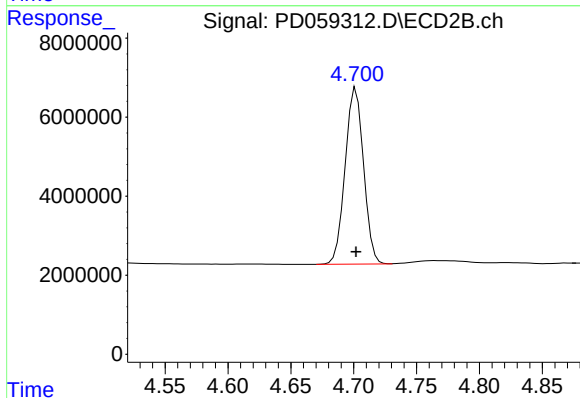


#3 gamma-BHC (Lindane)

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 45515810
Conc: 20.00 ng/ml

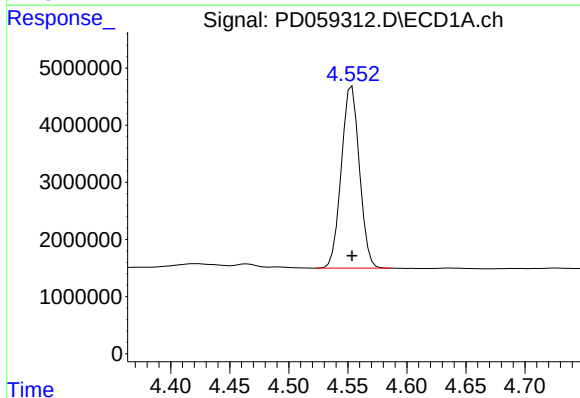


#4 Heptachlor

R.T.: 4.553 min
Delta R.T.: 0.000 min
Response: 34025881
Conc: 20.00 ng/ml

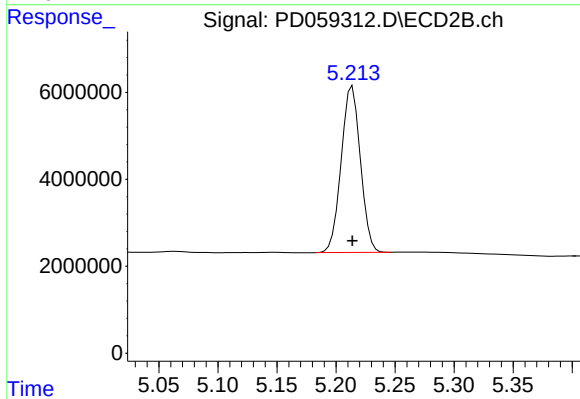

#4 Heptachlor


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 43281775
Conc: 20.00 ng/ml

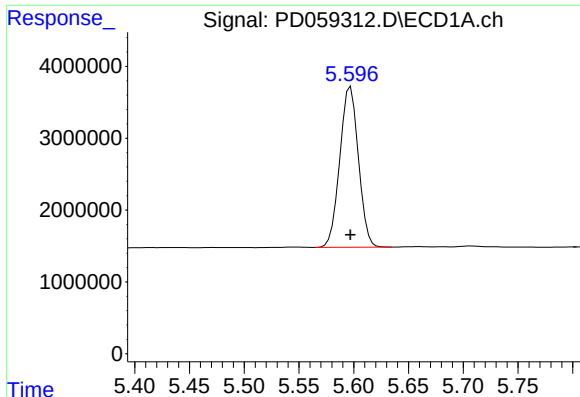

#9 Endosulfan I


R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 26397518
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

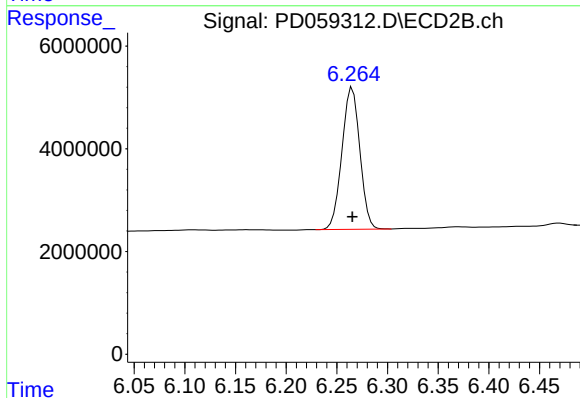


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 33866179
Conc: 20.00 ng/ml

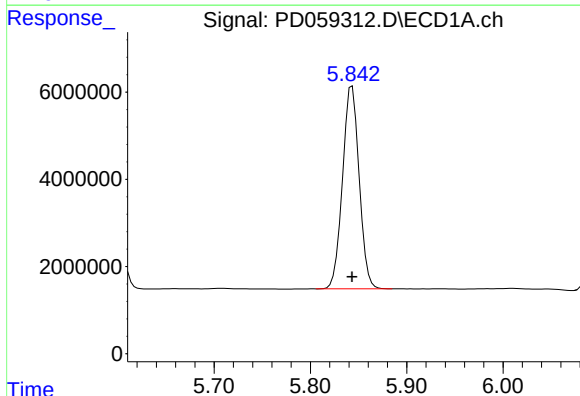


#13 Dieldrin

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 55562255
Conc: 40.00 ng/ml

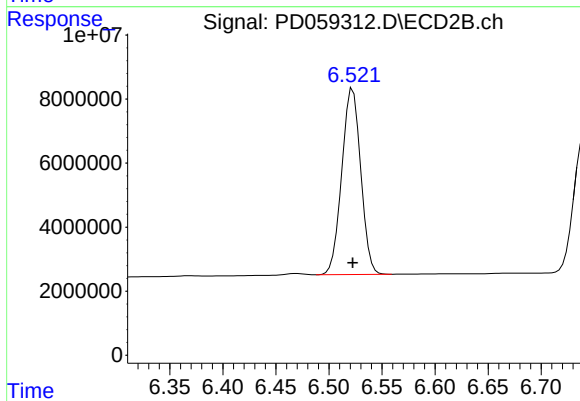

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 72090318
Conc: 40.00 ng/ml

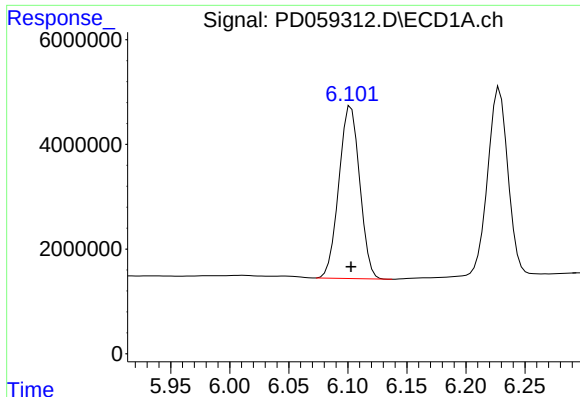

#14 Endrin


R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 40486761
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

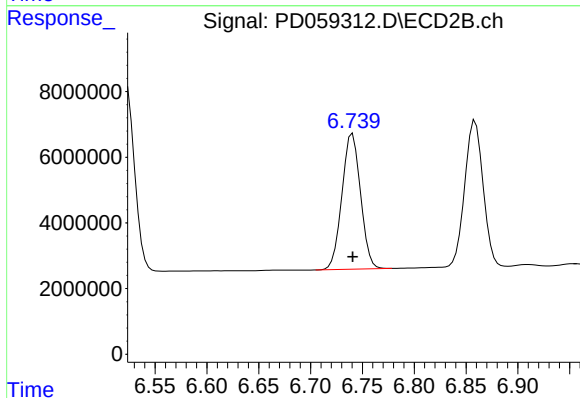


#14 Endrin

R.T.: 6.740 min
Delta R.T.: 0.000 min
Response: 51510369
Conc: 40.00 ng/ml

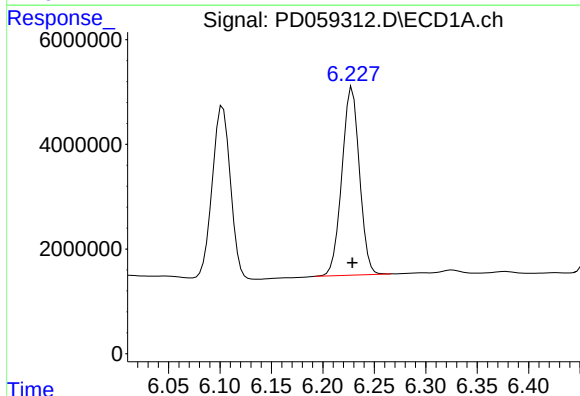


#16 4,4'-DDD

R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 42638929
Conc: 40.00 ng/ml

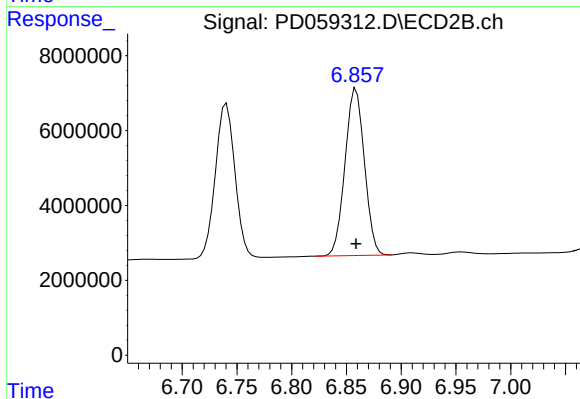

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 54949044
Conc: 40.00 ng/ml

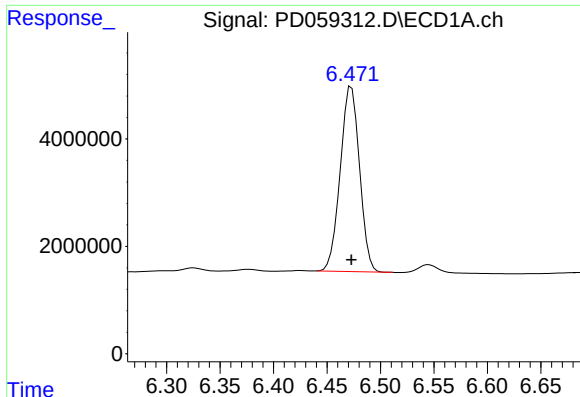

#17 4,4'-DDT


R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 43265979
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

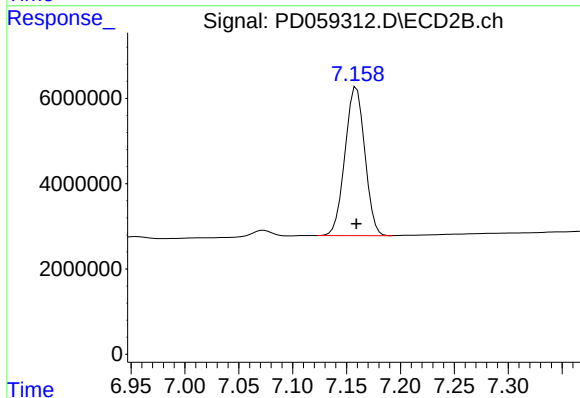


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 44647293
Conc: 40.00 ng/ml

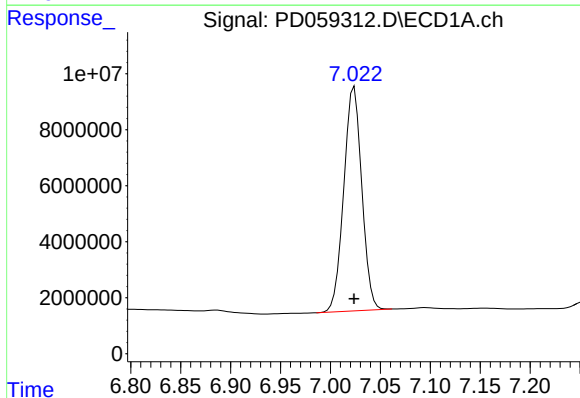


#20 Methoxychlor

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 100543318
Conc: 200.00 ng/ml

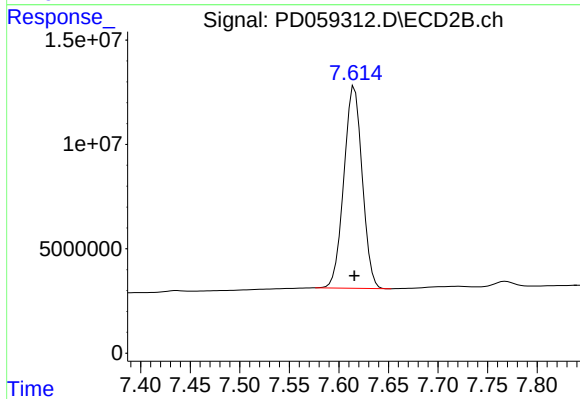

#20 Methoxychlor


R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 124762016
Conc: 200.00 ng/ml

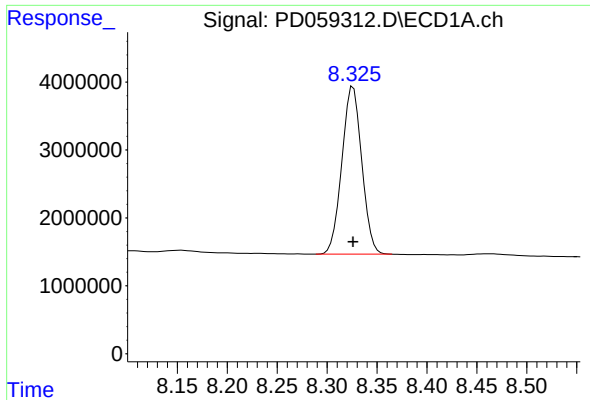

#27 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 34198147
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

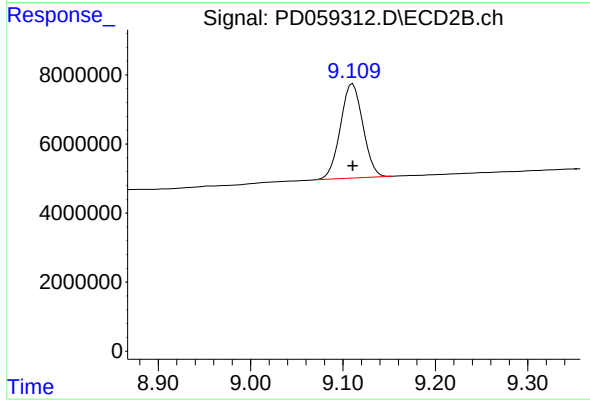

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 46404563
Conc: 40.00 ng/ml