

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
 Data File : PD059314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 23:27
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 04:48:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 04:46:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.514	4.026	49085045	68332537	37.950	39.453
27)	SA Decachlor...	8.326	9.110	62520445	89041149	73.127	76.752
Target Compounds							
2)	A alpha-BHC	3.957	4.416	71127261	99695252	39.397	40.187
3)	MA gamma-BHC...	4.244	4.702	69398034	91557261	38.379	40.231
4)	MA Heptachlor	4.554	5.213	65665788	86645546	38.598	40.038
9)	A Endosulfan I	5.597	6.265	50212750	66289739	38.044	39.148
13)	MA Dieldrin	5.843	6.523	108.6E6	144.2E6	78.171	80.014
14)	MA Endrin	6.103	6.741	78033816	102.8E6	77.096	79.829
16)	A 4,4'-DDD	6.228	6.860	82528787	109.8E6	77.421	79.946
17)	MA 4,4'-DDT	6.473	7.159	85084726	91177546	78.662	81.687
20)	A Methoxychlor	7.024	7.616	192.0E6	249.5E6	381.919	400.028


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 23:27
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 04:48:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 04:46:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

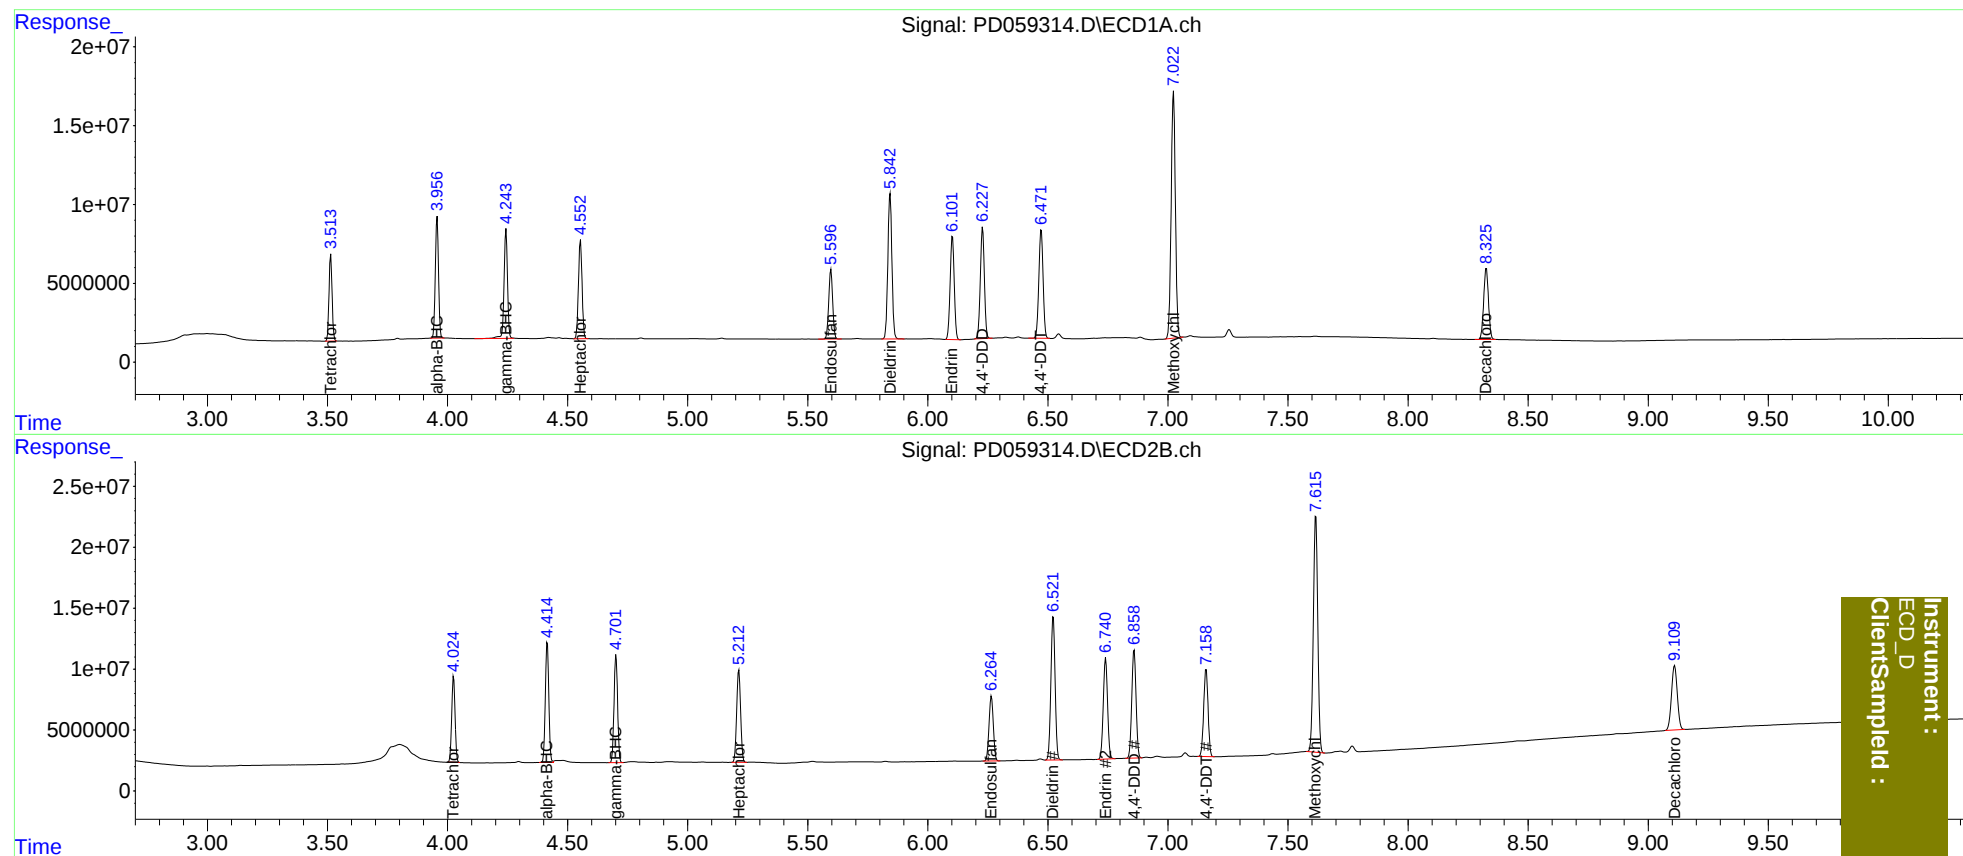


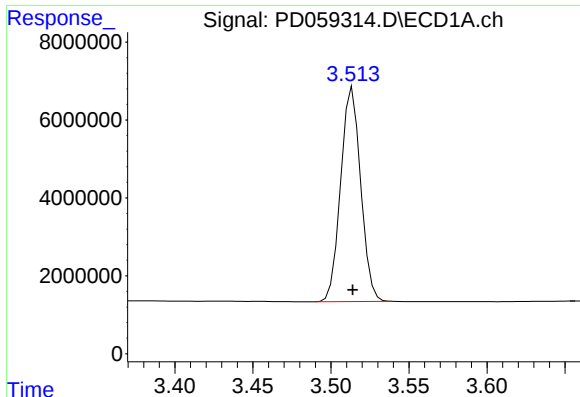

#1 Tetrachloro-m-xylene


R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 49085045
Conc: 37.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

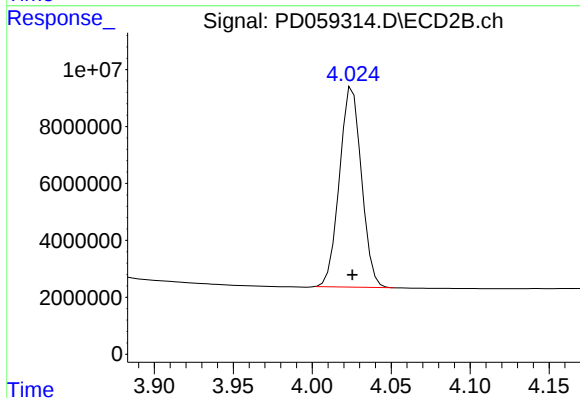


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 68332537
Conc: 39.45 ng/ml

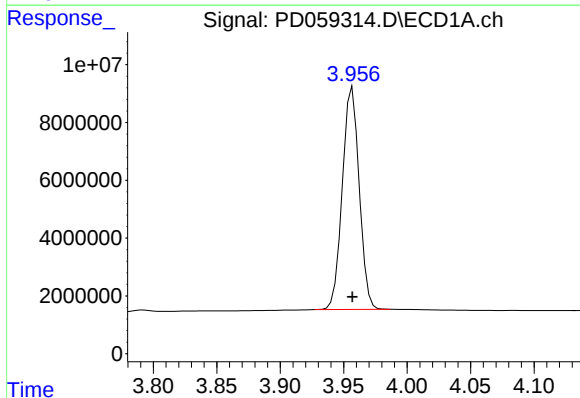


#2 alpha-BHC

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 71127261
Conc: 39.40 ng/ml

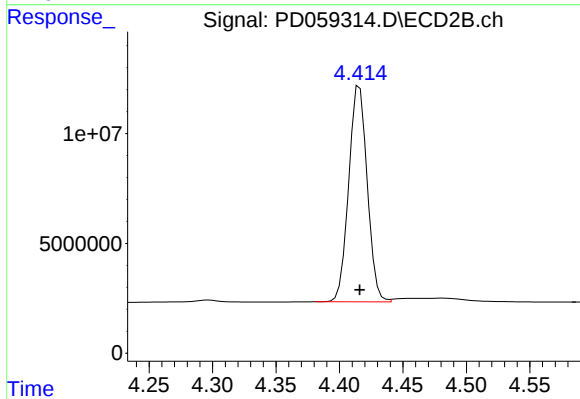

#2 alpha-BHC

R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 99695252
Conc: 40.19 ng/ml

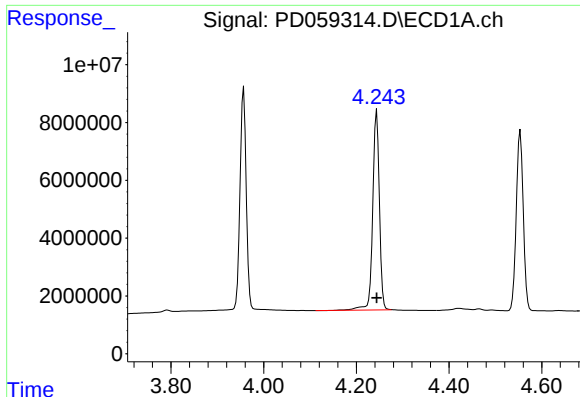

#3 gamma-BHC (Lindane)


R.T.: 4.244 min

Delta R.T.: 0.000 min

Response: 69398034

Conc: 38.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

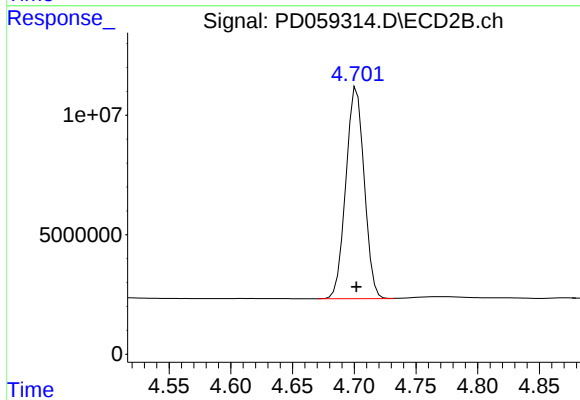


#3 gamma-BHC (Lindane)

R.T.: 4.702 min

Delta R.T.: 0.000 min

Response: 91557261

Conc: 40.23 ng/ml

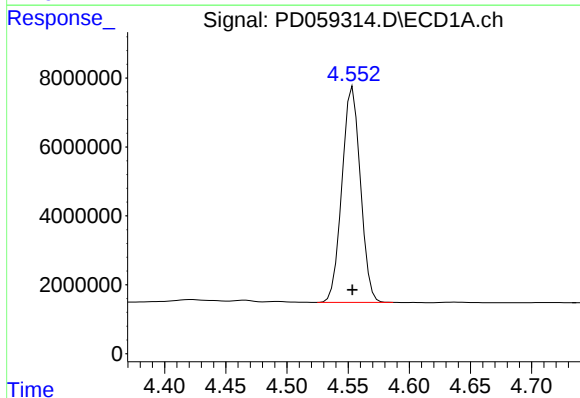


#4 Heptachlor

R.T.: 4.554 min

Delta R.T.: 0.000 min

Response: 65665788

Conc: 38.60 ng/ml

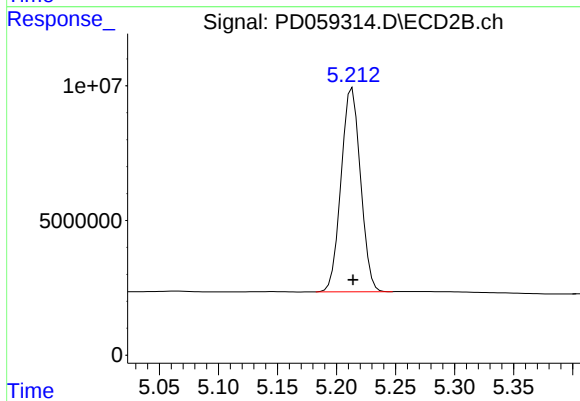


#4 Heptachlor

R.T.: 5.213 min

Delta R.T.: 0.000 min

Response: 86645546


Conc: 40.04 ng/ml

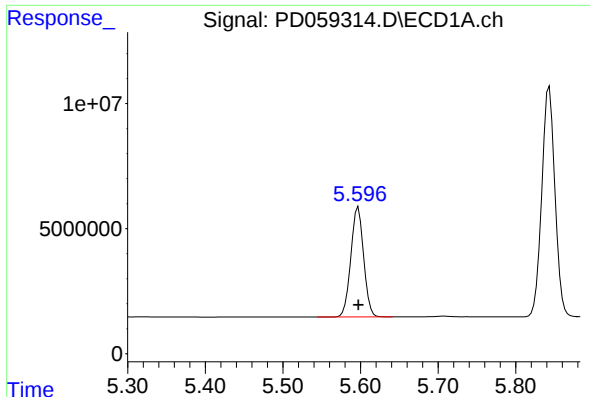

#9 Endosulfan I


R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 50212750
Conc: 38.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

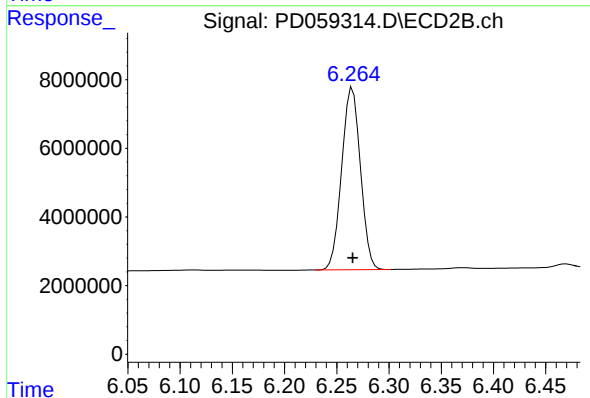


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 66289739
Conc: 39.15 ng/ml

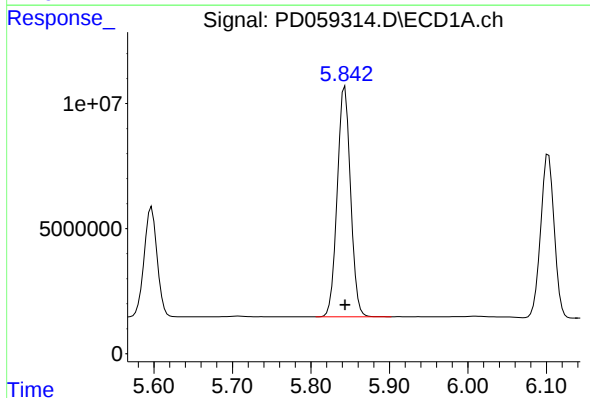


#13 Dieldrin

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 108583234
Conc: 78.17 ng/ml

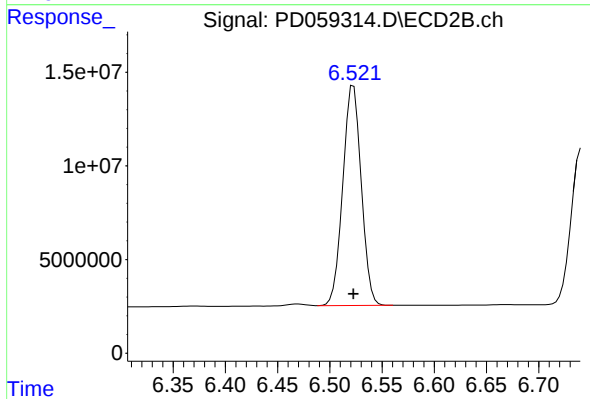

#13 Dieldrin


R.T.: 6.523 min
Delta R.T.: 0.000 min
Response: 144205570
Conc: 80.01 ng/ml

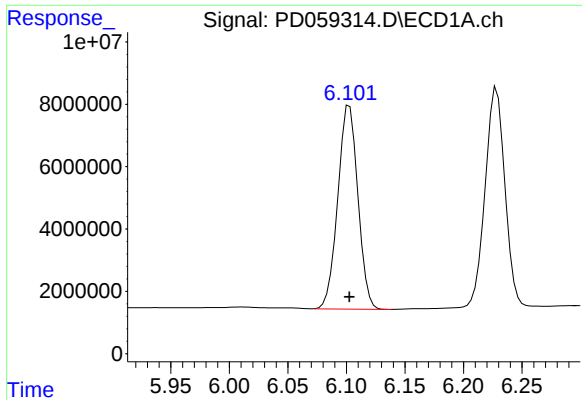

#14 Endrin


R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 78033816
Conc: 77.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

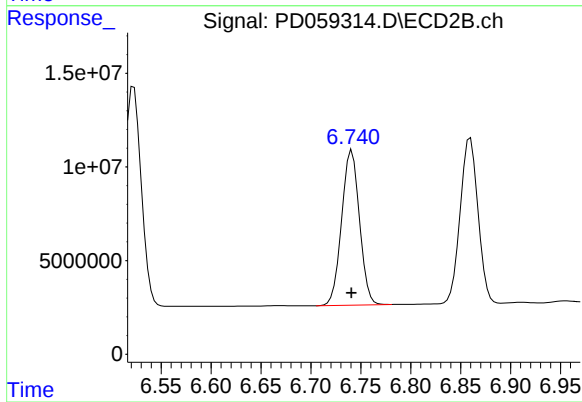


#14 Endrin

R.T.: 6.741 min
Delta R.T.: 0.000 min
Response: 102799928
Conc: 79.83 ng/ml

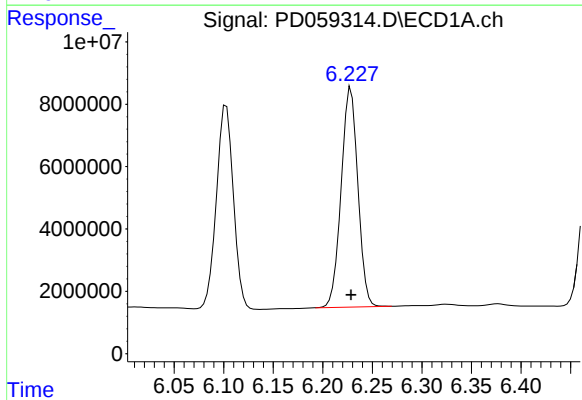


#16 4,4'-DDD

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 82528787
Conc: 77.42 ng/ml

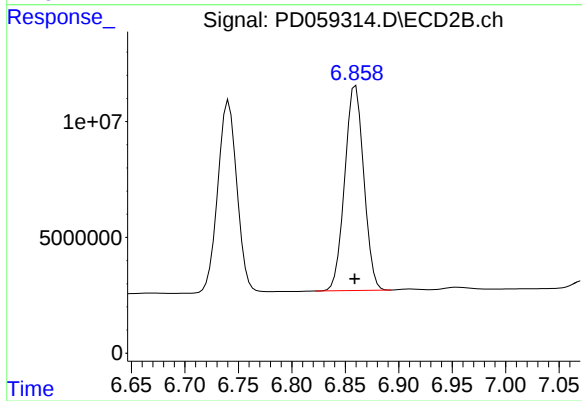

#16 4,4'-DDD


R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 109823895
Conc: 79.95 ng/ml

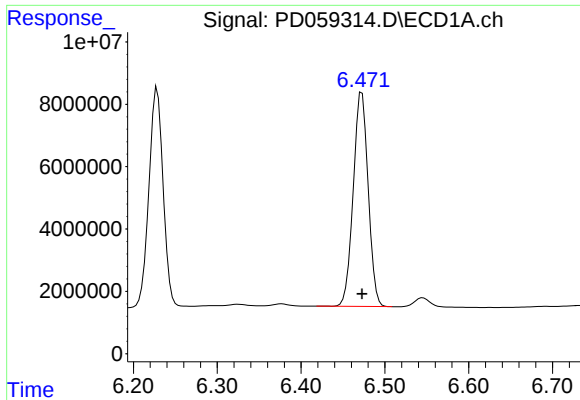

#17 4,4'-DDT


R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 85084726
Conc: 78.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

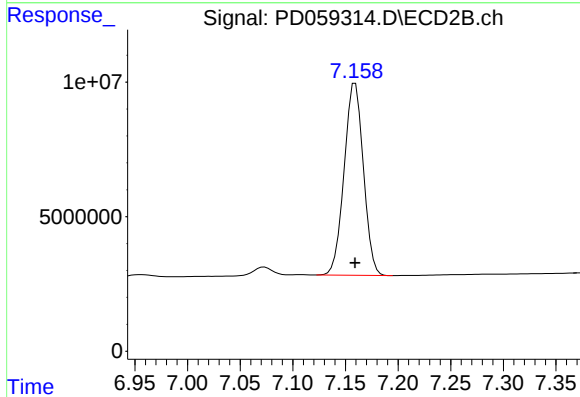


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 91177546
Conc: 81.69 ng/ml

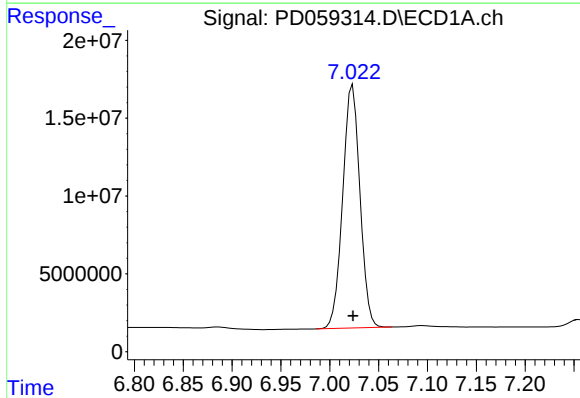


#20 Methoxychlor

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 191996953
Conc: 381.92 ng/ml

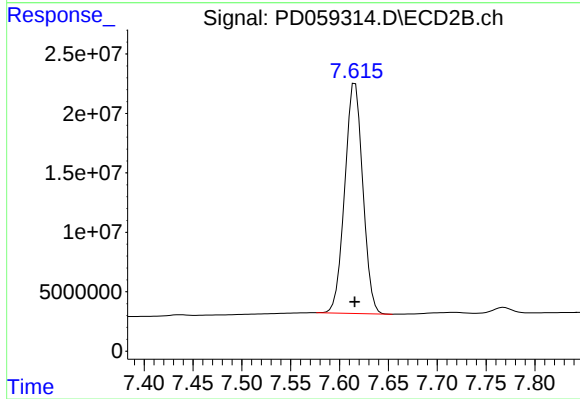

#20 Methoxychlor


R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 249541743
Conc: 400.03 ng/ml

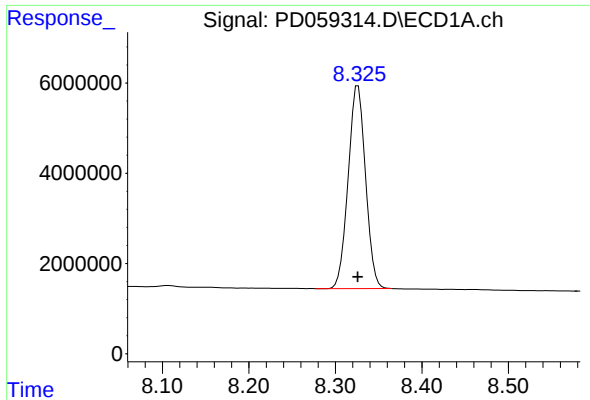

#27 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 62520445
Conc: 73.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

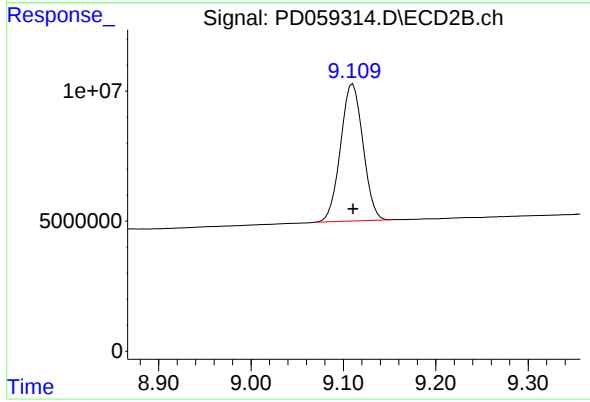

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 89041149
Conc: 76.75 ng/ml