

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
 Data File : PD059316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 23:55
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 04:49:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 04:46:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.514	4.026	93376239	132.5E6	72.193	76.490
27)	SA Decachlor...	8.326	9.109	114.7E6	173.9E6	134.182	149.906
Target Compounds							
2)	A alpha-BHC	3.957	4.416	139.8E6	199.5E6	77.412	80.416
3)	MA gamma-BHC...	4.244	4.702	132.3E6	181.8E6	73.153	79.906
4)	MA Heptachlor	4.554	5.214	128.4E6	169.4E6	75.444	78.270
9)	A Endosulfan I	5.597	6.265	97010182	131.6E6	73.499	77.704
13)	MA Dieldrin	5.843	6.523	214.8E6	290.8E6	154.665	161.351
14)	MA Endrin	6.102	6.741	154.5E6	210.1E6	152.639	163.172
16)	A 4,4'-DDD	6.228	6.859	161.3E6	222.0E6	151.343	161.636
17)	MA 4,4'-DDT	6.472	7.159	166.8E6	190.3E6	154.199	170.448
20)	A Methoxychlor	7.023	7.615	368.5E6	508.3E6	732.933	814.906

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 23:55
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 04:49:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 04:46:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

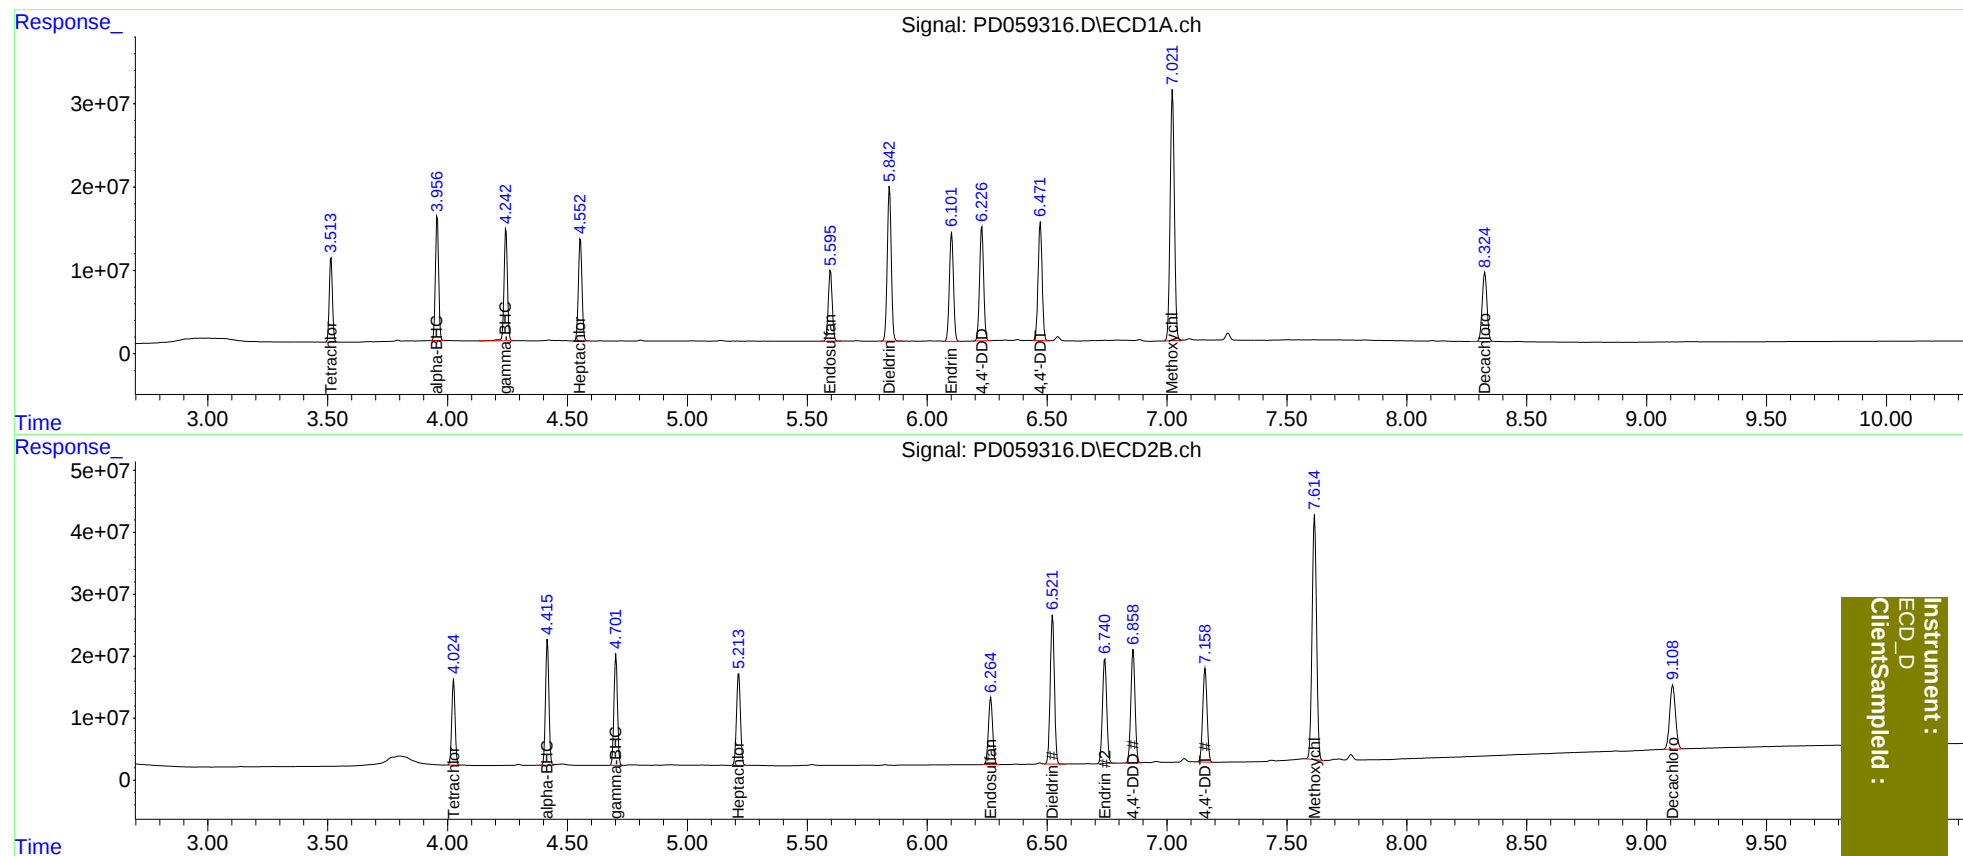


Instrument :
ECD_D
ClientSampled :

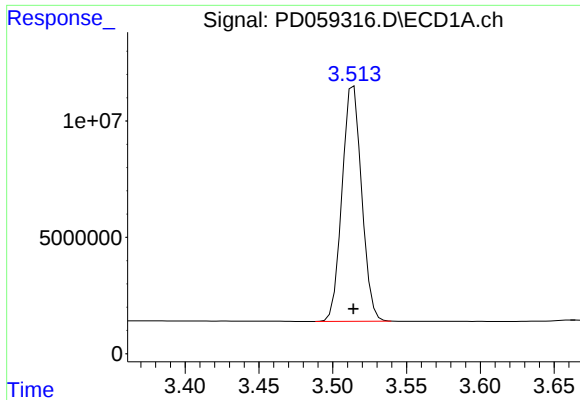

#1 Tetrachloro-m-xylene


R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 93376239
Conc: 72.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

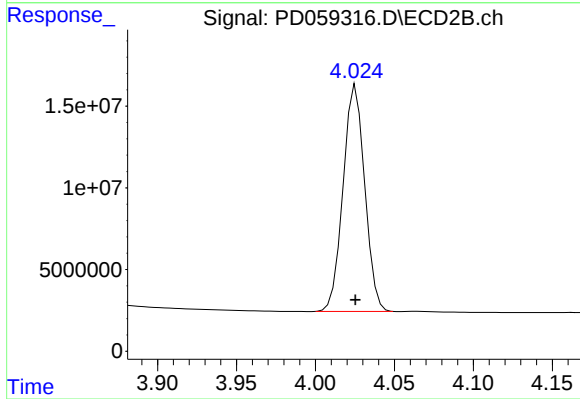


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 132479770
Conc: 76.49 ng/ml

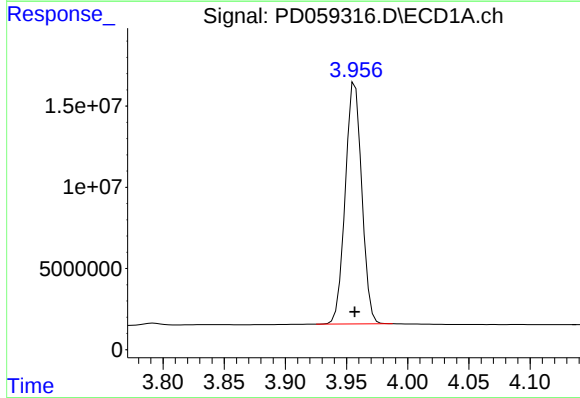


#2 alpha-BHC

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 139758915
Conc: 77.41 ng/ml

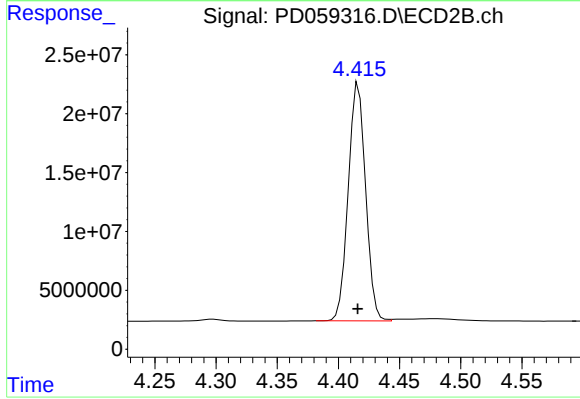

#2 alpha-BHC


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 199491841
Conc: 80.42 ng/ml

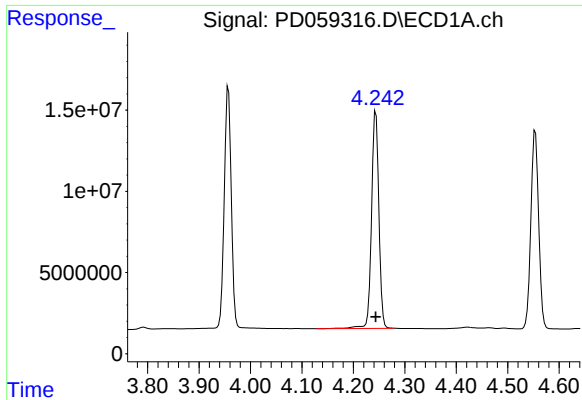

#3 gamma-BHC (Lindane)


R.T.: 4.244 min
Delta R.T.: 0.000 min
Response: 132276910
Conc: 73.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

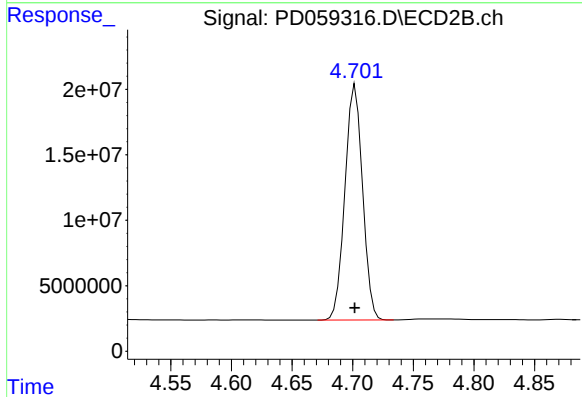


#3 gamma-BHC (Lindane)

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 181849650
Conc: 79.91 ng/ml

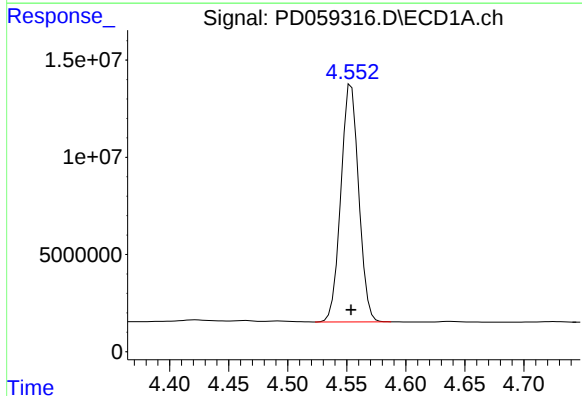


#4 Heptachlor

R.T.: 4.554 min
Delta R.T.: 0.000 min
Response: 128351868
Conc: 75.44 ng/ml

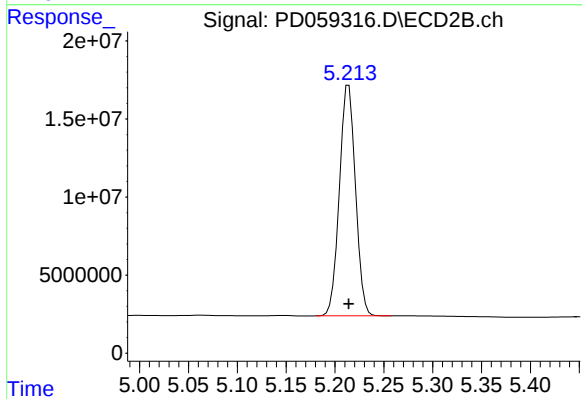

#4 Heptachlor


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 169383757
Conc: 78.27 ng/ml

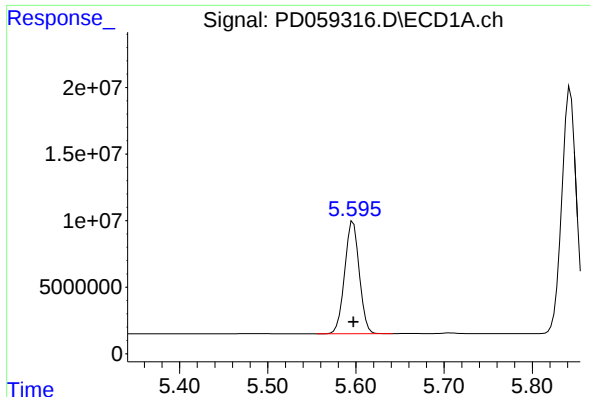

#9 Endosulfan I


R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 97010182
Conc: 73.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

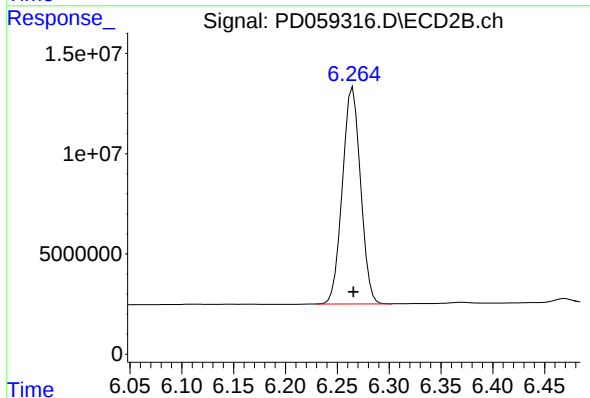


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 131576846
Conc: 77.70 ng/ml

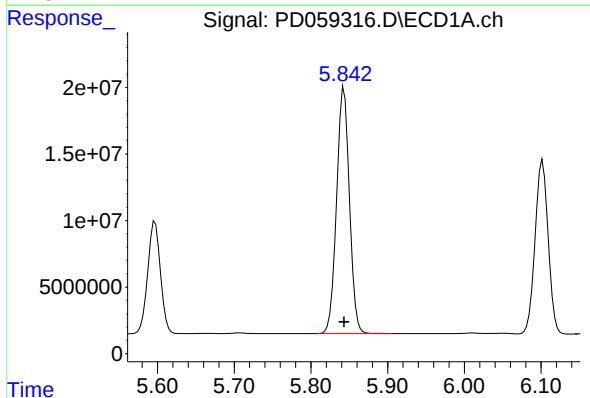


#13 Dieldrin

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 214838952
Conc: 154.67 ng/ml

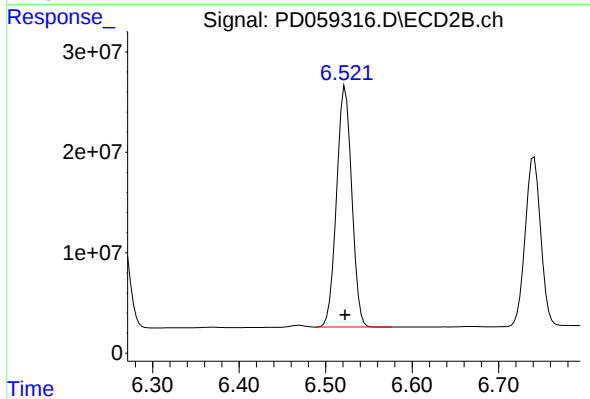

#13 Dieldrin


R.T.: 6.523 min
Delta R.T.: 0.000 min
Response: 290796411
Conc: 161.35 ng/ml

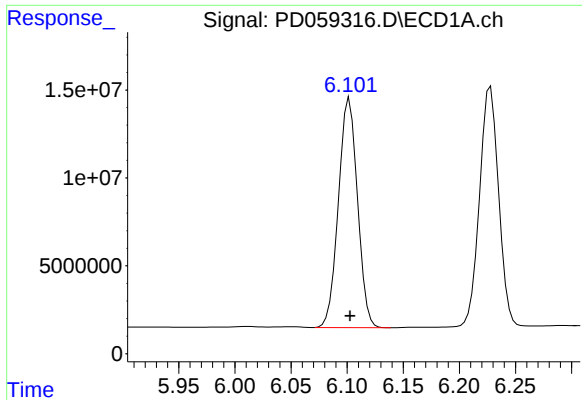

#14 Endrin


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 154496156
Conc: 152.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

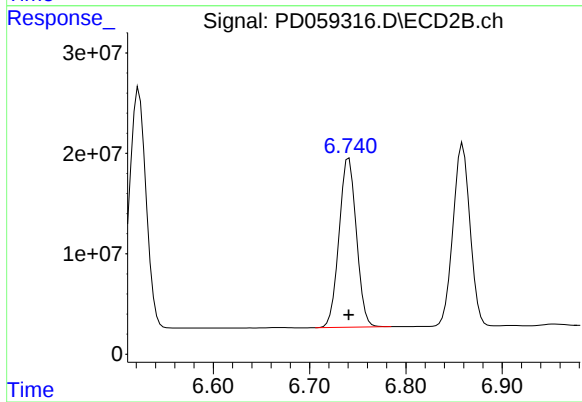


#14 Endrin

R.T.: 6.741 min
Delta R.T.: 0.000 min
Response: 210126195
Conc: 163.17 ng/ml

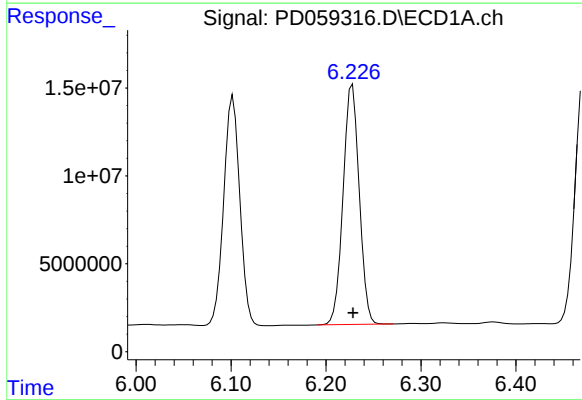


#16 4,4'-DDD

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 161327573
Conc: 151.34 ng/ml

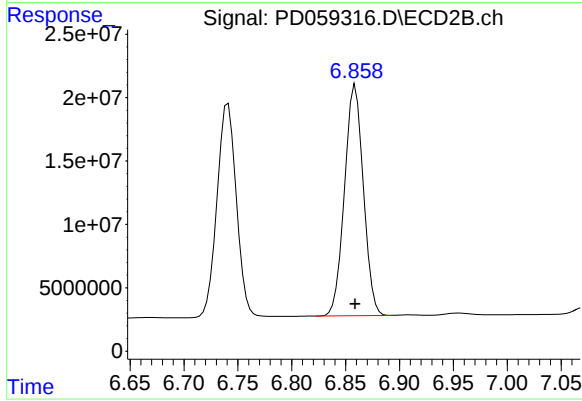

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 222044025
Conc: 161.64 ng/ml

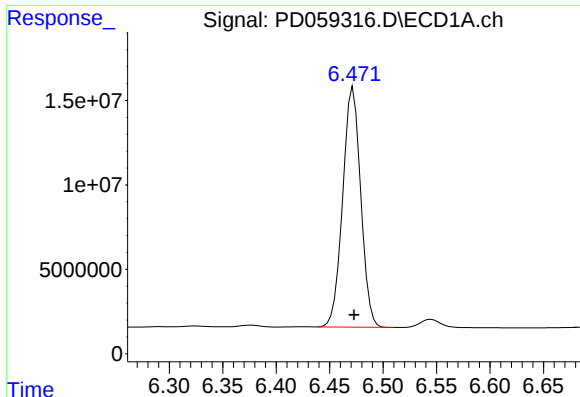

#17 4,4'-DDT


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 166788854
Conc: 154.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

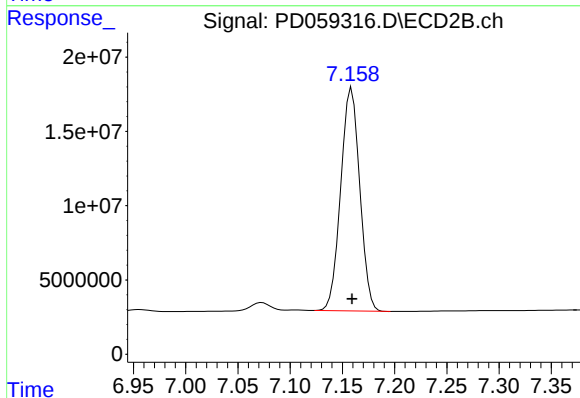


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 190250789
Conc: 170.45 ng/ml

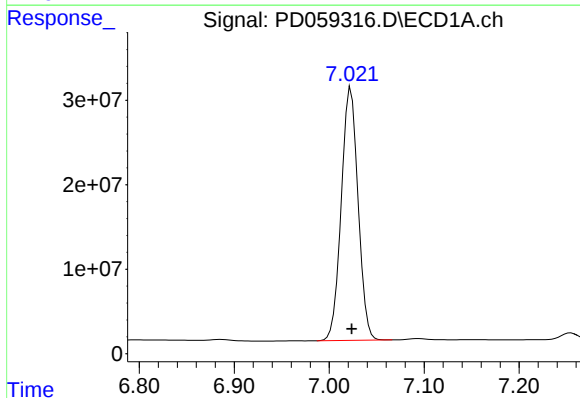


#20 Methoxychlor

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 368457489
Conc: 732.93 ng/ml

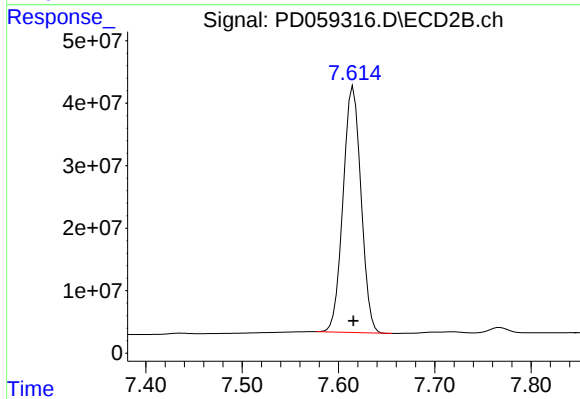

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 508346566
Conc: 814.91 ng/ml

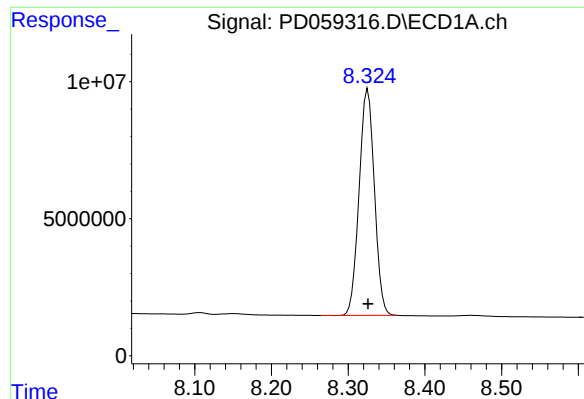

#27 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 114719375
Conc: 134.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

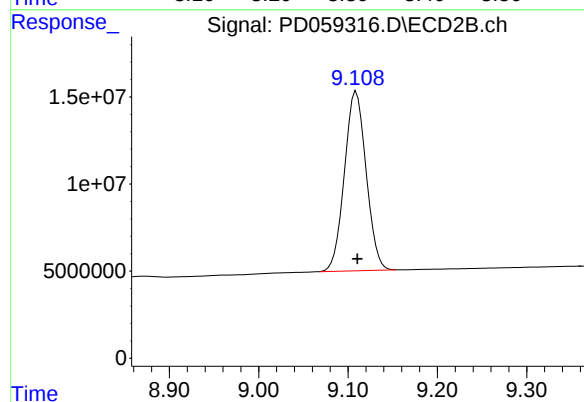

#27 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.001 min
Response: 173908515
Conc: 149.91 ng/ml