

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
 Data File : PD059301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 20:21
 Operator : DD\AJ
 Sample : RESC55
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC55

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 05:16:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.514	4.025	22548372	30623061	17.976	18.199
2)	SA Decachlor...	8.327	9.110	29601975	40997063	35.079	36.014
Target Compounds							
2)	A alpha-BHC	3.956	4.416	16416139	21486588	9.306	8.776
3)	MA gamma-BHC...	4.244	4.702	17501017	19839630	10.373	8.869
4)	MA Heptachlor	4.554	5.214	15825716	19135539	9.556	8.835
5)	MB Aldrin	4.807	5.520	14558225	17369219	9.007	8.594
6)	B beta-BHC	4.493	4.869	7096706	8583827	9.196	8.489
7)	B delta-BHC	4.703	5.088	13413561	17405062	8.114	7.653
8)	B Heptachlo...	5.254	5.907	12958445	16209439	9.061	8.614
9)	A Endosulfan I	5.597	6.265	12302504	15000354	9.565	9.049
10)	B trans-Chl...	5.484	6.141	12680809	15565466	8.977	8.540
11)	B cis-Chlor...	5.543	6.214	12632818	15346044	8.972	8.500
12)	B 4,4'-DDE	5.709	6.369	23580935	28575547	17.706	16.732
13)	MA Dieldrin	5.844	6.522	25188052	31389305	18.690	17.679
14)	MA Endrin	6.103	6.741	19580261	23794472	19.826	18.554
15)	B Endosulfa...	6.377	6.948	19172346	24064725	17.845	16.867
16)	A 4,4'-DDD	6.229	6.859	19924883	23639032	19.175	17.508
17)	MA 4,4'-DDT	6.473	7.159	19965402	18805673	18.963	16.921
18)	B Endrin al...	6.547	7.073	16352246	20509311	18.451	17.373
19)	B Endosulfa...	6.762	7.295	17466764	24076188	17.202	16.522
20)	A Methoxychlor	7.024	7.616	48605234	54112319	98.585	87.305
21)	B Endrin ke...	7.257	7.768	19635732	24413138	18.236	17.439

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 20:21
Operator : DD\AJ
Sample : RESC55
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 05:16:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

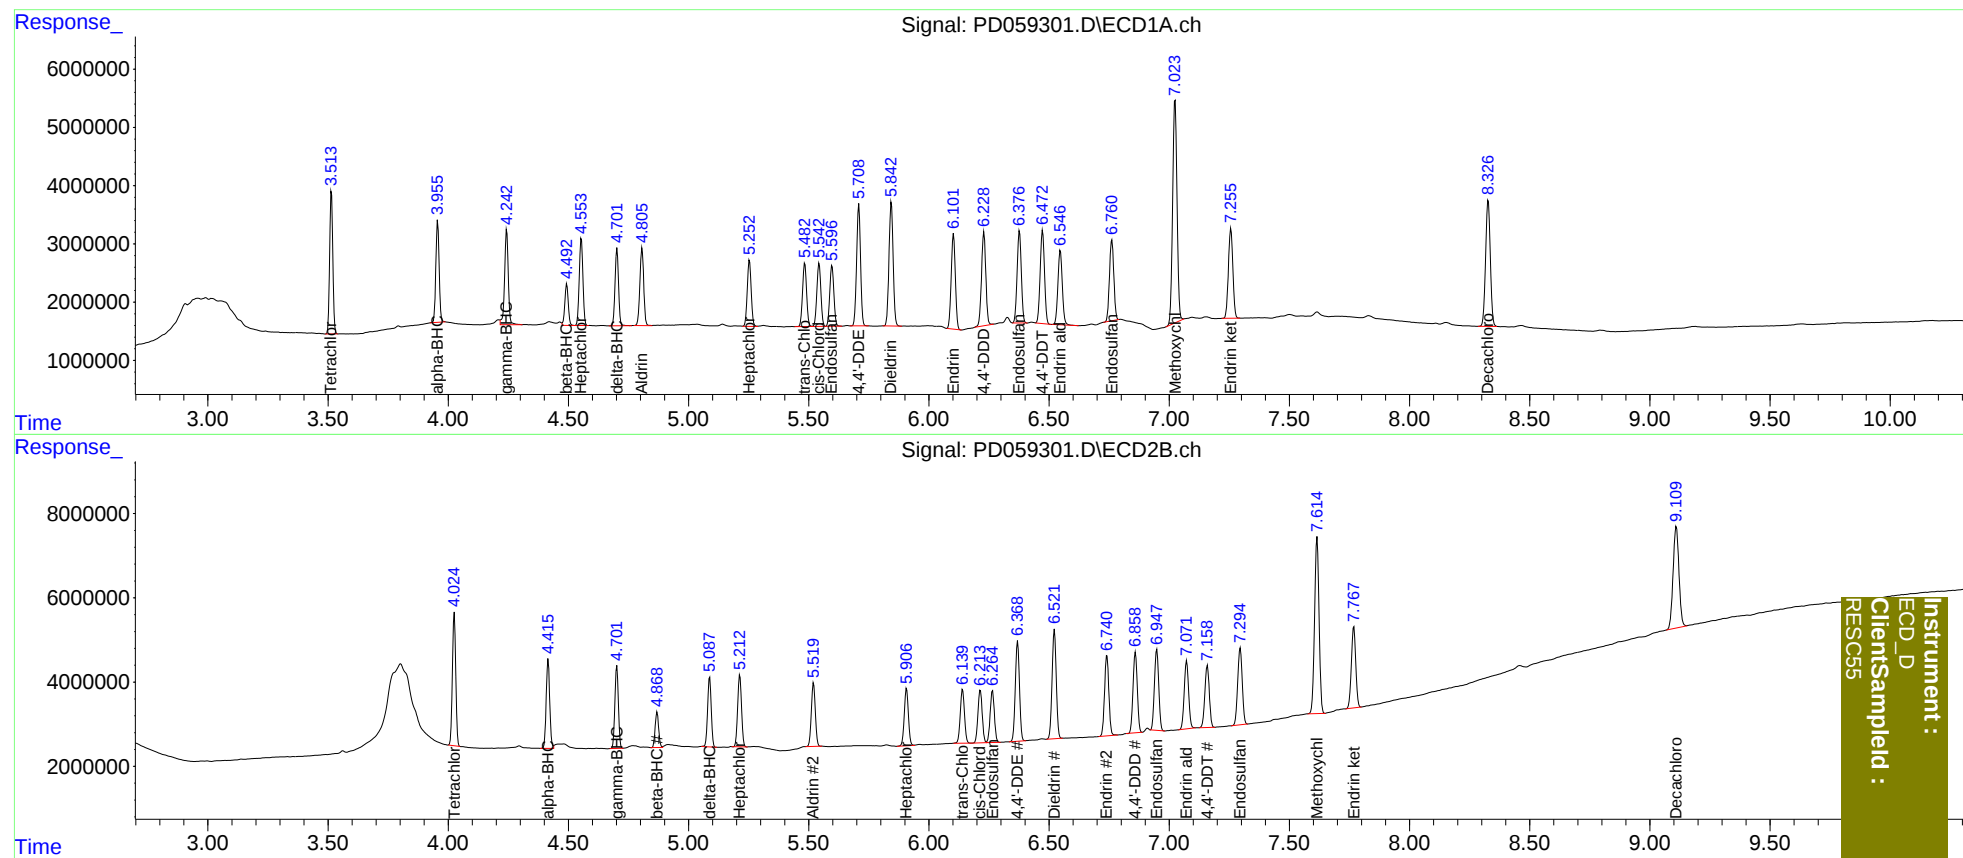

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092420\
Data File : PD059301.D
Acq On : 24 Sep 2020 20:21
Operator : DD\AJ
Sample : RESC55
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC55

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Title : GC Extractables
Last Update : Fri Sep 25 05:12:00 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.514	3.956	100.00%
3.956	4.244	100.00%
4.244	4.493	100.00%
4.493	4.554	100.00%
4.554	4.703	100.00%
4.703	4.807	100.00%
4.807	5.254	100.00%
5.254	5.484	100.00%
5.484	5.543	100.00%
5.543	5.597	100.00%
5.597	5.709	100.00%
5.709	5.844	100.00%
5.844	6.103	100.00%
6.103	6.229	100.00%
6.229	6.377	100.00%
6.377	6.473	100.00%
6.473	6.547	100.00%
6.547	6.762	100.00%
6.762	7.025	100.00%
7.025	7.257	100.00%
7.257	8.327	100.00%

Signal #2

4.025	4.416	100.00%
4.416	4.702	100.00%
4.702	4.869	100.00%
4.869	5.088	100.00%
5.088	5.214	100.00%
5.214	5.520	100.00%
5.520	5.907	100.00%
5.907	6.141	100.00%
6.141	6.214	100.00%
6.214	6.265	99.39%
6.265	6.369	100.00%
6.369	6.522	100.00%
6.522	6.741	100.00%
6.741	6.859	100.00%
6.859	6.948	100.00%
6.948	7.073	100.00%
7.073	7.159	100.00%
7.159	7.295	100.00%
7.295	7.616	100.00%
7.616	7.768	100.00%
7.768	9.110	100.00%

