

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 15:02
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:14:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:11:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.563	13083826	163.9E6	5.135	5.207
27)	SA Decachlor...	7.993	9.089	25466589	102.9E6	11.101	11.529
Target Compounds							
2)	A alpha-BHC	3.312	4.029	17554563	232.2E6	4.702	5.425
3)	MA gamma-BHC...	3.645	4.364	17095755	198.1E6	4.880	5.581
4)	MA Heptachlor	3.991	4.941	17474215	143.6E6	4.912	5.654
9)	A Endosulfan I	5.155	6.103	14505707	84734323	5.177	5.646
13)	MA Dieldrin	5.422	6.381	29758203	166.2E6	9.625	10.964
14)	MA Endrin	5.699	6.614	26201265	141.0E6	9.815	11.470
16)	A 4,4'-DDD	5.847	6.745	22483954	127.0E6	9.546	10.968
17)	MA 4,4'-DDT	6.101	7.056	22361386	121.4E6	9.234	10.606
20)	A Methoxychlor	6.681	7.534	68422246	295.4E6	52.956	56.565


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 15:02
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:14:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:11:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

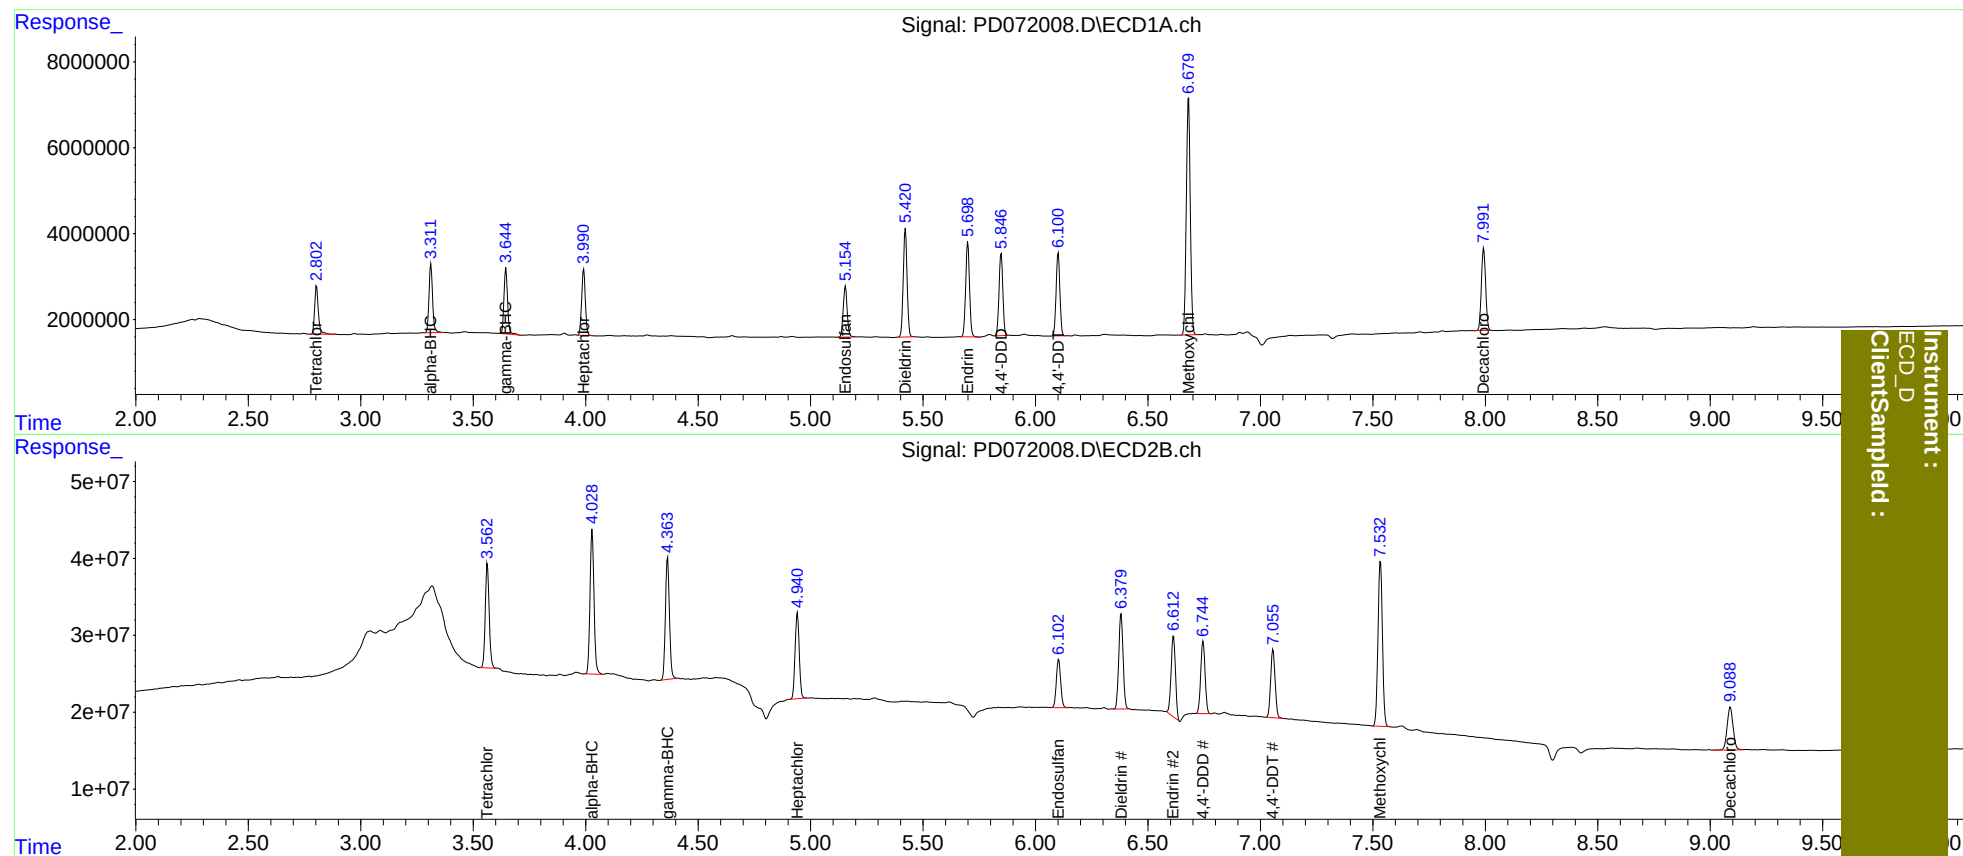


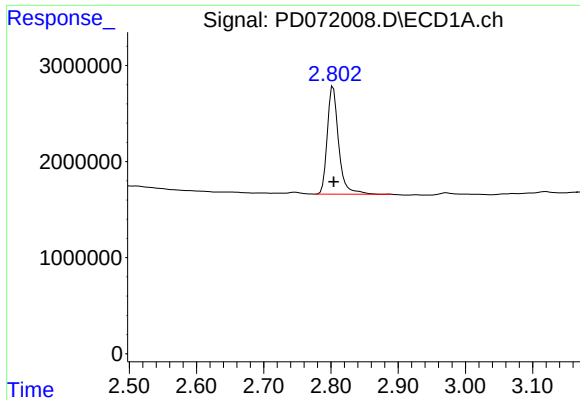

#1 Tetrachloro-m-xylene


R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 13083826
Conc: 5.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

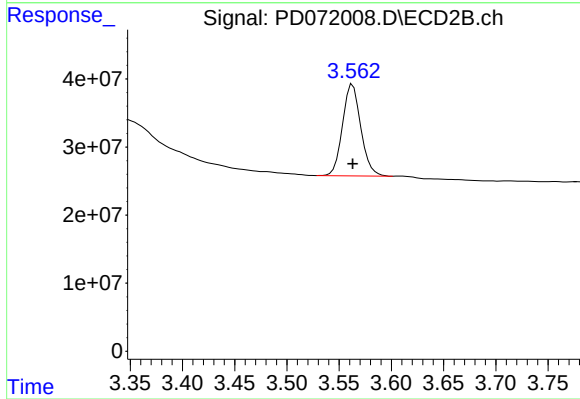


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 163889836
Conc: 5.21 ng/ml

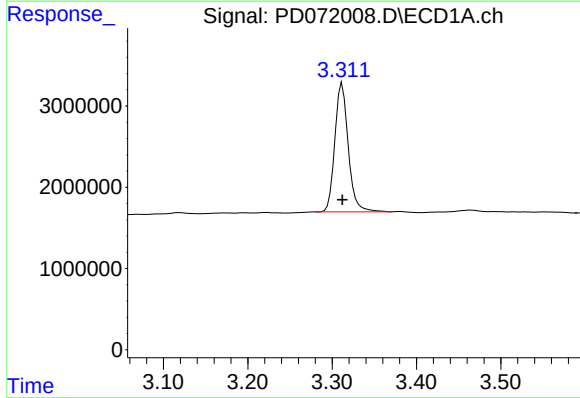


#2 alpha-BHC

R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 17554563
Conc: 4.70 ng/ml

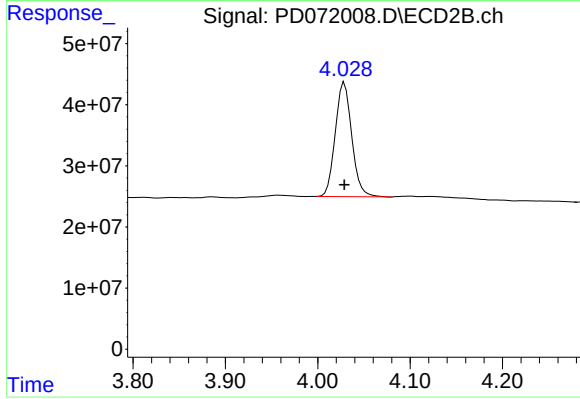

#2 alpha-BHC


R.T.: 4.029 min
Delta R.T.: 0.000 min
Response: 232241895
Conc: 5.42 ng/ml

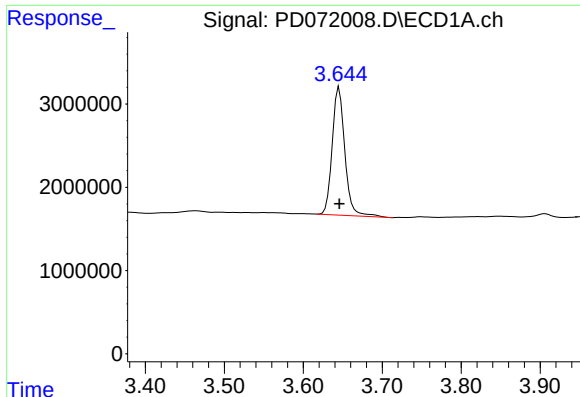

#3 gamma-BHC (Lindane)


R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 17095755
Conc: 4.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

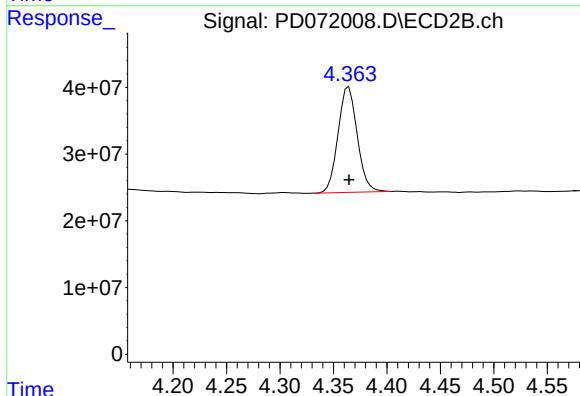


#3 gamma-BHC (Lindane)

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 198146048
Conc: 5.58 ng/ml

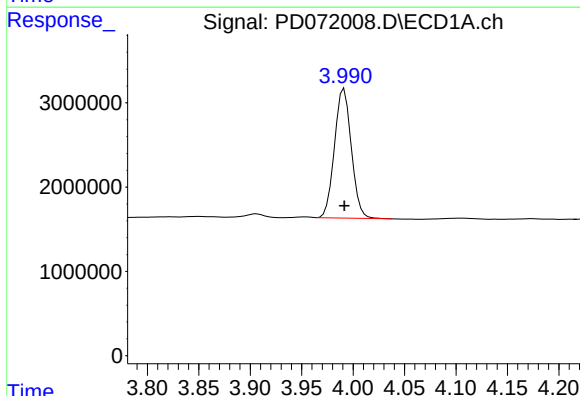


#4 Heptachlor

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 17474215
Conc: 4.91 ng/ml

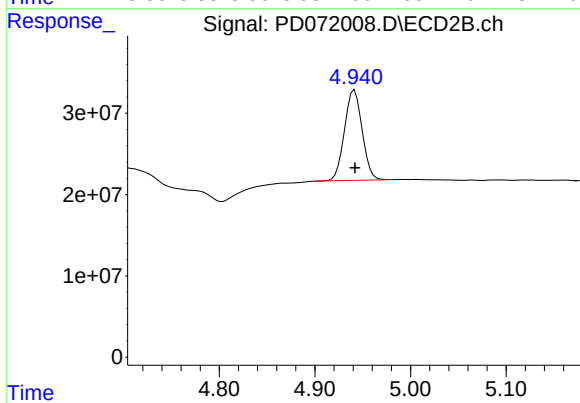

#4 Heptachlor


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 143590790
Conc: 5.65 ng/ml

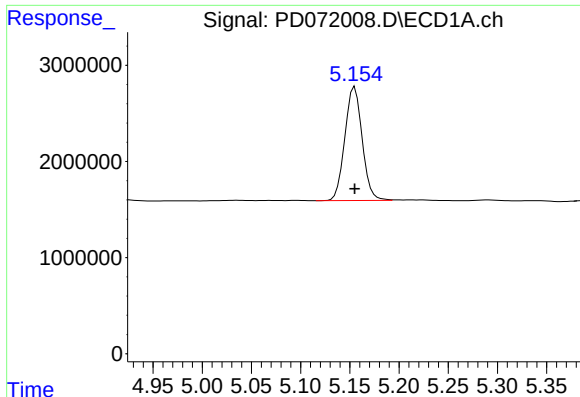

#9 Endosulfan I


R.T.: 5.155 min
Delta R.T.: 0.000 min
Response: 14505707
Conc: 5.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

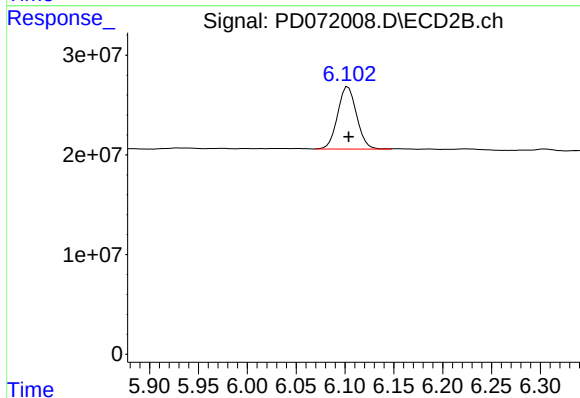


#9 Endosulfan I

R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 84734323
Conc: 5.65 ng/ml

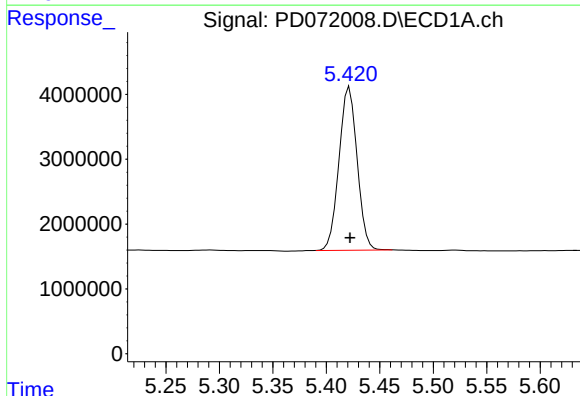


#13 Dieldrin

R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 29758203
Conc: 9.62 ng/ml

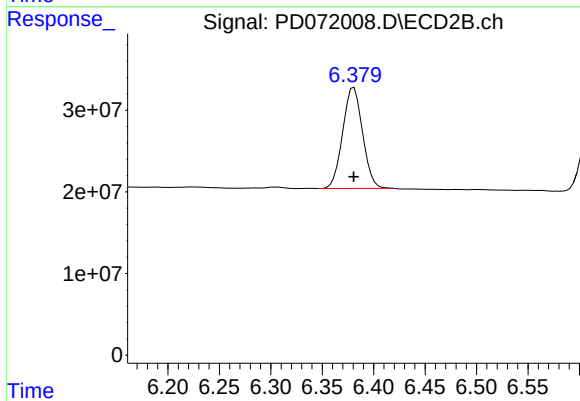

#13 Dieldrin


R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 166239415
Conc: 10.96 ng/ml

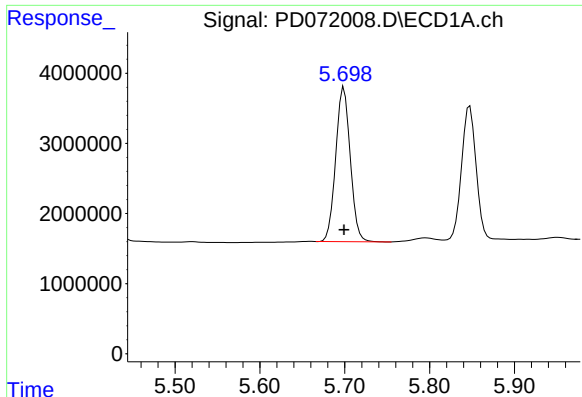

#14 Endrin


R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 26201265
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

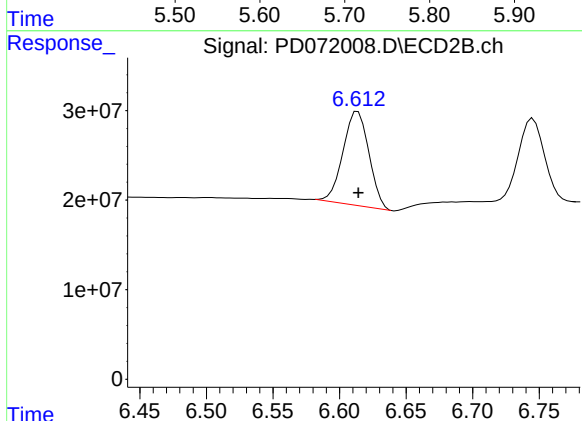


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 141002731
Conc: 11.47 ng/ml

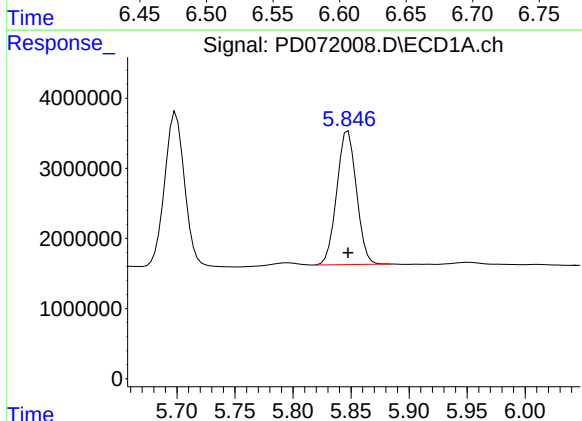


#16 4,4'-DDD

R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 22483954
Conc: 9.55 ng/ml

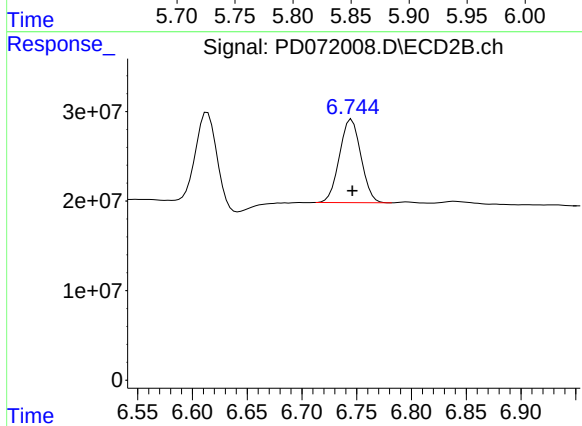

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 127045065
Conc: 10.97 ng/ml

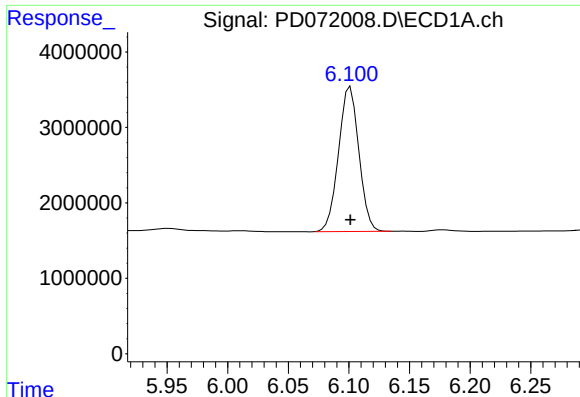

#17 4,4'-DDT


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 22361386
Conc: 9.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

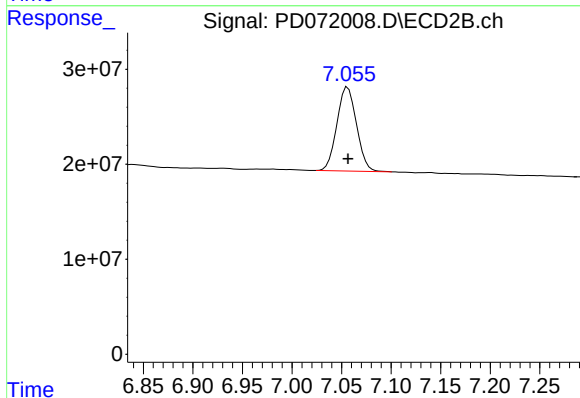


#17 4,4'-DDT

R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 121445055
Conc: 10.61 ng/ml

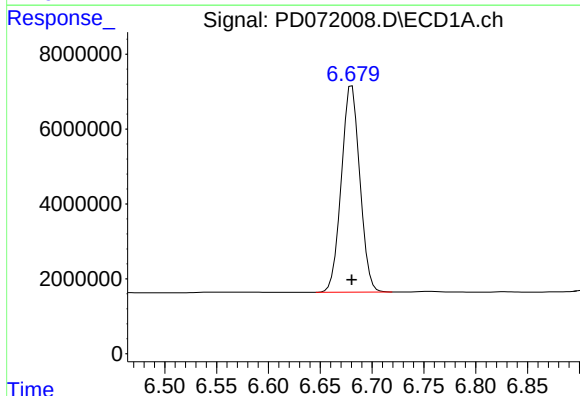


#20 Methoxychlor

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 68422246
Conc: 52.96 ng/ml

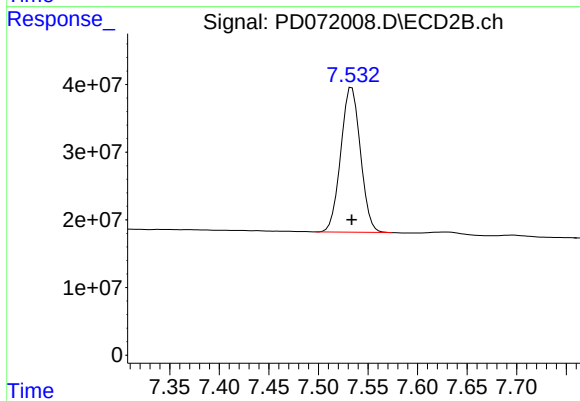

#20 Methoxychlor


R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 295437457
Conc: 56.56 ng/ml

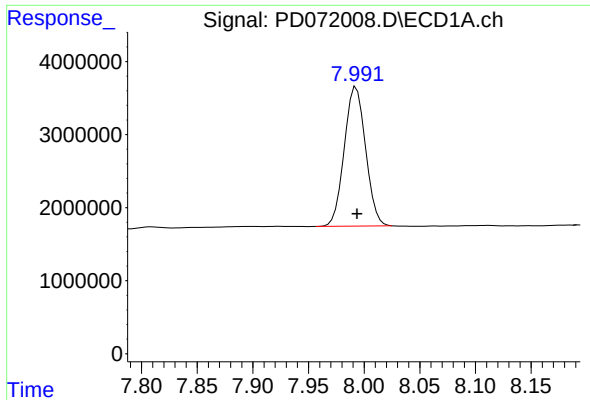

#27 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 25466589
Conc: 11.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

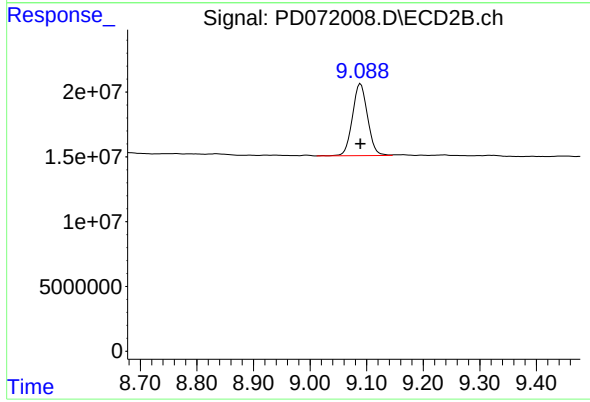

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 102884259
Conc: 11.53 ng/ml