

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 15:28
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:17:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:11:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.563	26278037	333.2E6	10.314	10.588
27)	SA Decachlor...	7.993	9.090	48983289	194.2E6	21.352	21.760
Target Compounds							
2)	A alpha-BHC	3.313	4.029	36632399	455.0E6	9.813	10.627
3)	MA gamma-BHC...	3.646	4.365	34721849	381.5E6	9.912	10.746
4)	MA Heptachlor	3.992	4.942	35656728	276.2E6	10.022	10.877
9)	A Endosulfan I	5.155	6.104	28683523	161.2E6	10.238	10.744
13)	MA Dieldrin	5.423	6.381	60901863	322.6E6	19.698	21.274
14)	MA Endrin	5.700	6.614	52961194	264.0E6	19.839	21.478
16)	A 4,4'-DDD	5.848	6.746	46429693	244.8E6	19.714	21.137
17)	MA 4,4'-DDT	6.102	7.057	46993077	239.5E6	19.405	20.920
20)	A Methoxychlor	6.681	7.534	134.1E6	562.5E6	103.821	107.704


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 15:28
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:17:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:11:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

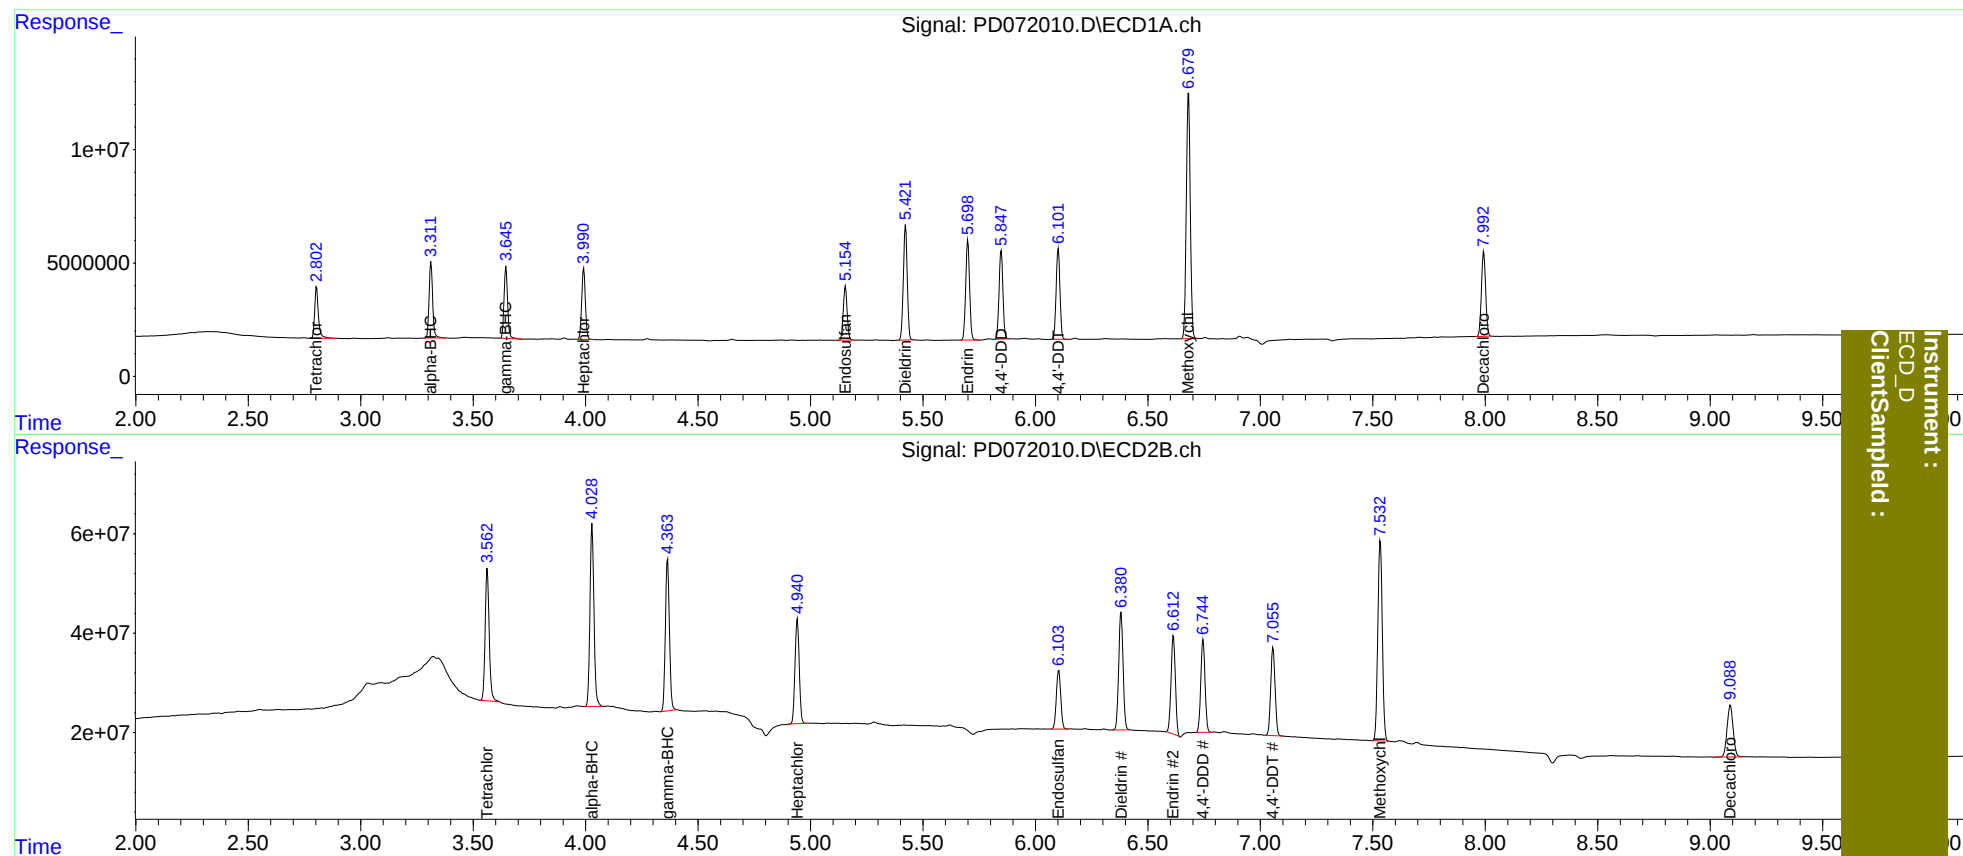


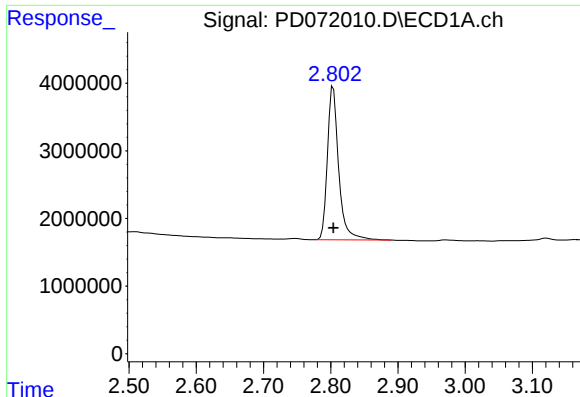

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 26278037
Conc: 10.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

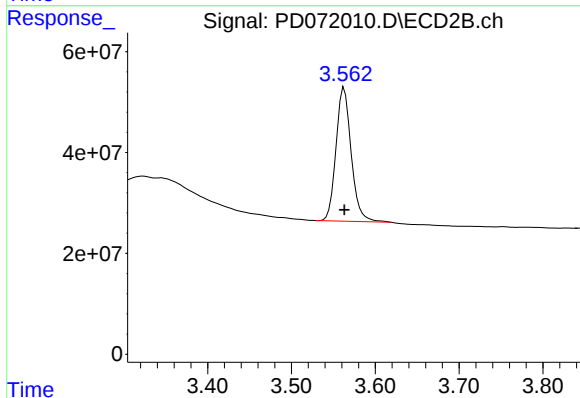


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 333242985
Conc: 10.59 ng/ml

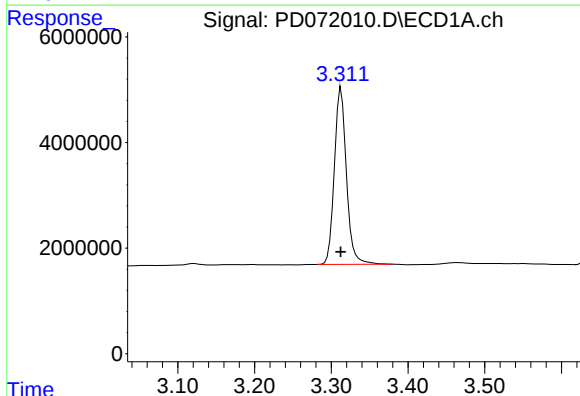


#2 alpha-BHC

R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 36632399
Conc: 9.81 ng/ml

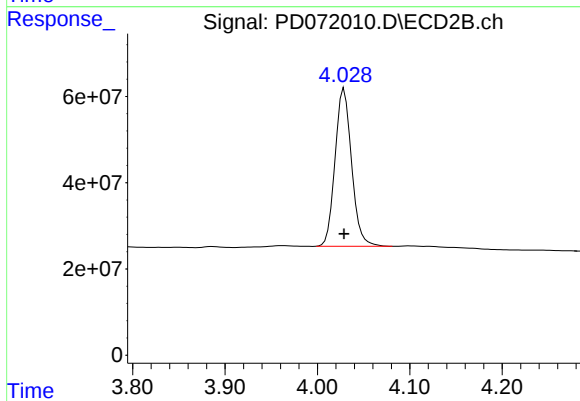

#2 alpha-BHC


R.T.: 4.029 min
Delta R.T.: 0.000 min
Response: 454957119
Conc: 10.63 ng/ml

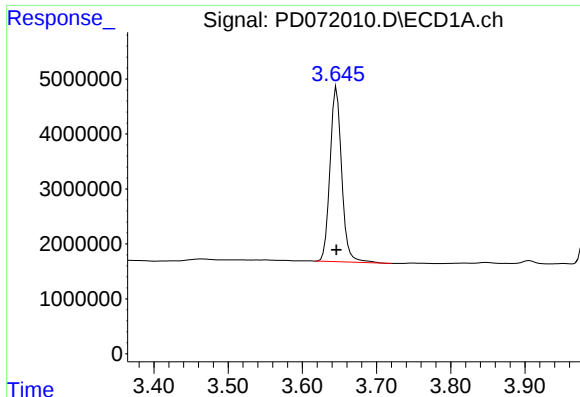

#3 gamma-BHC (Lindane)


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 34721849
Conc: 9.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

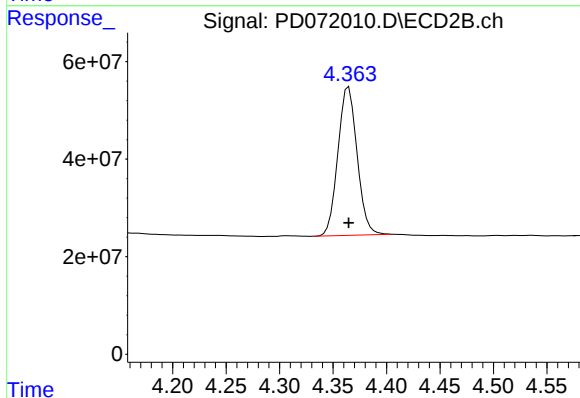


#3 gamma-BHC (Lindane)

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 381547077
Conc: 10.75 ng/ml

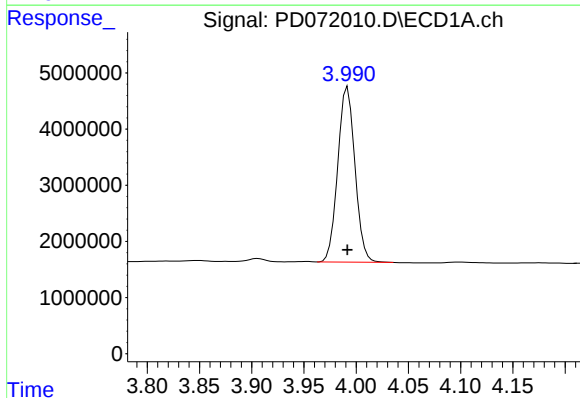


#4 Heptachlor

R.T.: 3.992 min
Delta R.T.: 0.000 min
Response: 35656728
Conc: 10.02 ng/ml

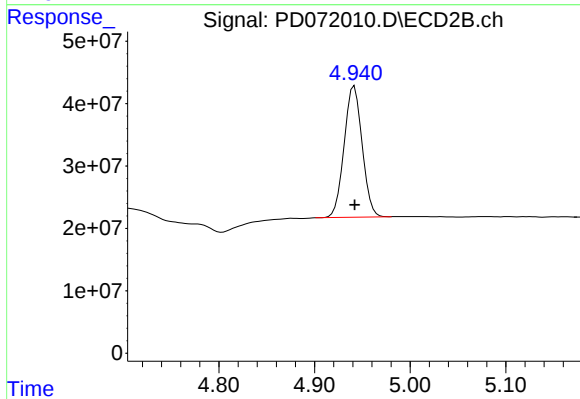

#4 Heptachlor


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 276226803
Conc: 10.88 ng/ml

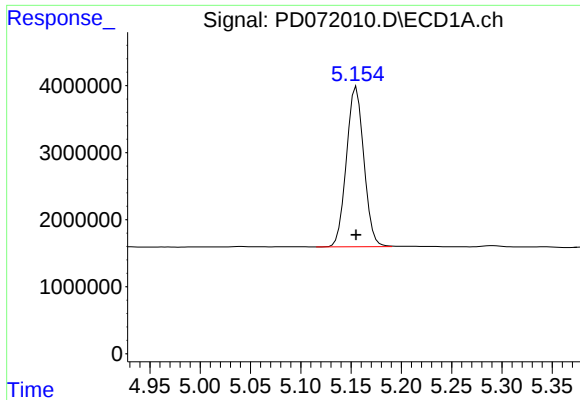

#9 Endosulfan I


R.T.: 5.155 min
Delta R.T.: 0.000 min
Response: 28683523
Conc: 10.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

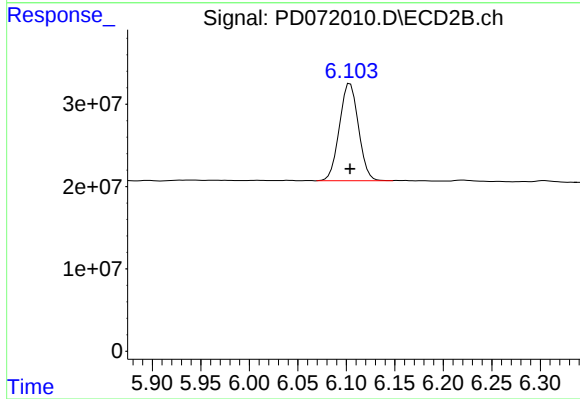


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 161229178
Conc: 10.74 ng/ml

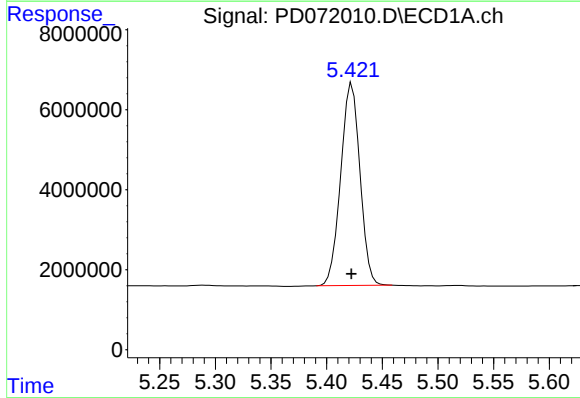


#13 Dieldrin

R.T.: 5.423 min
Delta R.T.: 0.000 min
Response: 60901863
Conc: 19.70 ng/ml

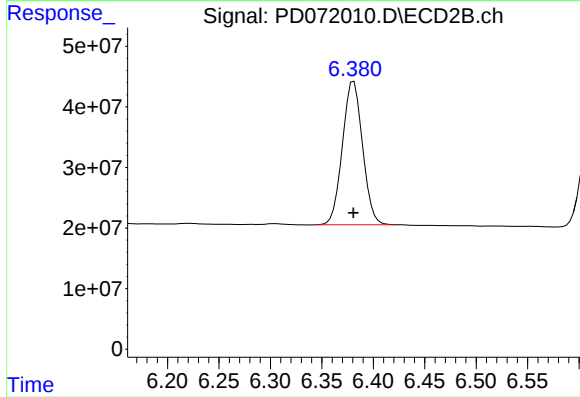

#13 Dieldrin


R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 322581033
Conc: 21.27 ng/ml

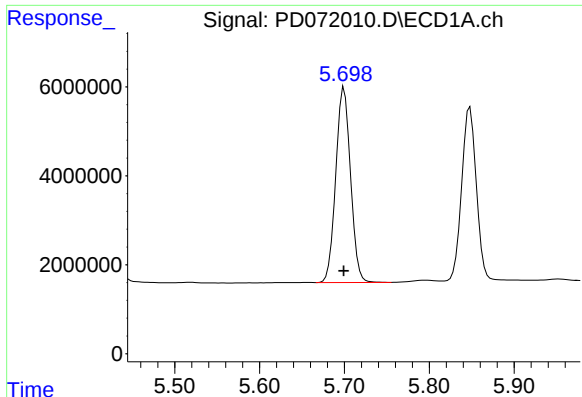

#14 Endrin


R.T.: 5.700 min
Delta R.T.: 0.000 min
Response: 52961194
Conc: 19.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

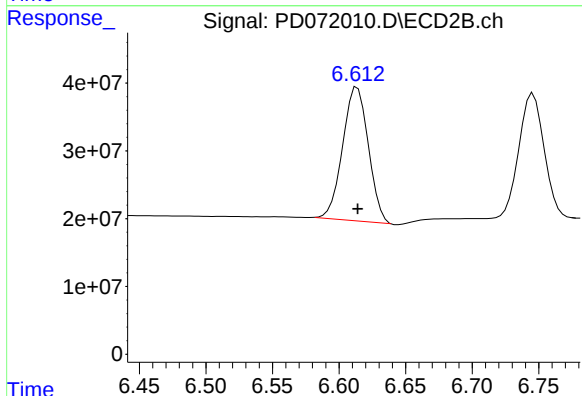


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 264046282
Conc: 21.48 ng/ml

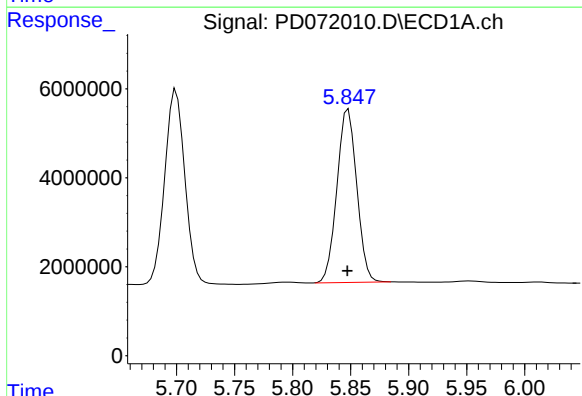


#16 4,4'-DDD

R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 46429693
Conc: 19.71 ng/ml

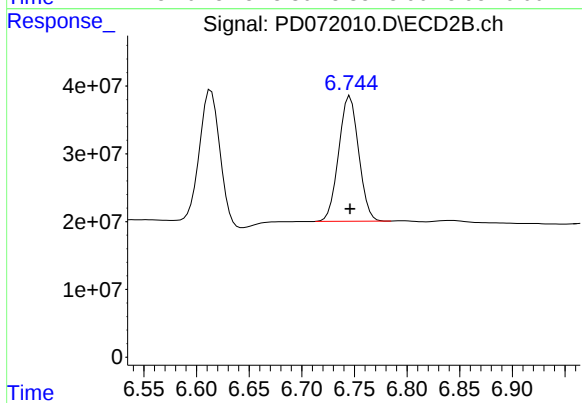

#16 4,4'-DDD


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 244826977
Conc: 21.14 ng/ml

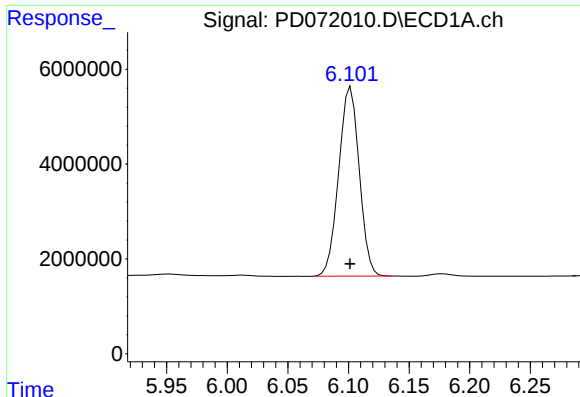

#17 4,4'-DDT


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 46993077
Conc: 19.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

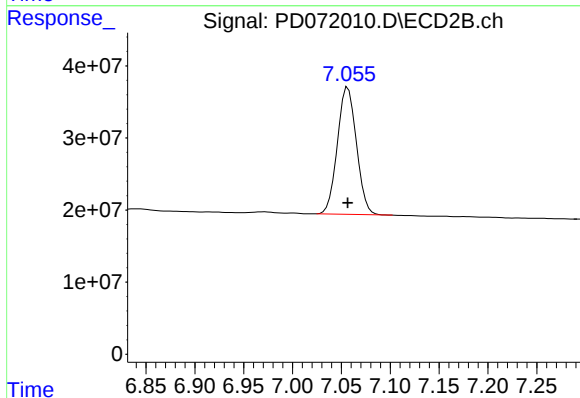


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 239536343
Conc: 20.92 ng/ml

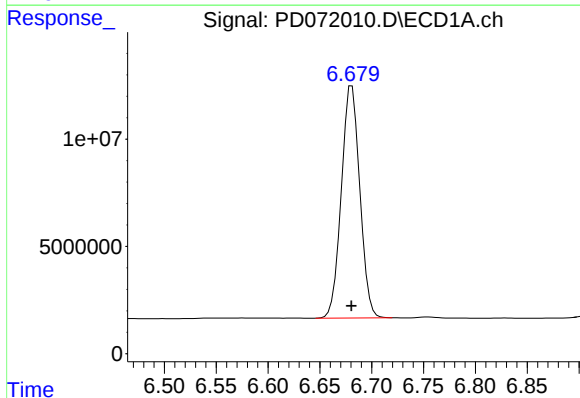


#20 Methoxychlor

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 134142441
Conc: 103.82 ng/ml

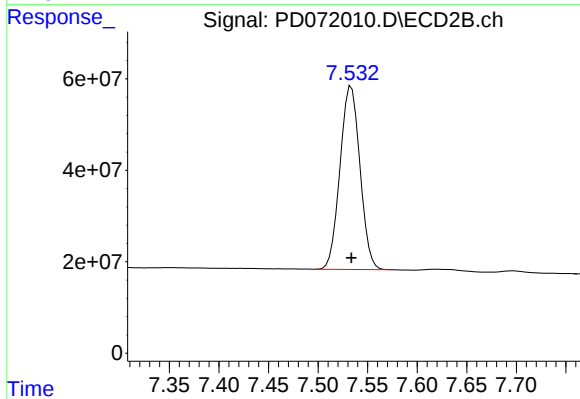

#20 Methoxychlor


R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 562538506
Conc: 107.70 ng/ml

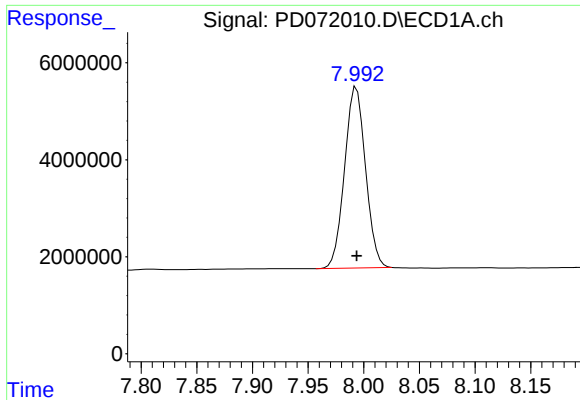

#27 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 48983289
Conc: 21.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

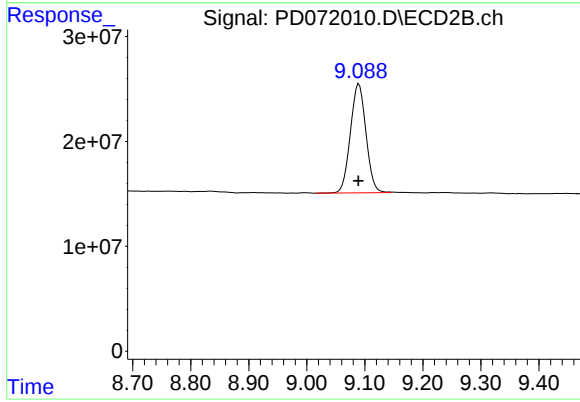

#27 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 194186454
Conc: 21.76 ng/ml