

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 15:55
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:21:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:21:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.563	50955738	629.5E6	20.000	20.000
27)	SA Decachlor...	7.994	9.089	92814658	357.0E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.312	4.029	74663584	856.2E6	20.000	20.000
3)	MA gamma-BHC...	3.646	4.365	70062271	710.1E6	20.000	20.000
4)	MA Heptachlor	3.992	4.942	71153582	507.9E6	20.000	20.000
9)	A Endosulfan I	5.155	6.104	56035227	300.1E6	20.000	20.000
13)	MA Dieldrin	5.422	6.381	123.7E6	606.5E6	40.000	40.000
14)	MA Endrin	5.699	6.614	106.8E6	491.7E6	40.000	40.000
16)	A 4,4'-DDD	5.847	6.746	94208168	463.3E6	40.000	40.000
17)	MA 4,4'-DDT	6.101	7.057	96866960	458.0E6	40.000	40.000
20)	A Methoxychlor	6.680	7.534	258.4E6	1044.6E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 15:55
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:21:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:21:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

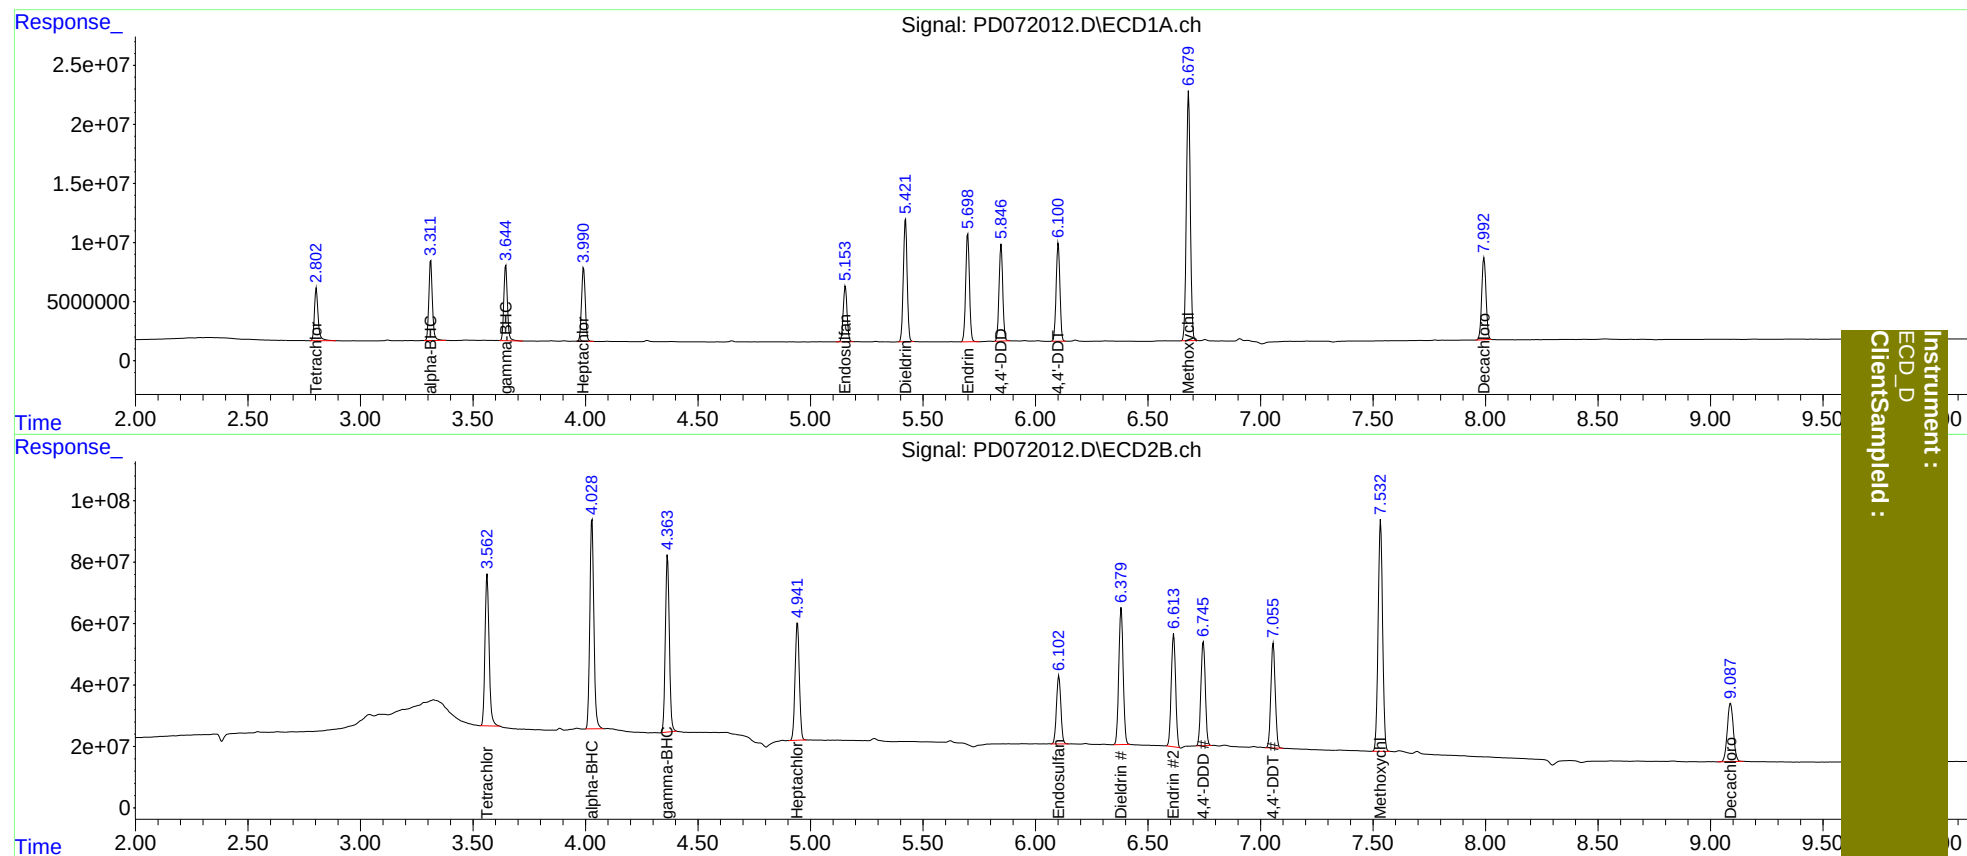


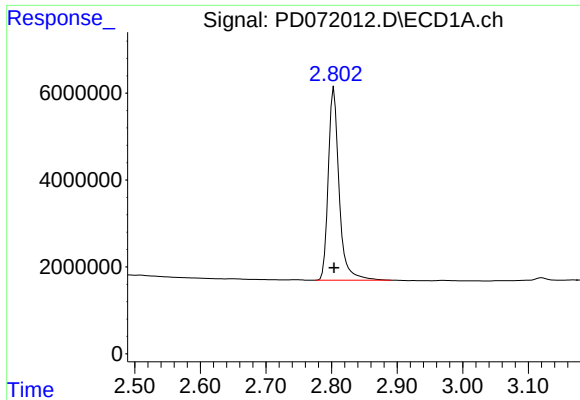

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 50955738
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

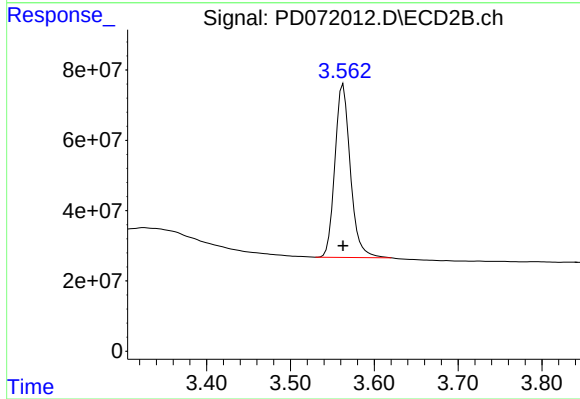


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 629455685
Conc: 20.00 ng/ml

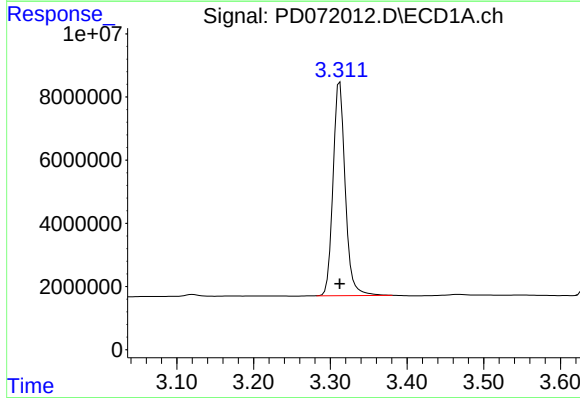


#2 alpha-BHC

R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 74663584
Conc: 20.00 ng/ml

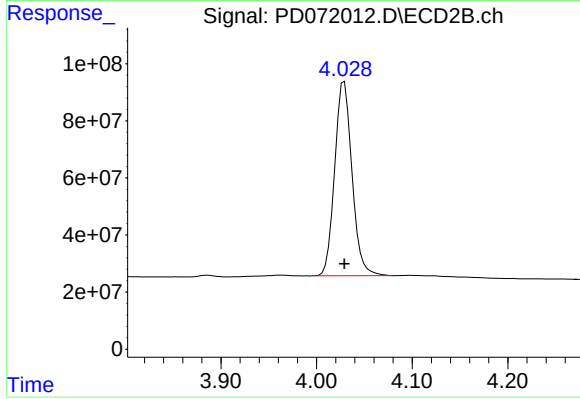

#2 alpha-BHC


R.T.: 4.029 min
Delta R.T.: 0.000 min
Response: 856223253
Conc: 20.00 ng/ml

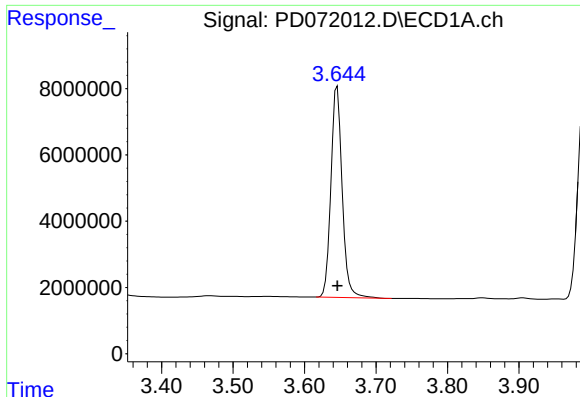

#3 gamma-BHC (Lindane)


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 70062271
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

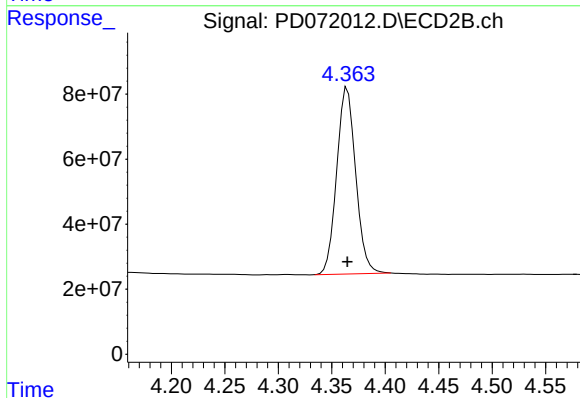


#3 gamma-BHC (Lindane)

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 710116131
Conc: 20.00 ng/ml

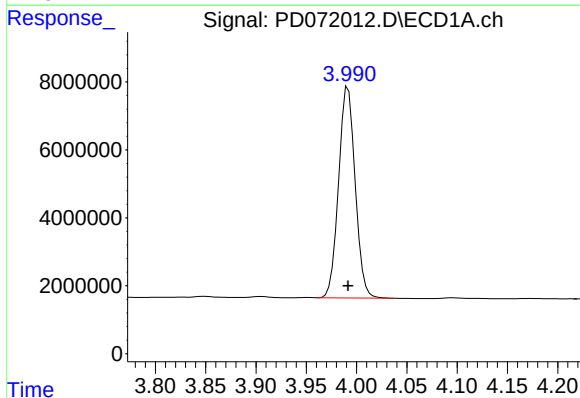


#4 Heptachlor

R.T.: 3.992 min
Delta R.T.: 0.000 min
Response: 71153582
Conc: 20.00 ng/ml

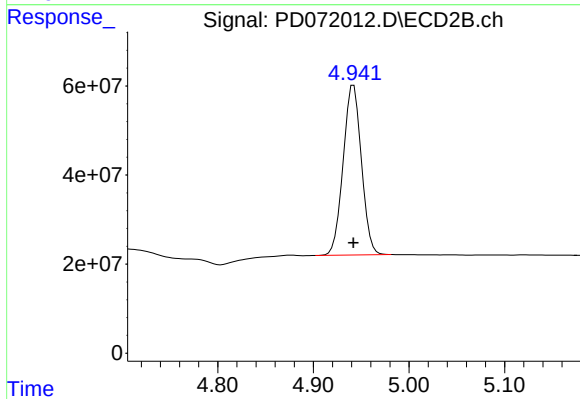

#4 Heptachlor


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 507931966
Conc: 20.00 ng/ml

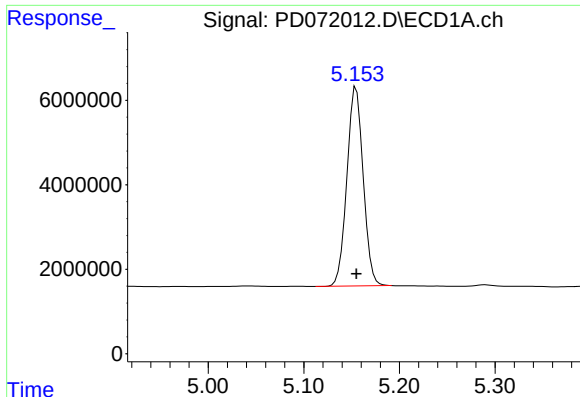

#9 Endosulfan I


R.T.: 5.155 min
Delta R.T.: 0.000 min
Response: 56035227
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

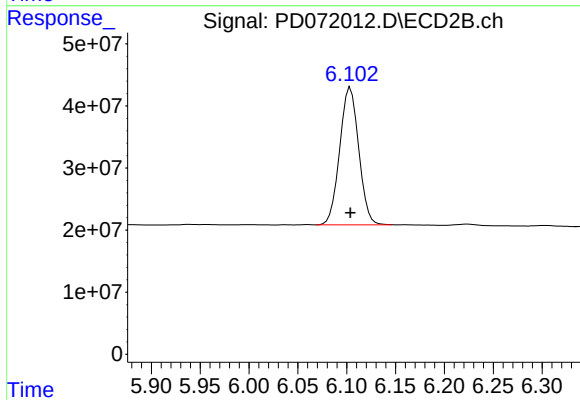


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 300134389
Conc: 20.00 ng/ml

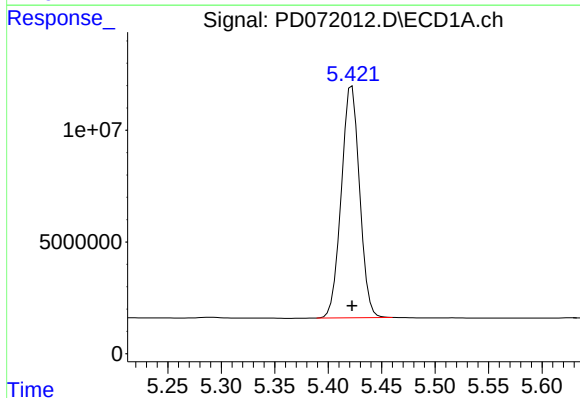


#13 Dieldrin

R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 123673730
Conc: 40.00 ng/ml

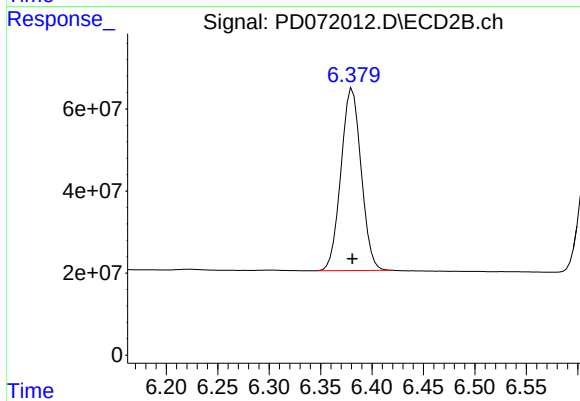

#13 Dieldrin


R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 606516717
Conc: 40.00 ng/ml

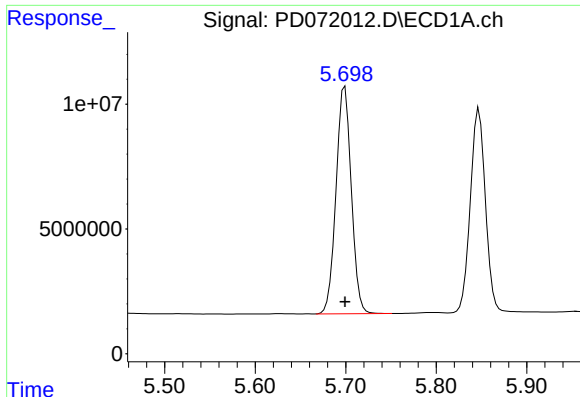

#14 Endrin


R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 106782609
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

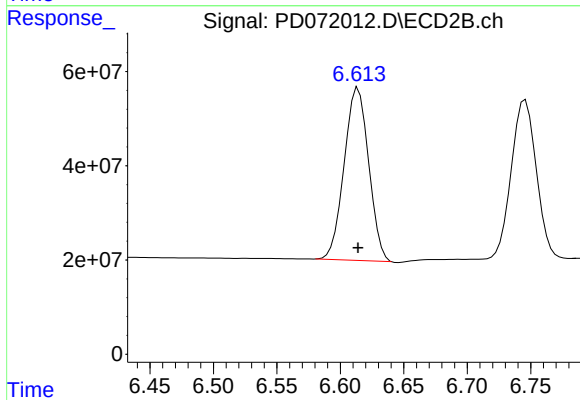


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 491742660
Conc: 40.00 ng/ml

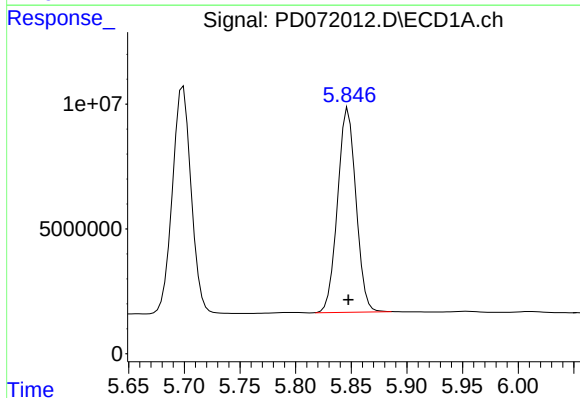


#16 4,4'-DDD

R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 94208168
Conc: 40.00 ng/ml

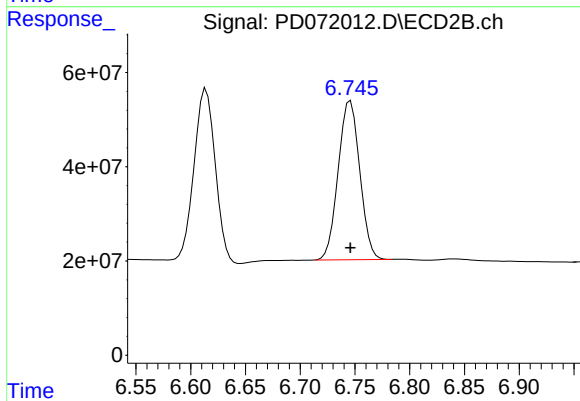

#16 4,4'-DDD


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 463324066
Conc: 40.00 ng/ml

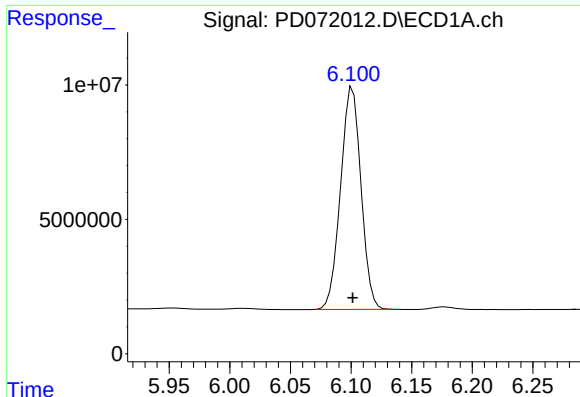

#17 4,4'-DDT


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 96866960
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

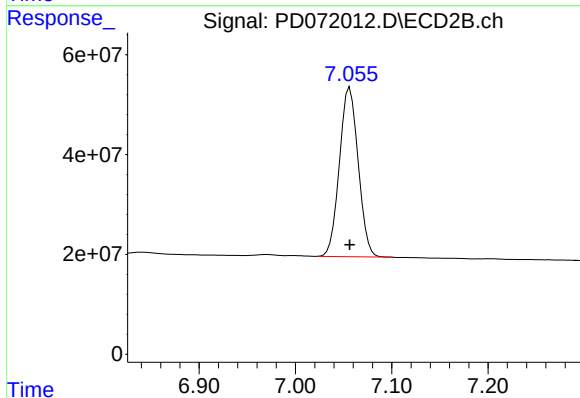


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 458015291
Conc: 40.00 ng/ml

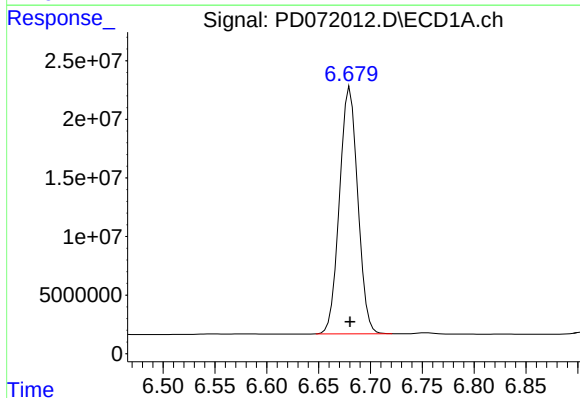


#20 Methoxychlor

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 258410165
Conc: 200.00 ng/ml

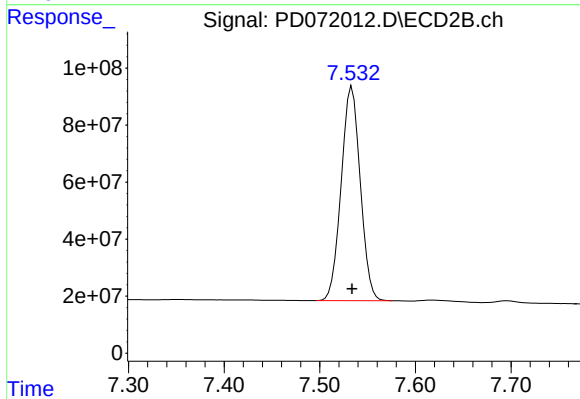

#20 Methoxychlor


R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 1044602731
Conc: 200.00 ng/ml

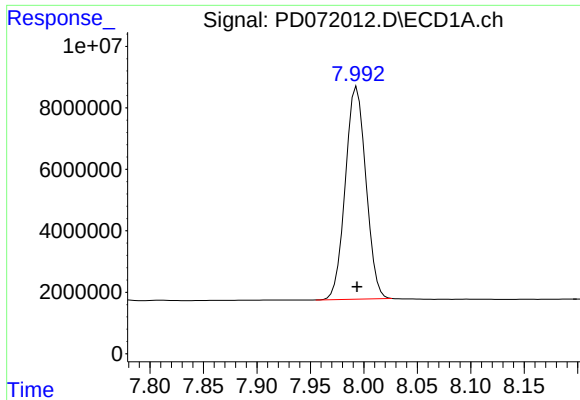

#27 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: 0.000 min
Response: 92814658
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

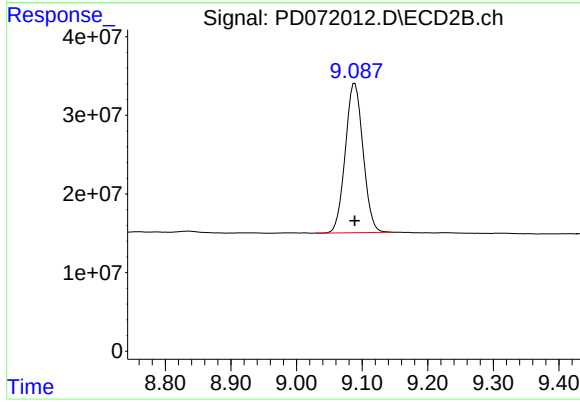

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 356957883
Conc: 40.00 ng/ml