

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 16:22
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:23:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:21:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.563	98770026	1147.2E6	38.767	36.451
27)	SA Decachlor...	7.993	9.089	177.3E6	658.4E6	76.408	73.780
Target Compounds							
2)	A alpha-BHC	3.312	4.029	150.3E6	1581.3E6	40.253	36.937
3)	MA gamma-BHC...	3.646	4.364	139.8E6	1301.8E6	39.913	36.665
4)	MA Heptachlor	3.991	4.942	141.5E6	915.0E6	39.780	36.029
9)	A Endosulfan I	5.155	6.104	109.6E6	547.5E6	39.127	36.481
13)	MA Dieldrin	5.422	6.381	248.0E6	1129.2E6	80.195	74.473
14)	MA Endrin	5.700	6.614	211.3E6	908.5E6	79.147	73.902
16)	A 4,4'-DDD	5.848	6.745	187.9E6	865.7E6	79.774	74.736
17)	MA 4,4'-DDT	6.101	7.057	196.5E6	868.5E6	81.150	75.846
20)	A Methoxychlor	6.681	7.533	495.1E6	1926.1E6	383.154	368.766


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 16:22
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:23:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:21:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

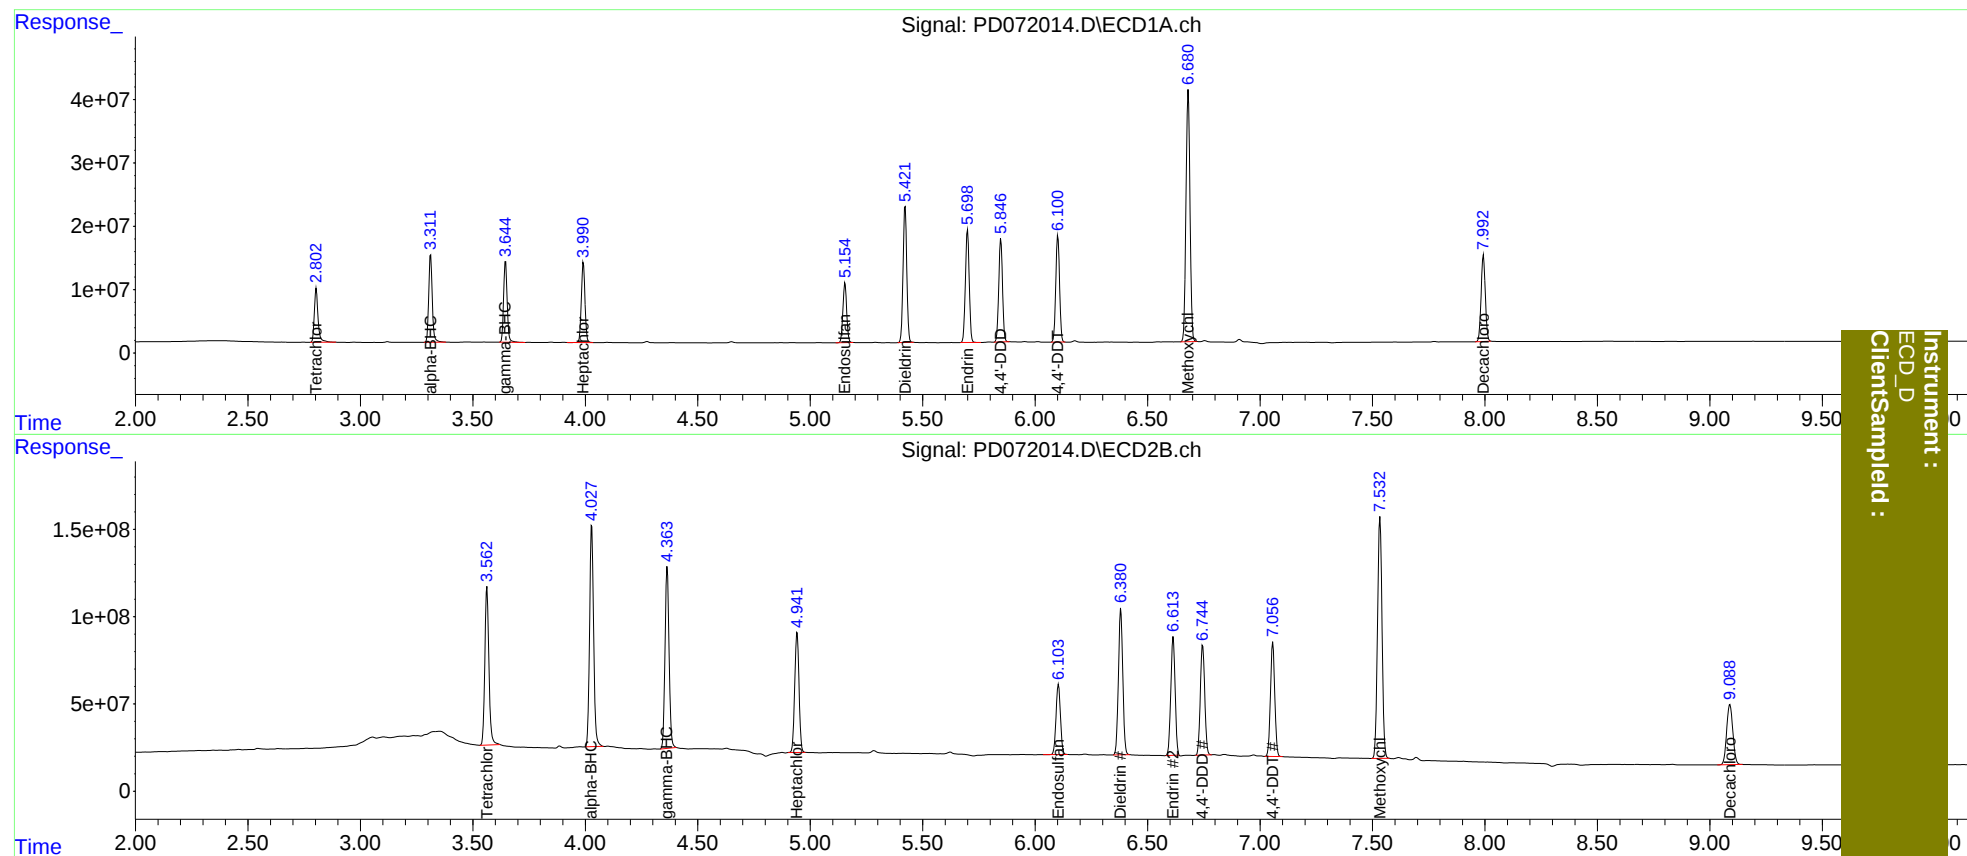


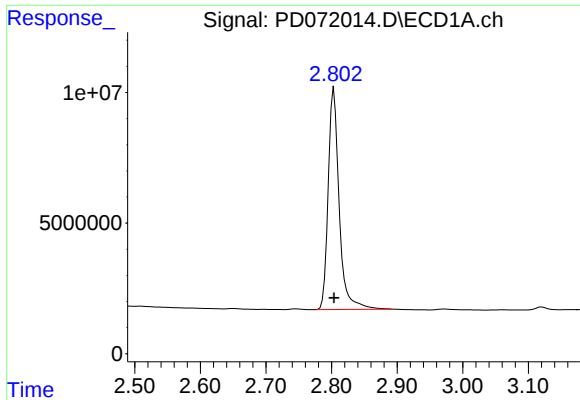

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 98770026
Conc: 38.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

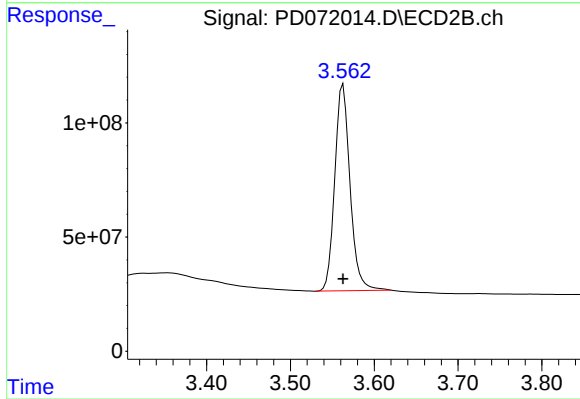


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 1147201489
Conc: 36.45 ng/ml

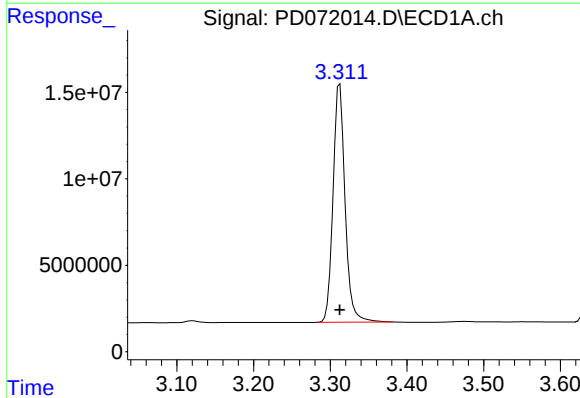


#2 alpha-BHC

R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 150269838
Conc: 40.25 ng/ml

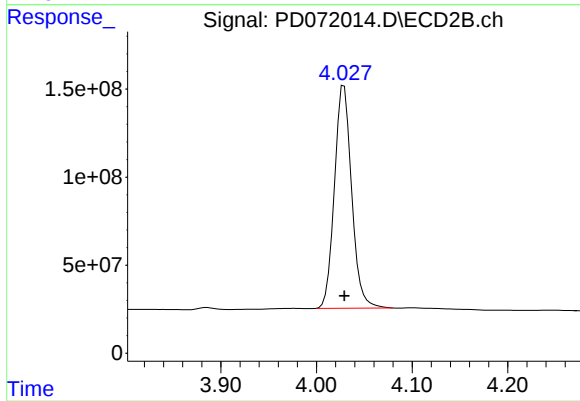

#2 alpha-BHC


R.T.: 4.029 min
Delta R.T.: 0.000 min
Response: 1581313504
Conc: 36.94 ng/ml

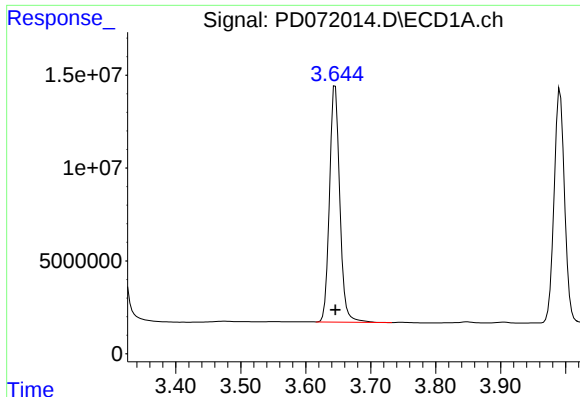

#3 gamma-BHC (Lindane)


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 139820413
Conc: 39.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

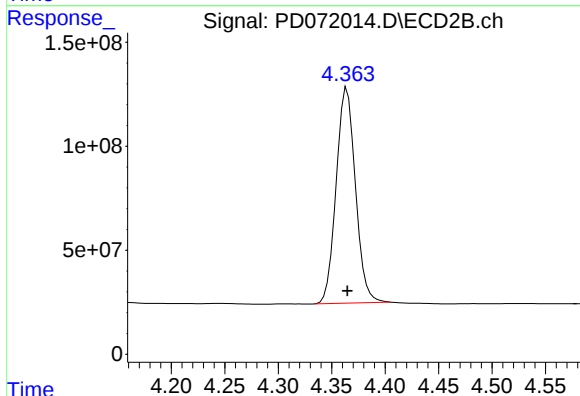


#3 gamma-BHC (Lindane)

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 1301822919
Conc: 36.67 ng/ml

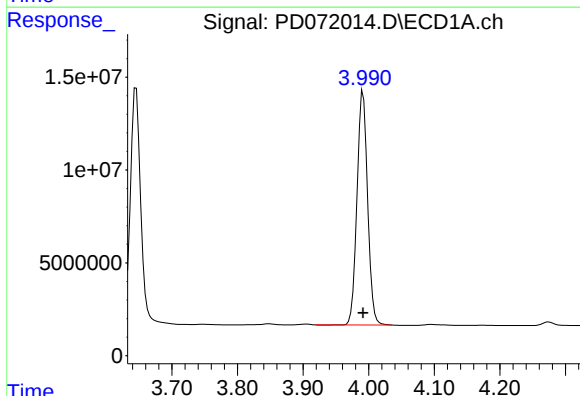


#4 Heptachlor

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 141524708
Conc: 39.78 ng/ml

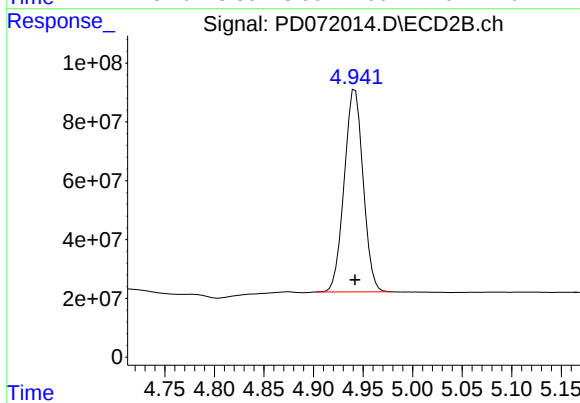

#4 Heptachlor


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 915011399
Conc: 36.03 ng/ml

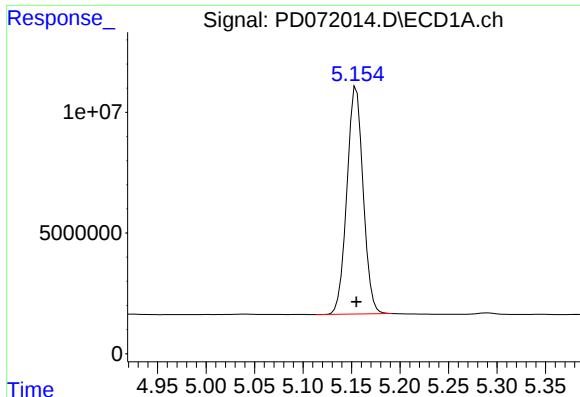

#9 Endosulfan I


R.T.: 5.155 min
Delta R.T.: 0.000 min
Response: 109623191
Conc: 39.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

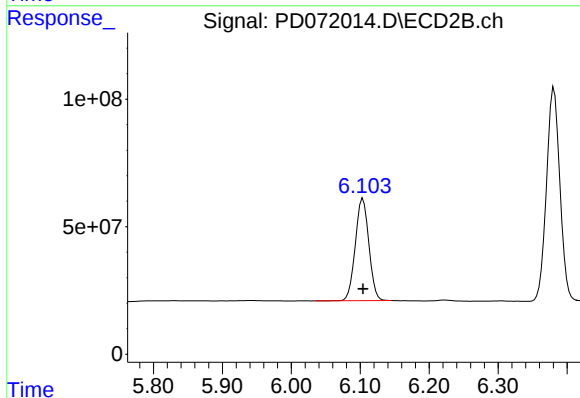


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 547454002
Conc: 36.48 ng/ml

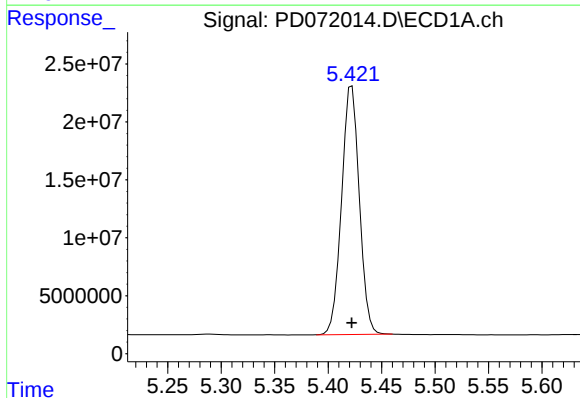


#13 Dieldrin

R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 247950606
Conc: 80.20 ng/ml

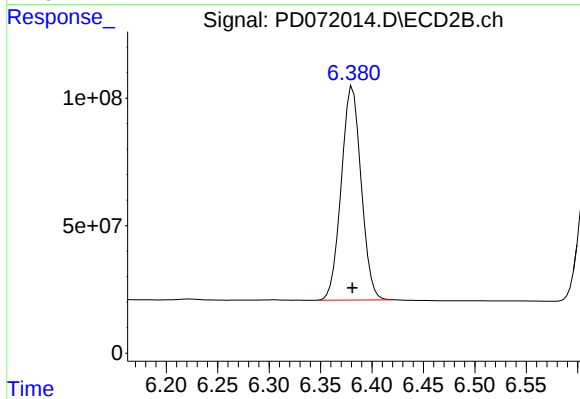

#13 Dieldrin


R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 1129223478
Conc: 74.47 ng/ml

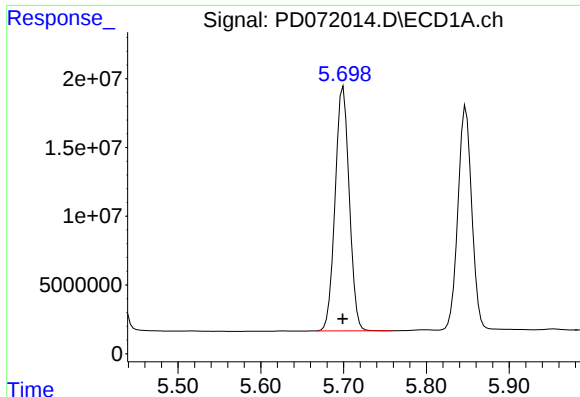

#14 Endrin


R.T.: 5.700 min
Delta R.T.: 0.000 min
Response: 211288418
Conc: 79.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

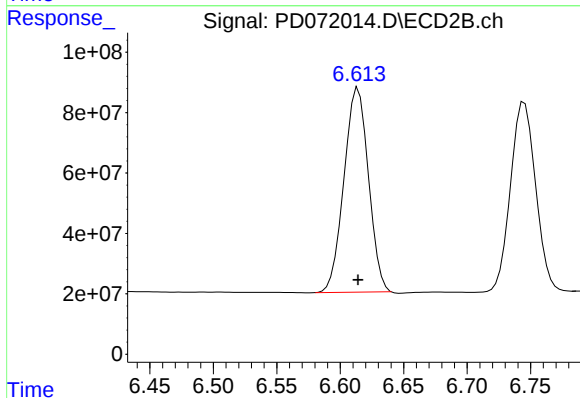


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 908524441
Conc: 73.90 ng/ml

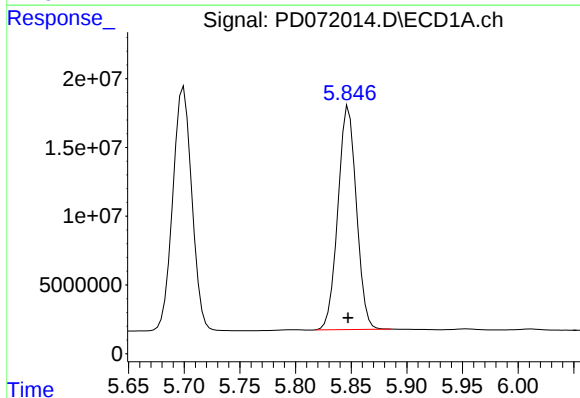


#16 4,4'-DDD

R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 187883162
Conc: 79.77 ng/ml

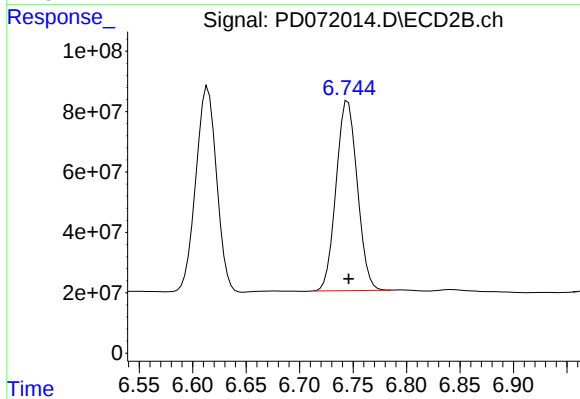

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 865671033
Conc: 74.74 ng/ml

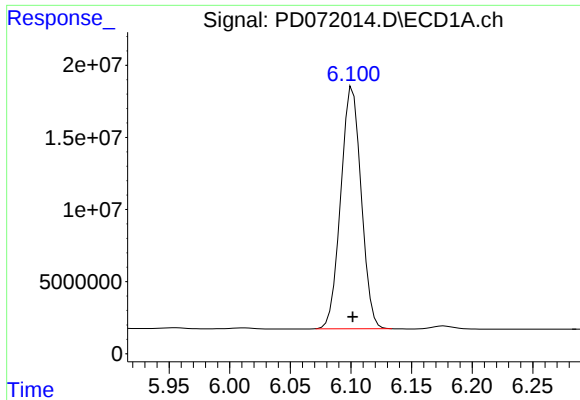

#17 4,4'-DDT


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 196518501
Conc: 81.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

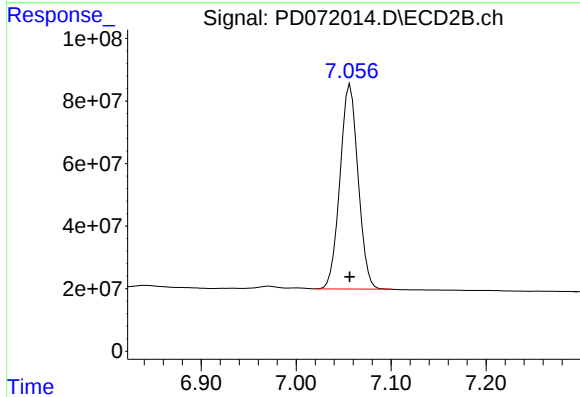


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 868461192
Conc: 75.85 ng/ml

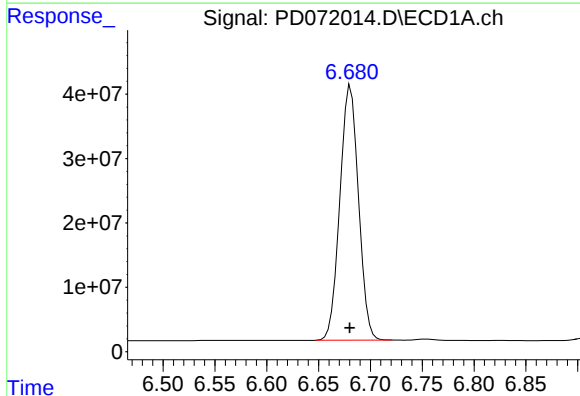


#20 Methoxychlor

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 495054093
Conc: 383.15 ng/ml

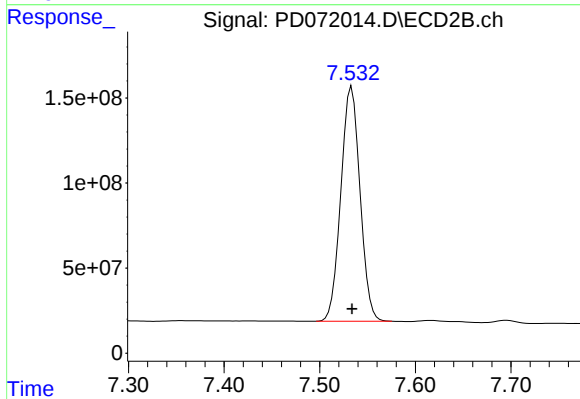

#20 Methoxychlor


R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 1926071524
Conc: 368.77 ng/ml

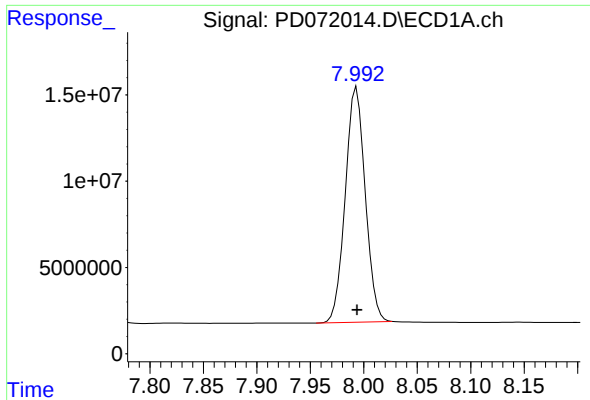

#27 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 177293758
Conc: 76.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

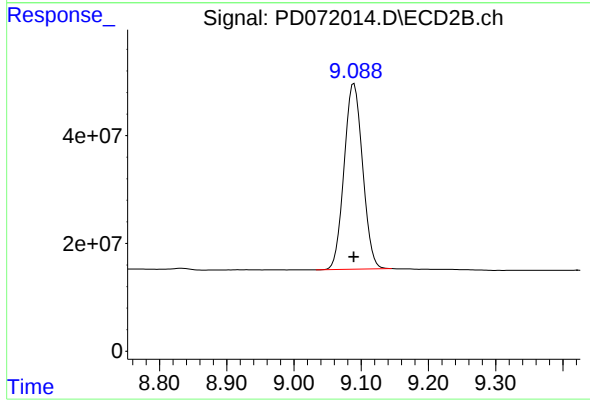

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 658407462
Conc: 73.78 ng/ml