

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 16:48
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:28:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:21:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.824	3.563	193.2E6	2223.8E6	75.842	70.658
27)	SA Decachlor...	8.013	9.089	350.3E6	1221.6E6	150.985	136.895
Target Compounds							
2)	A alpha-BHC	3.332	4.029	308.3E6	3074.3E6	82.576	71.810
3)	MA gamma-BHC...	3.666	4.365	287.5E6	2484.9E6	82.075	69.986
4)	MA Heptachlor	4.012	4.942	288.8E6	1719.2E6	81.163	67.694
9)	A Endosulfan I	5.175	6.104	222.3E6	1021.7E6	79.336	68.086
13)	MA Dieldrin	5.443	6.381	505.6E6	2154.8E6	163.531	142.108
14)	MA Endrin	5.720	6.614	428.4E6	1709.5E6	160.475	139.053
16)	A 4,4'-DDD	5.868	6.746	383.9E6	1664.8E6	162.990	143.726
17)	MA 4,4'-DDT	6.122	7.057	402.6E6	1674.1E6	166.241	146.203
20)	A Methoxychlor	6.700	7.533	948.9E6	3536.1E6	734.446	677.030


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 16:48
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:28:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:21:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

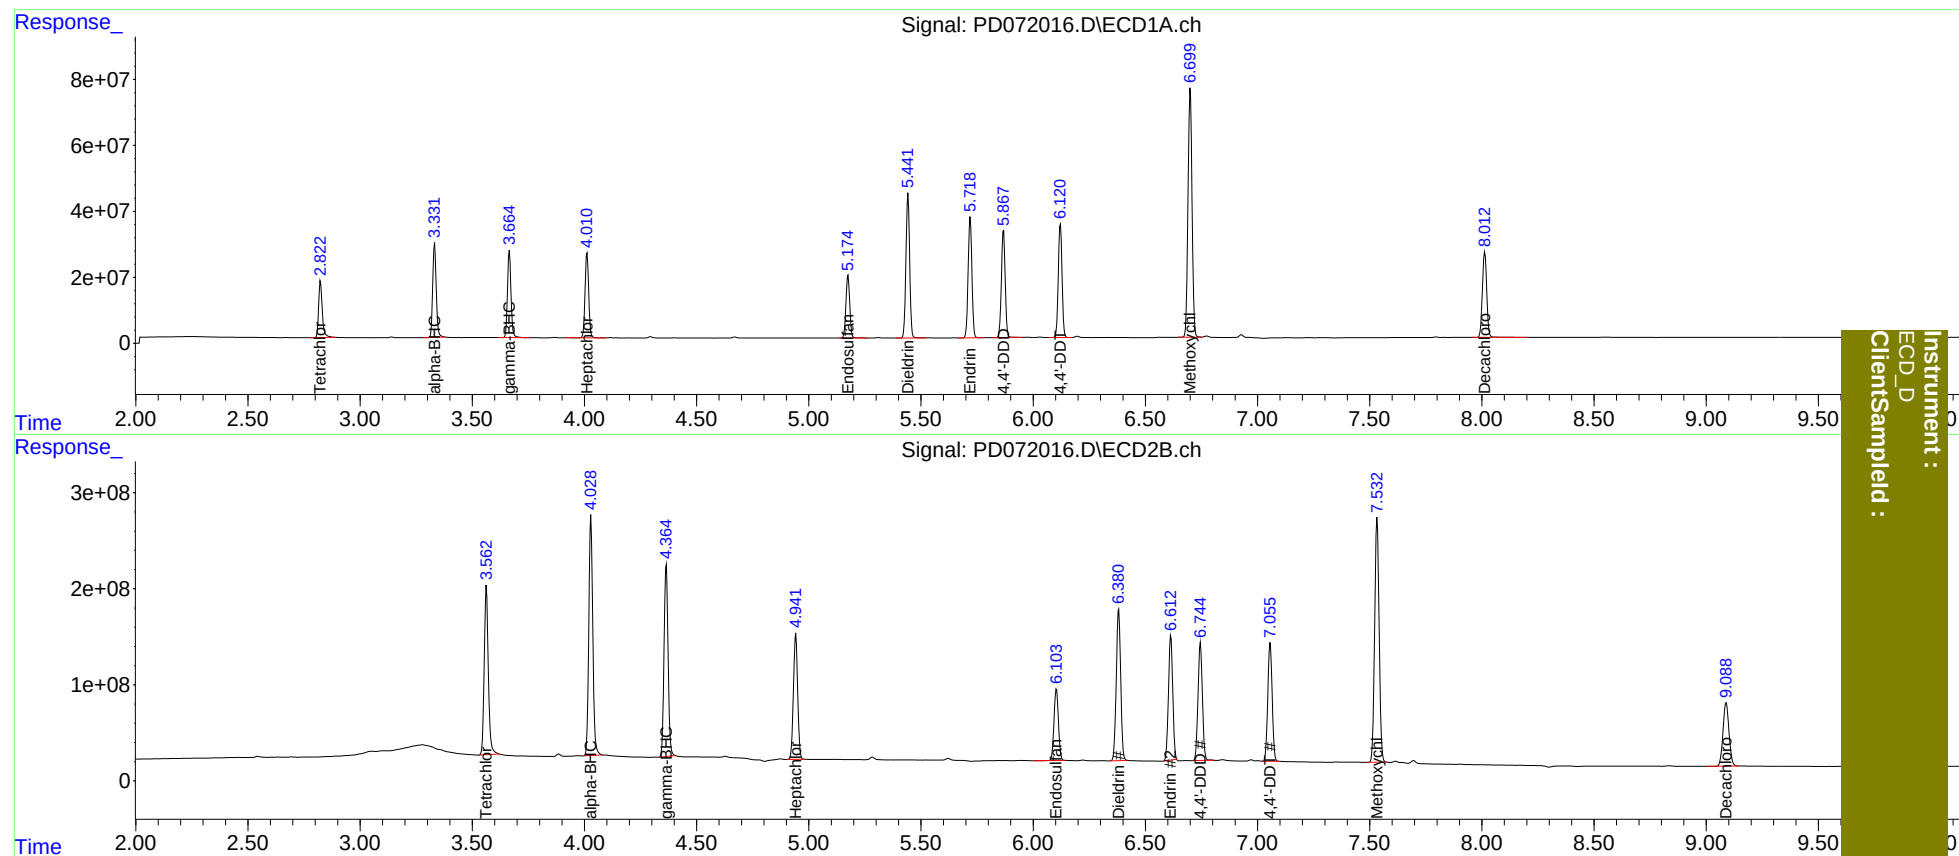


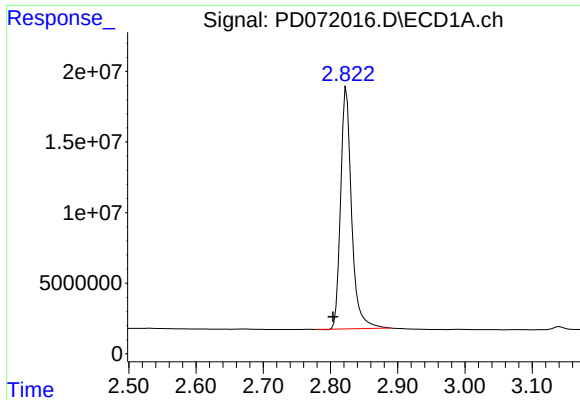

#1 Tetrachloro-m-xylene


R.T.: 2.824 min
Delta R.T.: 0.020 min
Response: 193228264
Conc: 75.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

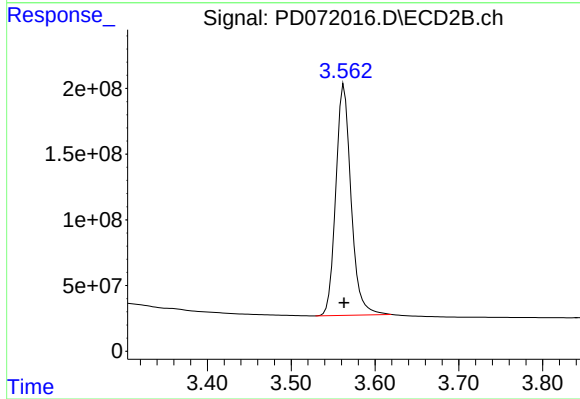


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 2223806859
Conc: 70.66 ng/ml

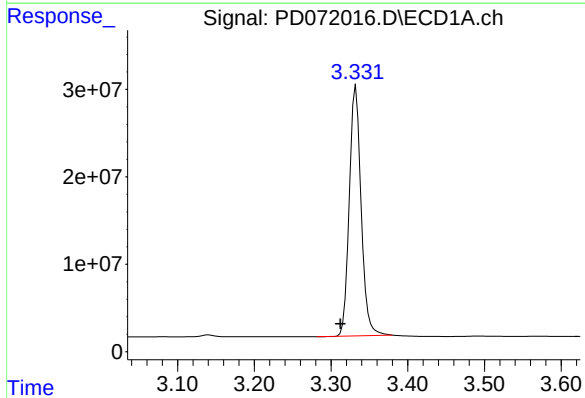


#2 alpha-BHC

R.T.: 3.332 min
Delta R.T.: 0.020 min
Response: 308270767
Conc: 82.58 ng/ml

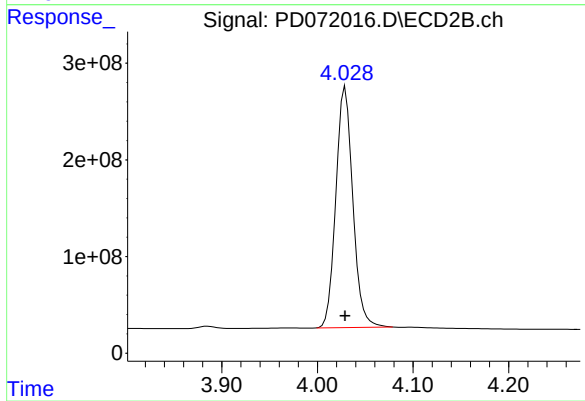

#2 alpha-BHC


R.T.: 4.029 min
Delta R.T.: 0.000 min
Response: 3074264210
Conc: 71.81 ng/ml

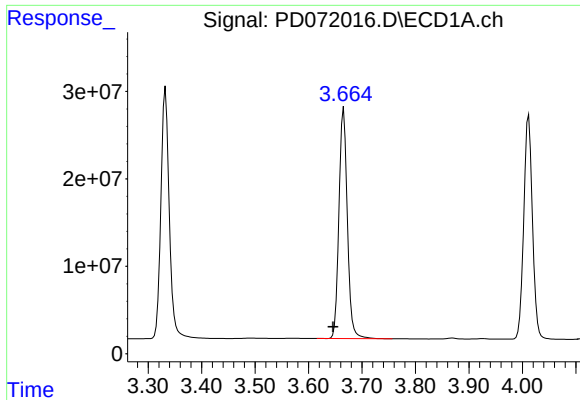

#3 gamma-BHC (Lindane)


R.T.: 3.666 min
Delta R.T.: 0.020 min
Response: 287517892
Conc: 82.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

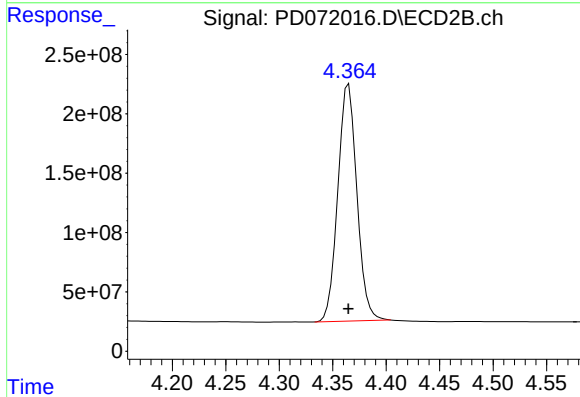


#3 gamma-BHC (Lindane)

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 2484898529
Conc: 69.99 ng/ml

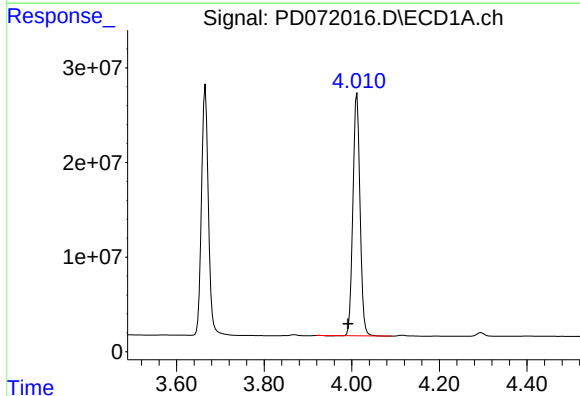


#4 Heptachlor

R.T.: 4.012 min
Delta R.T.: 0.020 min
Response: 288752531
Conc: 81.16 ng/ml

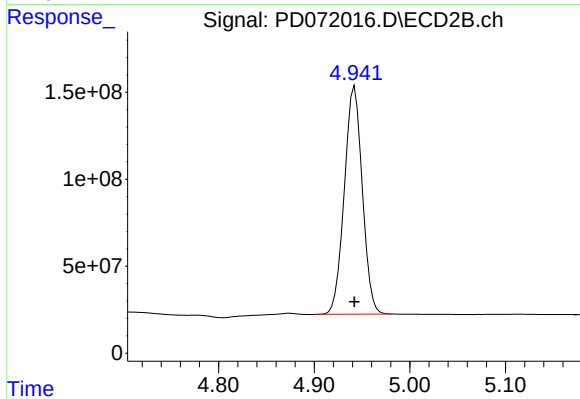

#4 Heptachlor


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 1719189614
Conc: 67.69 ng/ml

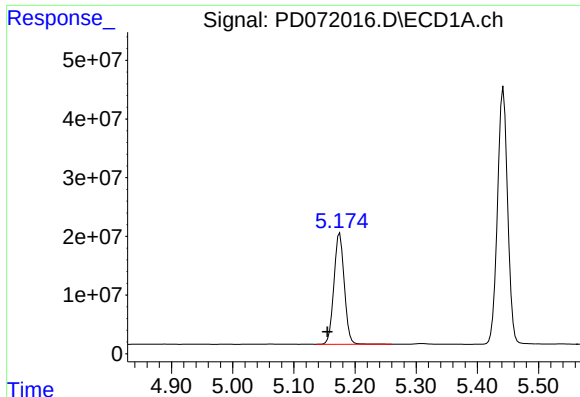

#9 Endosulfan I


R.T.: 5.175 min
Delta R.T.: 0.020 min
Response: 222281688
Conc: 79.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

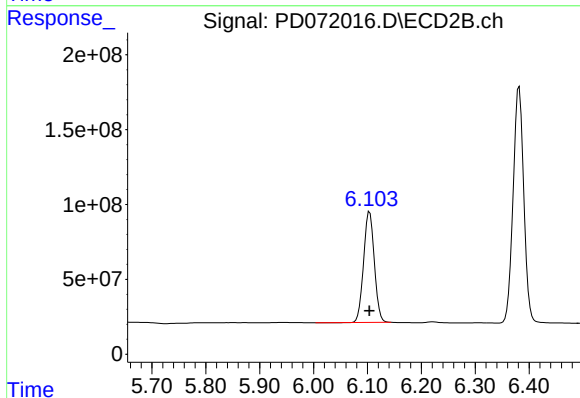


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 1021742528
Conc: 68.09 ng/ml

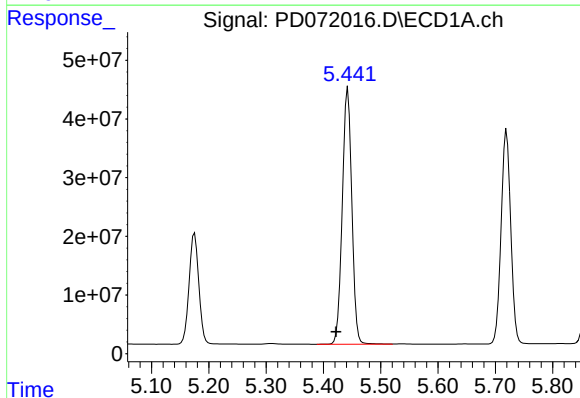


#13 Dieldrin

R.T.: 5.443 min
Delta R.T.: 0.020 min
Response: 505611439
Conc: 163.53 ng/ml

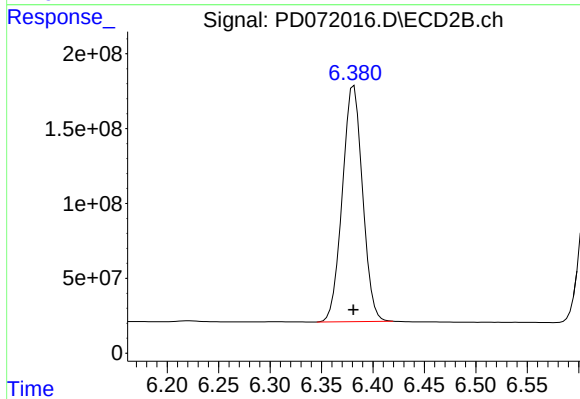

#13 Dieldrin


R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 2154767820
Conc: 142.11 ng/ml

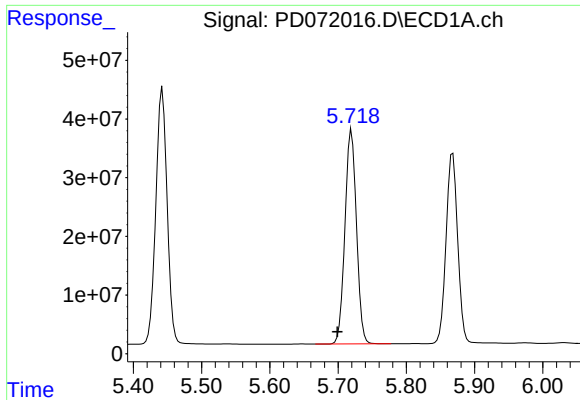

#14 Endrin


R.T.: 5.720 min
Delta R.T.: 0.021 min
Response: 428399203
Conc: 160.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

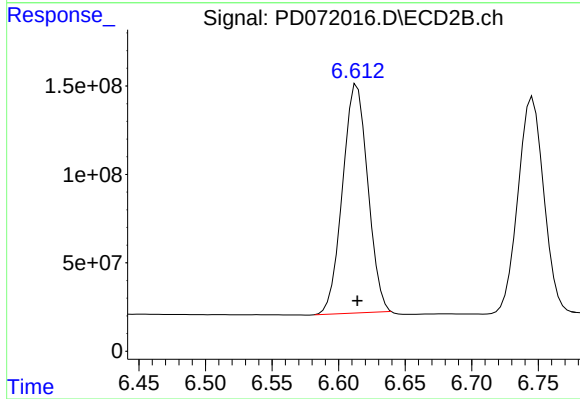


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 1709462226
Conc: 139.05 ng/ml

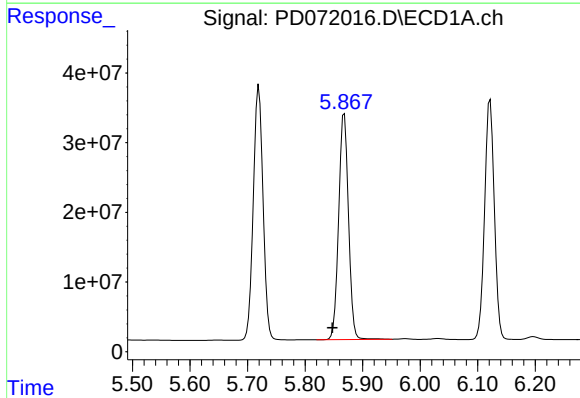


#16 4,4'-DDD

R.T.: 5.868 min
Delta R.T.: 0.021 min
Response: 383874836
Conc: 162.99 ng/ml

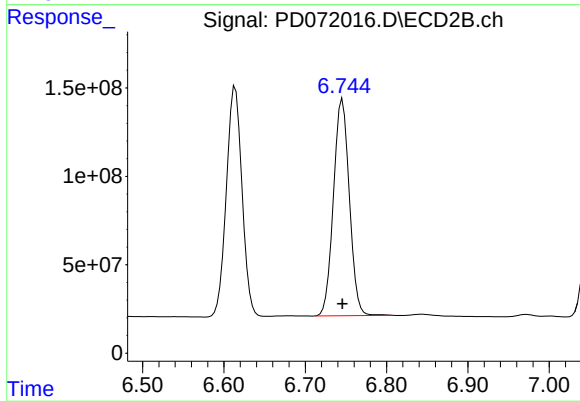

#16 4,4'-DDD


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 1664792374
Conc: 143.73 ng/ml

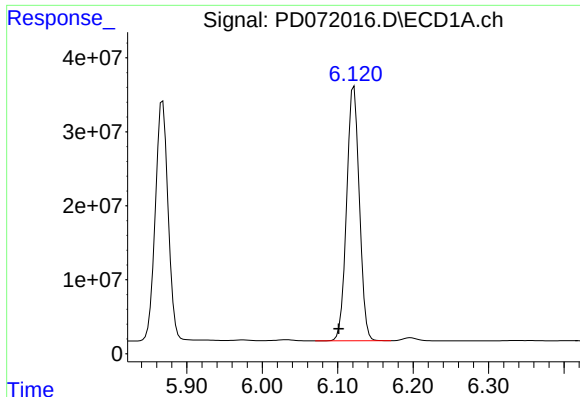

#17 4,4'-DDT


R.T.: 6.122 min
Delta R.T.: 0.020 min
Response: 402581025
Conc: 166.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

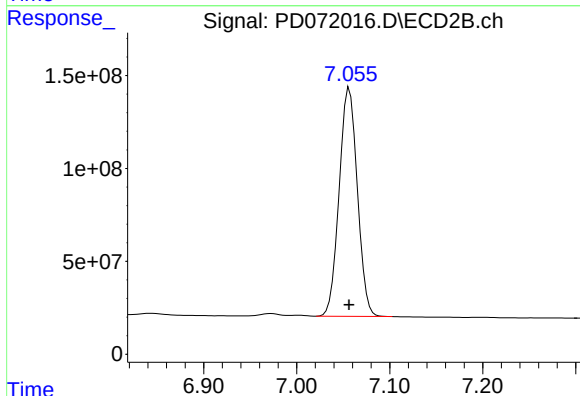


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 1674077112
Conc: 146.20 ng/ml

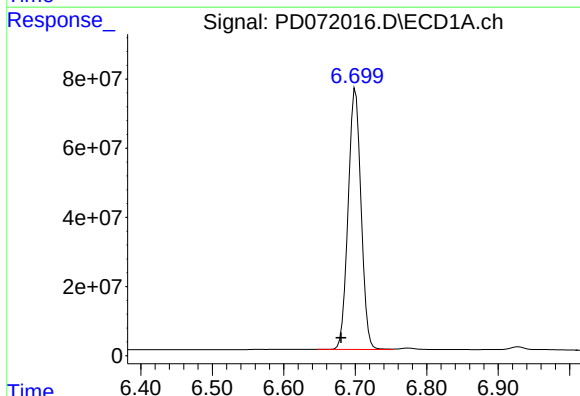


#20 Methoxychlor

R.T.: 6.700 min
Delta R.T.: 0.020 min
Response: 948941821
Conc: 734.45 ng/ml

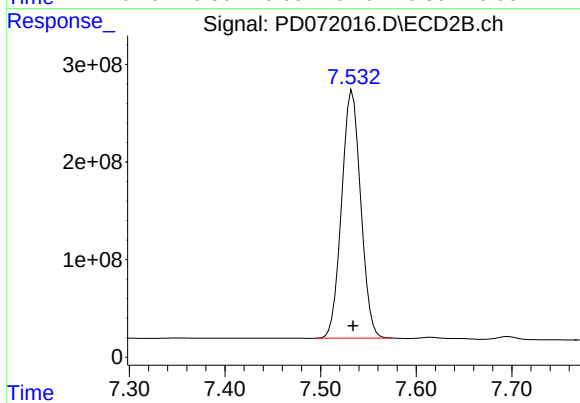

#20 Methoxychlor


R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 3536139183
Conc: 677.03 ng/ml

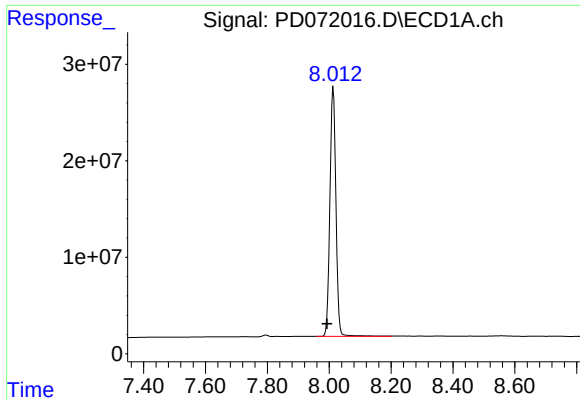

#27 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: 0.020 min
Response: 350340381
Conc: 150.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

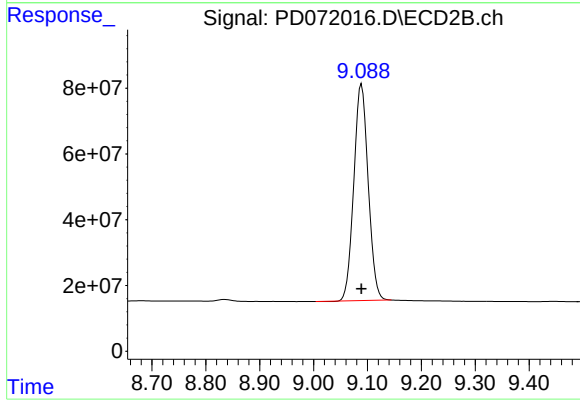

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 1221641586
Conc: 136.89 ng/ml