

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 17:02
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:36:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:34:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.563	190.8E6	2147.8E6	76.548	71.902
27)	SA Decachlor...	7.993	9.090	362.1E6	1249.5E6	147.407	135.258
Target Compounds							
5)	MB Aldrin	4.275	5.284	285.2E6	1459.9E6	79.690	66.058
6)	B beta-BHC	3.944	4.571	118.0E6	985.1E6	72.899	65.377
7)	B delta-BHC	4.178	4.819	289.2E6	1786.2E6	81.286	70.660
8)	B Heptachlo...	4.782	5.716	247.3E6	1102.0E6	77.299	68.862
10)	B trans-Chl...	5.034	5.971	258.3E6	1179.0E6	78.896	67.689
11)	B cis-Chlor...	5.099	6.048	249.9E6	1139.7E6	77.836	67.163
12)	B 4,4'-DDE	5.290	6.221	480.2E6	2114.5E6	159.628	140.311
15)	B Endosulfa...	5.995	6.839	387.9E6	1679.3E6	153.577	137.509
18)	B Endrin al...	6.175	6.971	326.9E6	1422.4E6	150.257	136.909
19)	B Endosulfa...	6.399	7.203	388.4E6	1626.5E6	153.369	140.656
21)	B Endrin ke...	6.909	7.695	439.6E6	1740.4E6	154.203	138.727

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 17:02
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:36:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:34:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

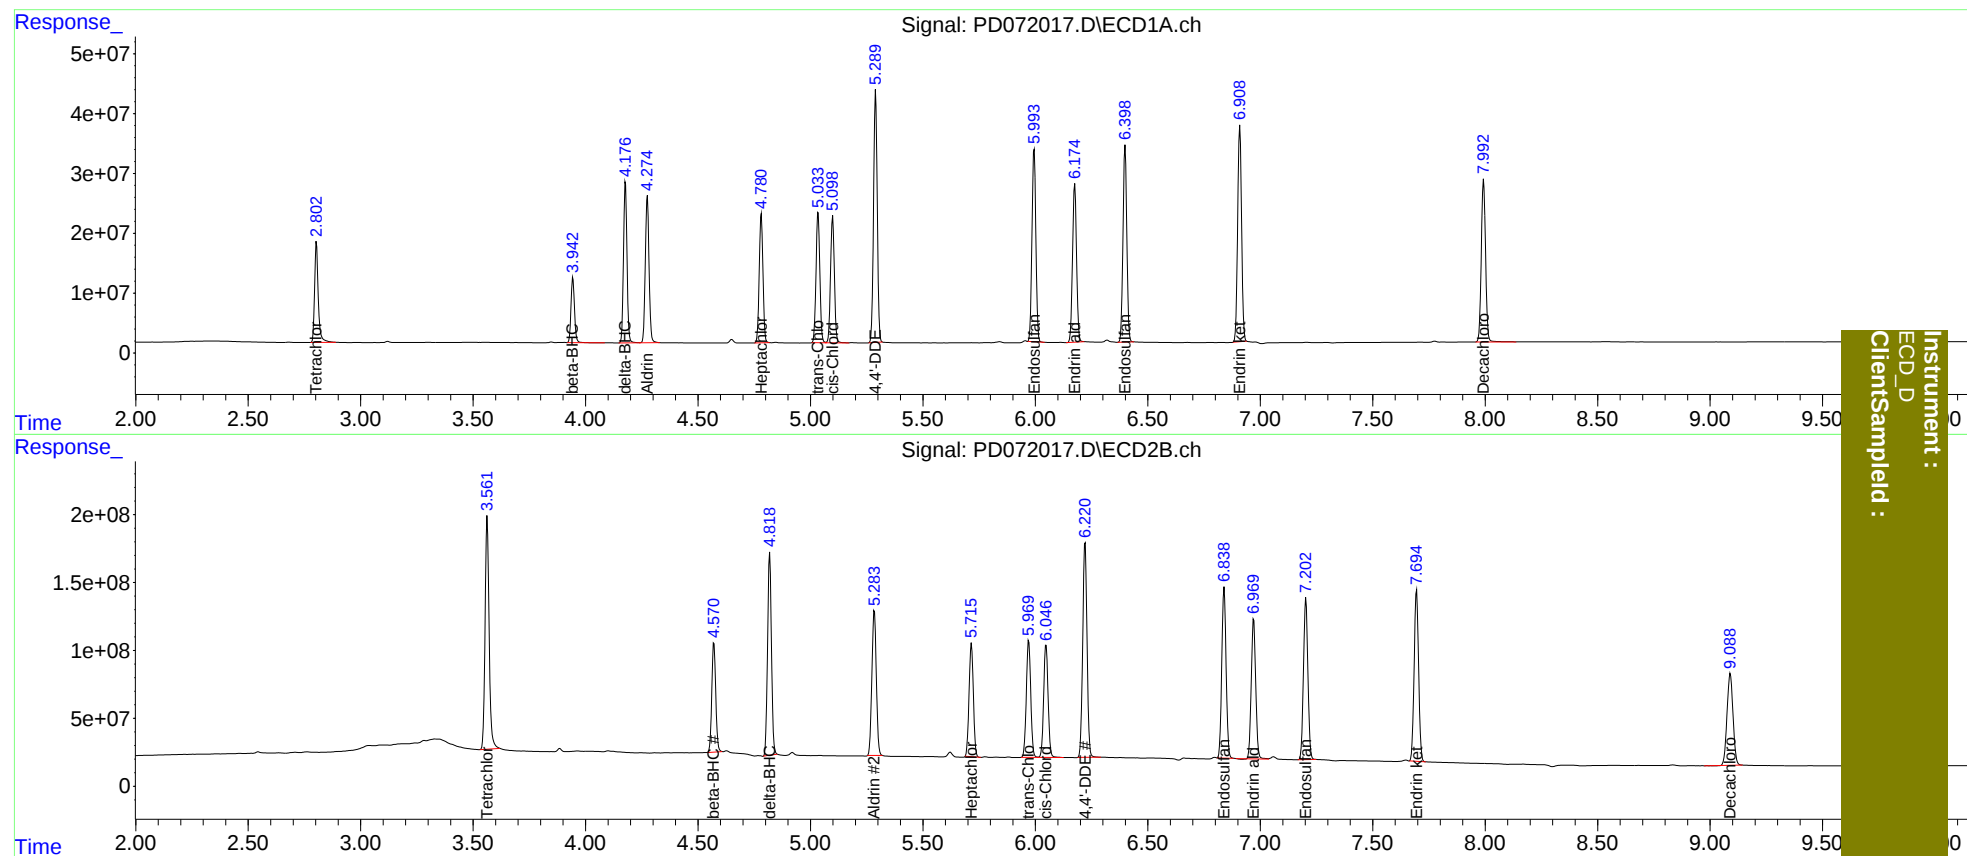


Instrument :
ECD_D
ClientSampled :

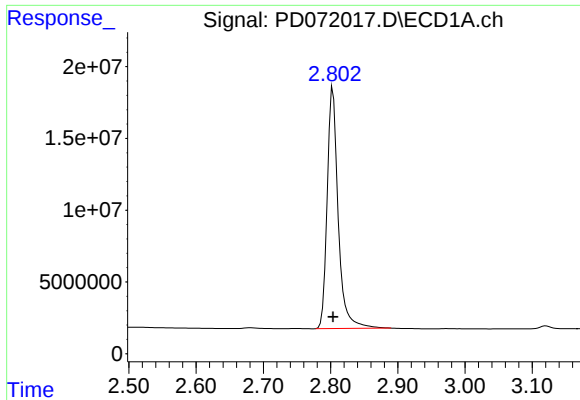

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 190837462
Conc: 76.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

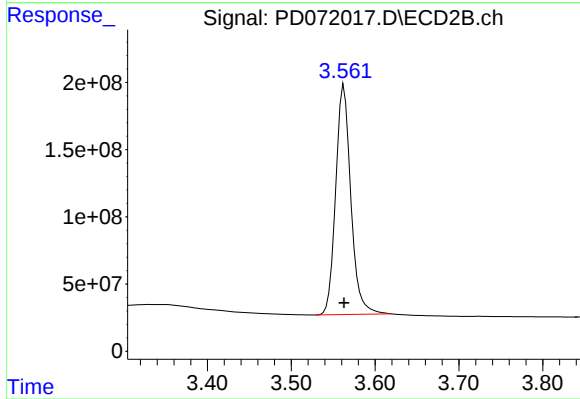


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 2147811508
Conc: 71.90 ng/ml

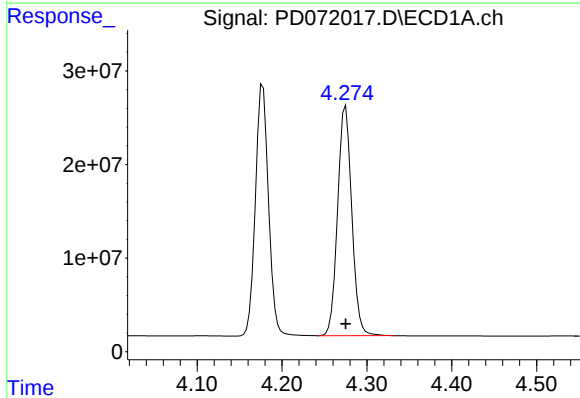


#5 Aldrin

R.T.: 4.275 min
Delta R.T.: 0.000 min
Response: 285155047
Conc: 79.69 ng/ml

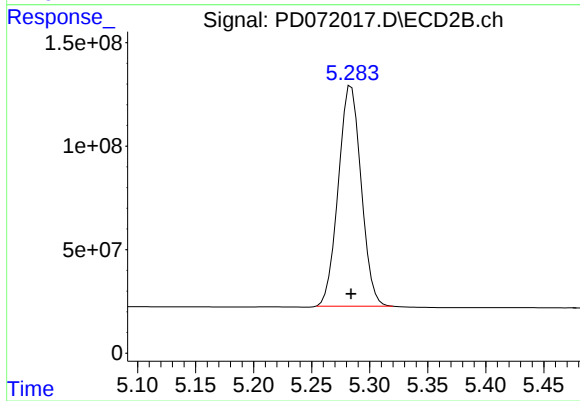

#5 Aldrin


R.T.: 5.284 min
Delta R.T.: 0.000 min
Response: 1459887612
Conc: 66.06 ng/ml

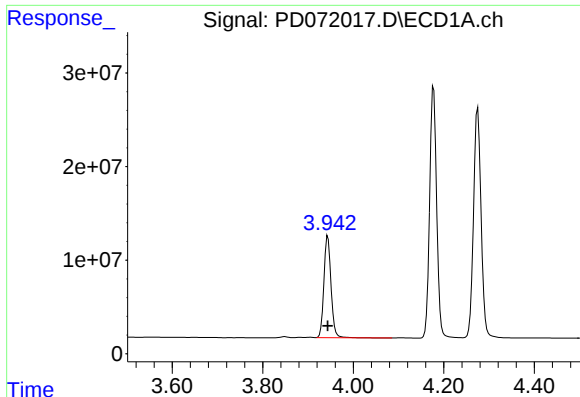

#6 beta-BHC


R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 118039372
Conc: 72.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

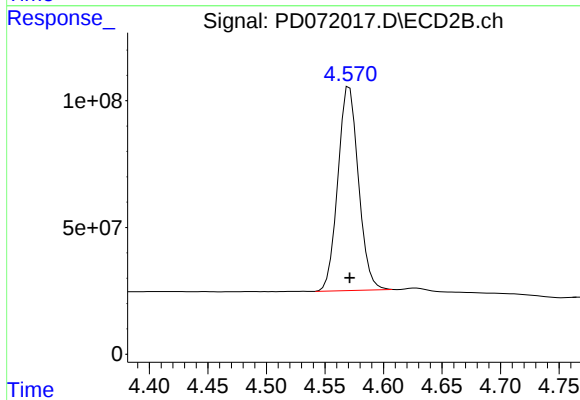


#6 beta-BHC

R.T.: 4.571 min
Delta R.T.: 0.000 min
Response: 985056952
Conc: 65.38 ng/ml

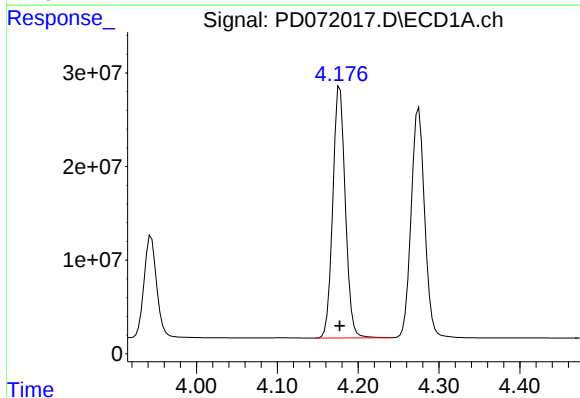


#7 delta-BHC

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 289249769
Conc: 81.29 ng/ml

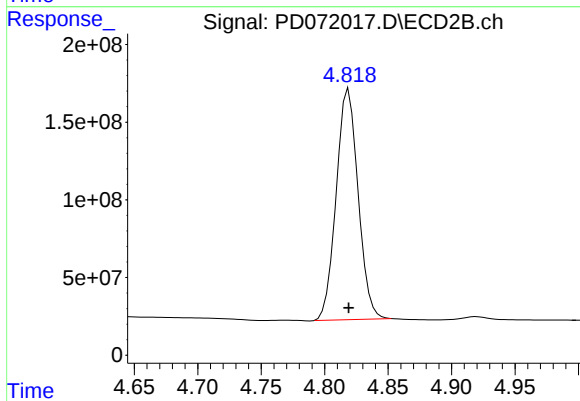

#7 delta-BHC


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 1786198063
Conc: 70.66 ng/ml

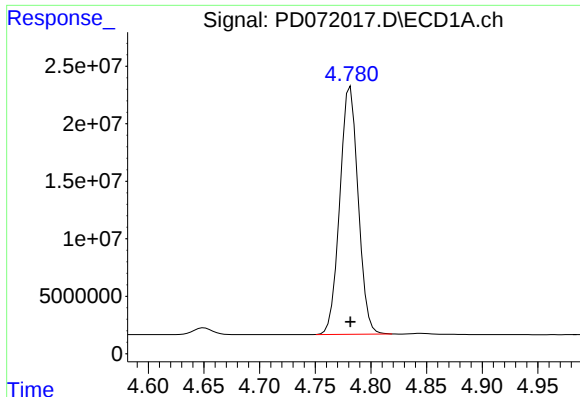

#8 Heptachlor epoxide


R.T.: 4.782 min
Delta R.T.: 0.000 min
Response: 247265430
Conc: 77.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

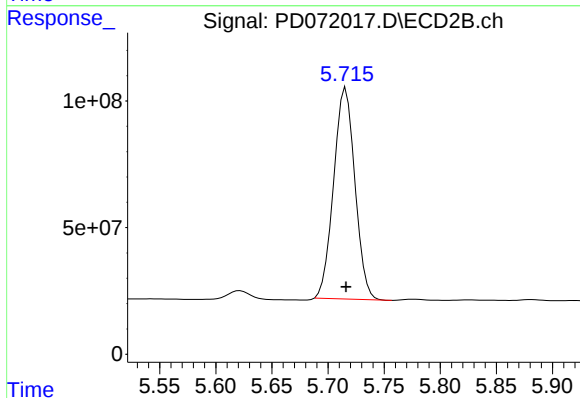


#8 Heptachlor epoxide

R.T.: 5.716 min
Delta R.T.: 0.000 min
Response: 1102002087
Conc: 68.86 ng/ml

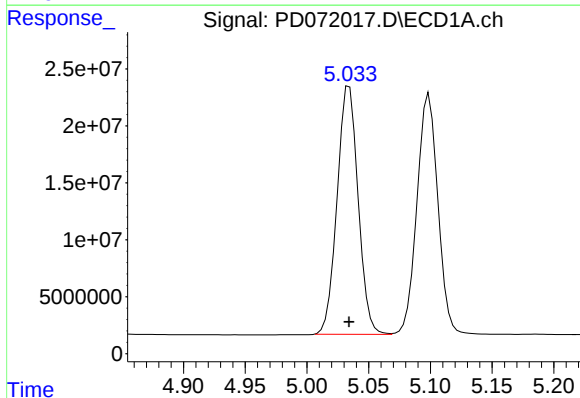


#10 trans-Chlordane

R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 258326018
Conc: 78.90 ng/ml

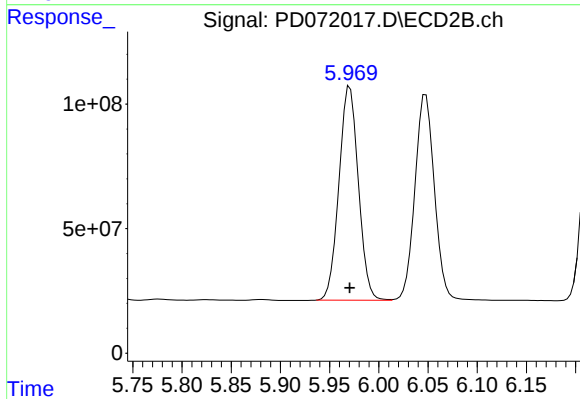

#10 trans-Chlordane


R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 1178952070
Conc: 67.69 ng/ml

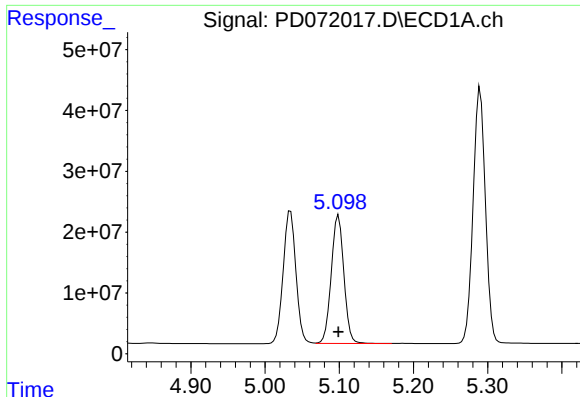

#11 cis-Chlordane


R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 249860038
Conc: 77.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

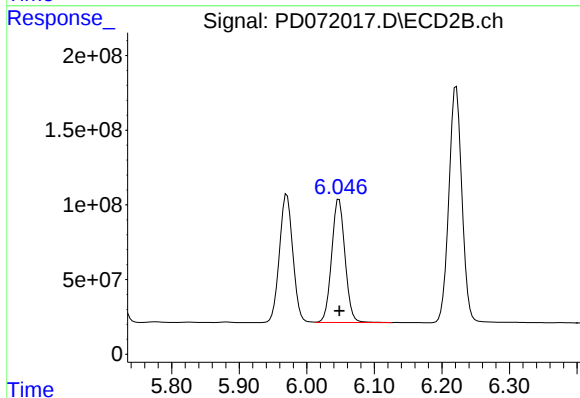


#11 cis-Chlordane

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 1139656667
Conc: 67.16 ng/ml

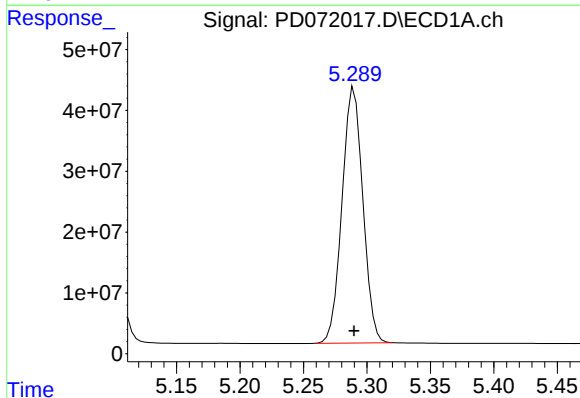


#12 4,4'-DDE

R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 480202577
Conc: 159.63 ng/ml

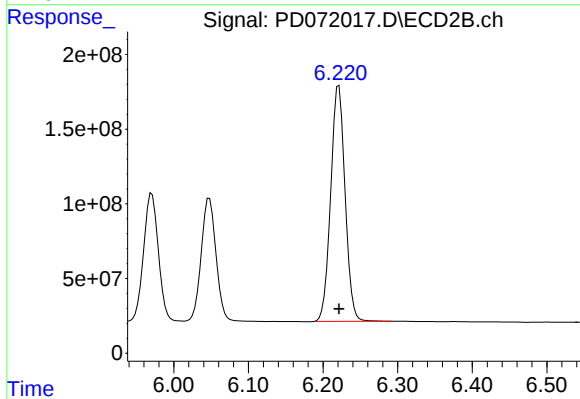

#12 4,4'-DDE


R.T.: 6.221 min
Delta R.T.: 0.000 min
Response: 2114540392
Conc: 140.31 ng/ml

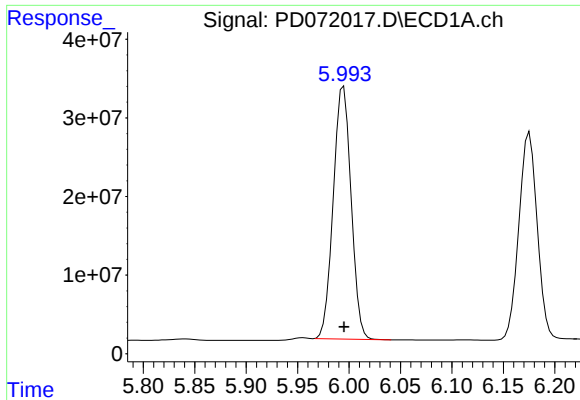

#15 Endosulfan II


R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 387933479
Conc: 153.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

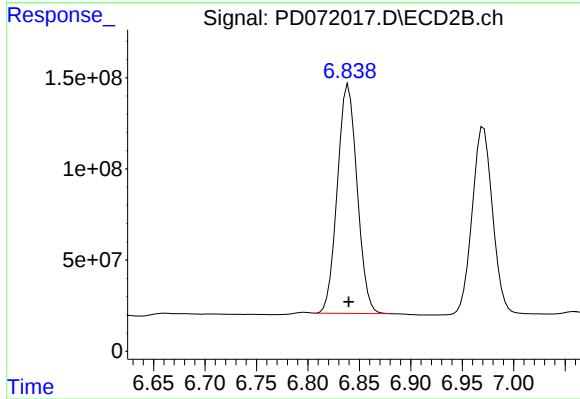


#15 Endosulfan II

R.T.: 6.839 min
Delta R.T.: 0.000 min
Response: 1679338635
Conc: 137.51 ng/ml

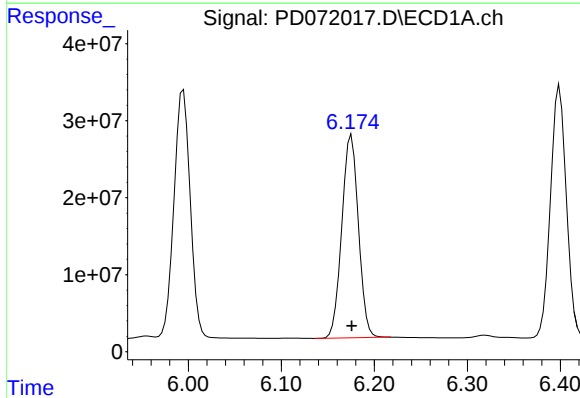


#18 Endrin aldehyde

R.T.: 6.175 min
Delta R.T.: 0.000 min
Response: 326872560
Conc: 150.26 ng/ml

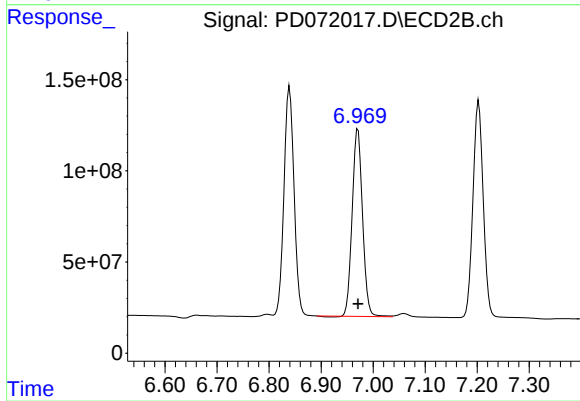

#18 Endrin aldehyde


R.T.: 6.971 min
Delta R.T.: 0.000 min
Response: 1422421605
Conc: 136.91 ng/ml

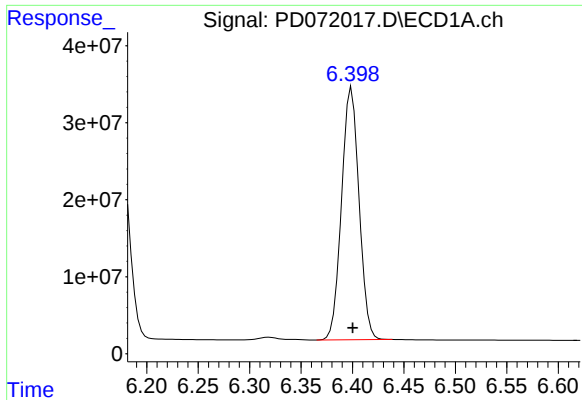

#19 Endosulfan Sulfate


R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 388409989
Conc: 153.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

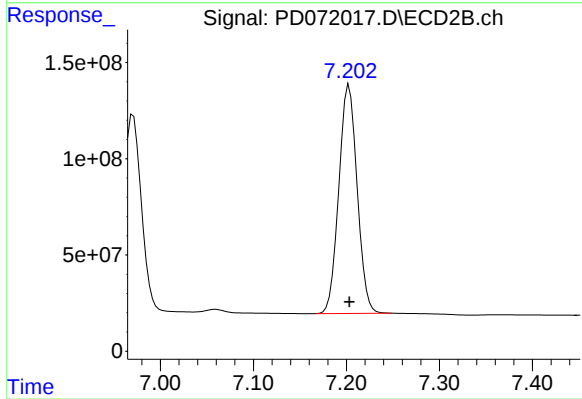


#19 Endosulfan Sulfate

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 1626482908
Conc: 140.66 ng/ml

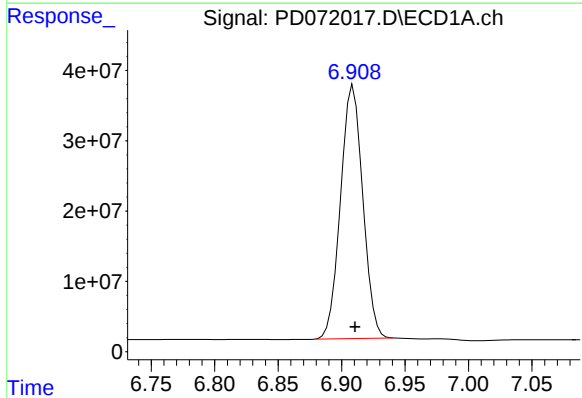


#21 Endrin ketone

R.T.: 6.909 min
Delta R.T.: -0.001 min
Response: 439584490
Conc: 154.20 ng/ml

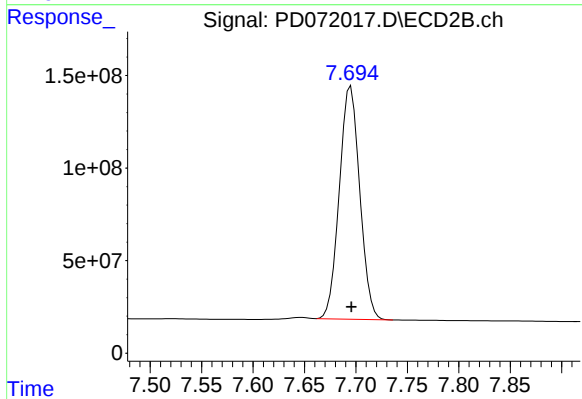

#21 Endrin ketone


R.T.: 7.695 min
Delta R.T.: 0.000 min
Response: 1740428706
Conc: 138.73 ng/ml

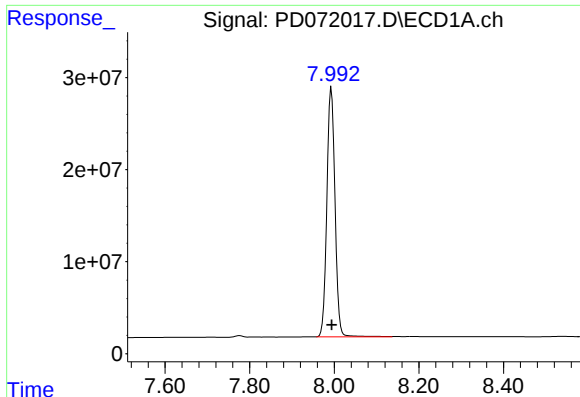

#27 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 362140789
Conc: 147.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

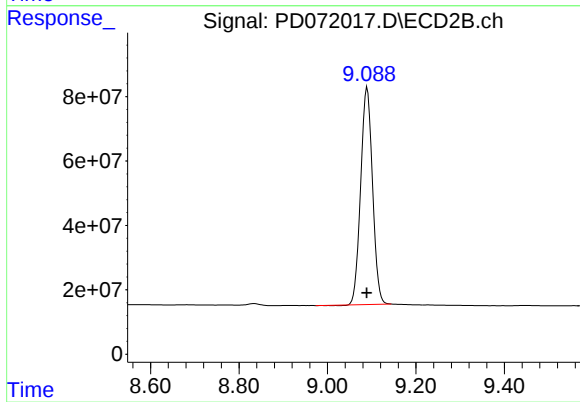

#27 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.001 min
Response: 1249470517
Conc: 135.26 ng/ml