

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
 Data File : PD072001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 13:29
 Operator : AR\AJ
 Sample : RESC037
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC039

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 17:47:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.563	49734146	622.2E6	19.616	20.194
27)	SA Decachlor...	7.994	9.089	89685720	356.4E6	38.255	39.788
Target Compounds							
2)	A alpha-BHC	3.312	4.029	35176248	436.9E6	9.498	10.270
3)	MA gamma-BHC...	3.646	4.365	31167201	364.1E6	8.913	10.292
4)	MA Heptachlor	3.992	4.942	33036473	252.9E6	9.298	10.026
5)	MB Aldrin	4.275	5.284	33212104	224.0E6	9.345	10.194
6)	B beta-BHC	3.944	4.572	15357640	154.9E6	9.595	10.410
7)	B delta-BHC	4.178	4.820	32145080	229.0E6	9.078	9.190
8)	B Heptachlo...	4.782	5.716	29476809	119.3E6	9.259	7.824
9)	A Endosulfan I	5.156	6.104	26562389	151.3E6	9.426	10.150
10)	B trans-Chl...	5.034	5.971	30229966	170.5E6	9.256	9.867
11)	B cis-Chlor...	5.099	6.049	29861349	167.1E6	9.306	9.928
12)	B 4,4'-DDE	5.290	6.222	53788208	297.9E6	18.174	19.852
13)	MA Dieldrin	5.423	6.381	56220909	301.3E6	18.287	19.957
14)	MA Endrin	5.700	6.614	49068704	254.3E6	18.508	20.631
15)	B Endosulfa...	5.995	6.840	46661425	248.5E6	18.697	20.458
16)	A 4,4'-DDD	5.848	6.747	42624885	230.8E6	18.258	19.982
17)	MA 4,4'-DDT	6.102	7.057	43351749	230.9E6	18.093	20.298
18)	B Endrin al...	6.176	6.971	41513230	211.3E6	19.118	20.375
19)	B Endosulfa...	6.400	7.204	47806828	233.1E6	18.944	20.234
20)	A Methoxychlor	6.681	7.533	127.0E6	544.6E6	98.816	104.766
21)	B Endrin ke...	6.910	7.696	54904383	257.5E6	19.415	20.620

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 13:29
Operator : AR\AJ
Sample : RESC037
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:47:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

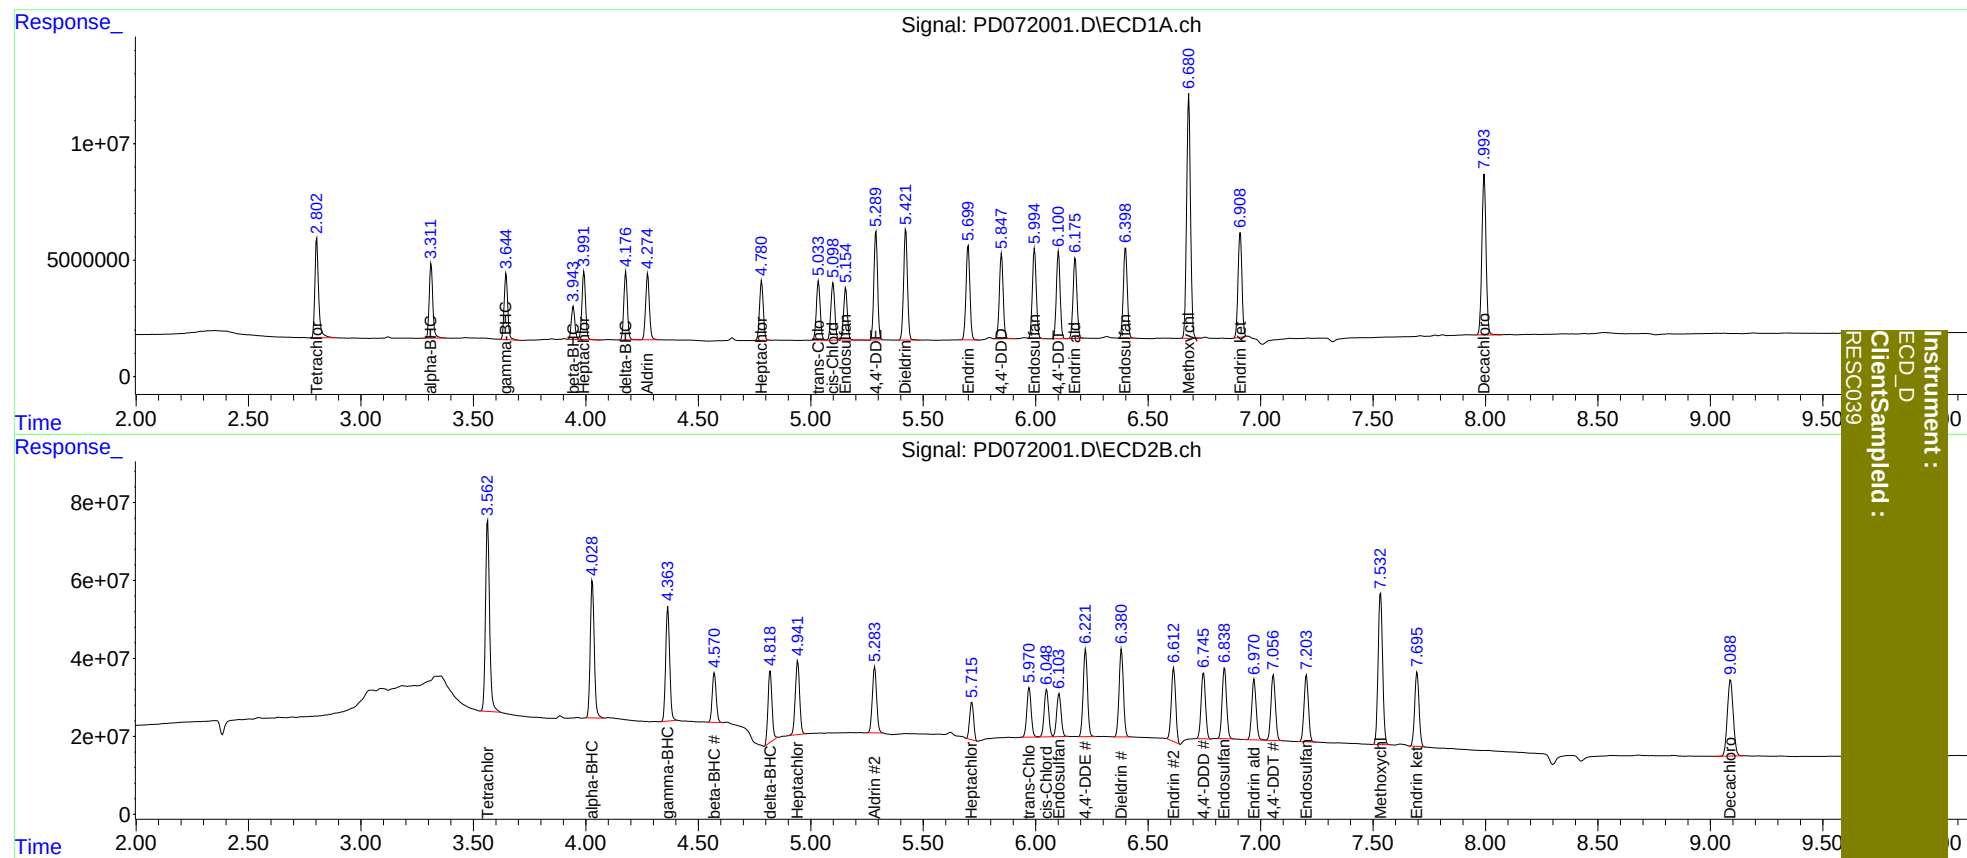

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072001.D
Acq On : 23 Sep 2022 13:29
Operator : AR\AJ
Sample : RESC037
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC039

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Title : GC Extractables
Last Update : Fri Sep 23 17:46:27 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
2.804	3.312	100.00%
3.312	3.646	100.00%
3.646	3.944	100.00%
3.944	3.992	98.90%
3.992	4.178	100.00%
4.178	4.275	100.00%
4.275	4.782	100.00%
4.782	5.034	100.00%
5.034	5.099	99.92%
5.099	5.156	99.69%
5.156	5.290	100.00%
5.290	5.423	100.00%
5.423	5.700	100.00%
5.700	5.848	100.00%
5.848	5.995	100.00%
5.995	6.102	100.00%
6.102	6.176	100.00%
6.176	6.400	100.00%
6.400	6.681	100.00%
6.681	6.910	100.00%
6.910	7.994	100.00%

Signal #2


3.563	4.029	100.00%
4.029	4.365	100.00%
4.365	4.572	100.00%
4.572	4.820	100.00%
4.820	4.942	100.00%
4.942	5.284	100.00%
5.284	5.716	100.00%
5.716	5.971	100.00%
5.971	6.049	100.00%
6.049	6.104	98.83%
6.104	6.222	100.00%
6.222	6.381	100.00%
6.381	6.614	100.00%
6.614	6.747	100.00%
6.747	6.840	100.00%
6.840	6.971	100.00%
6.971	7.057	100.00%
7.057	7.204	100.00%
7.204	7.533	100.00%
7.533	7.696	100.00%
7.696	9.089	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 13:29
Operator : AR\AJ
Sample : RESC037
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC039

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:47:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

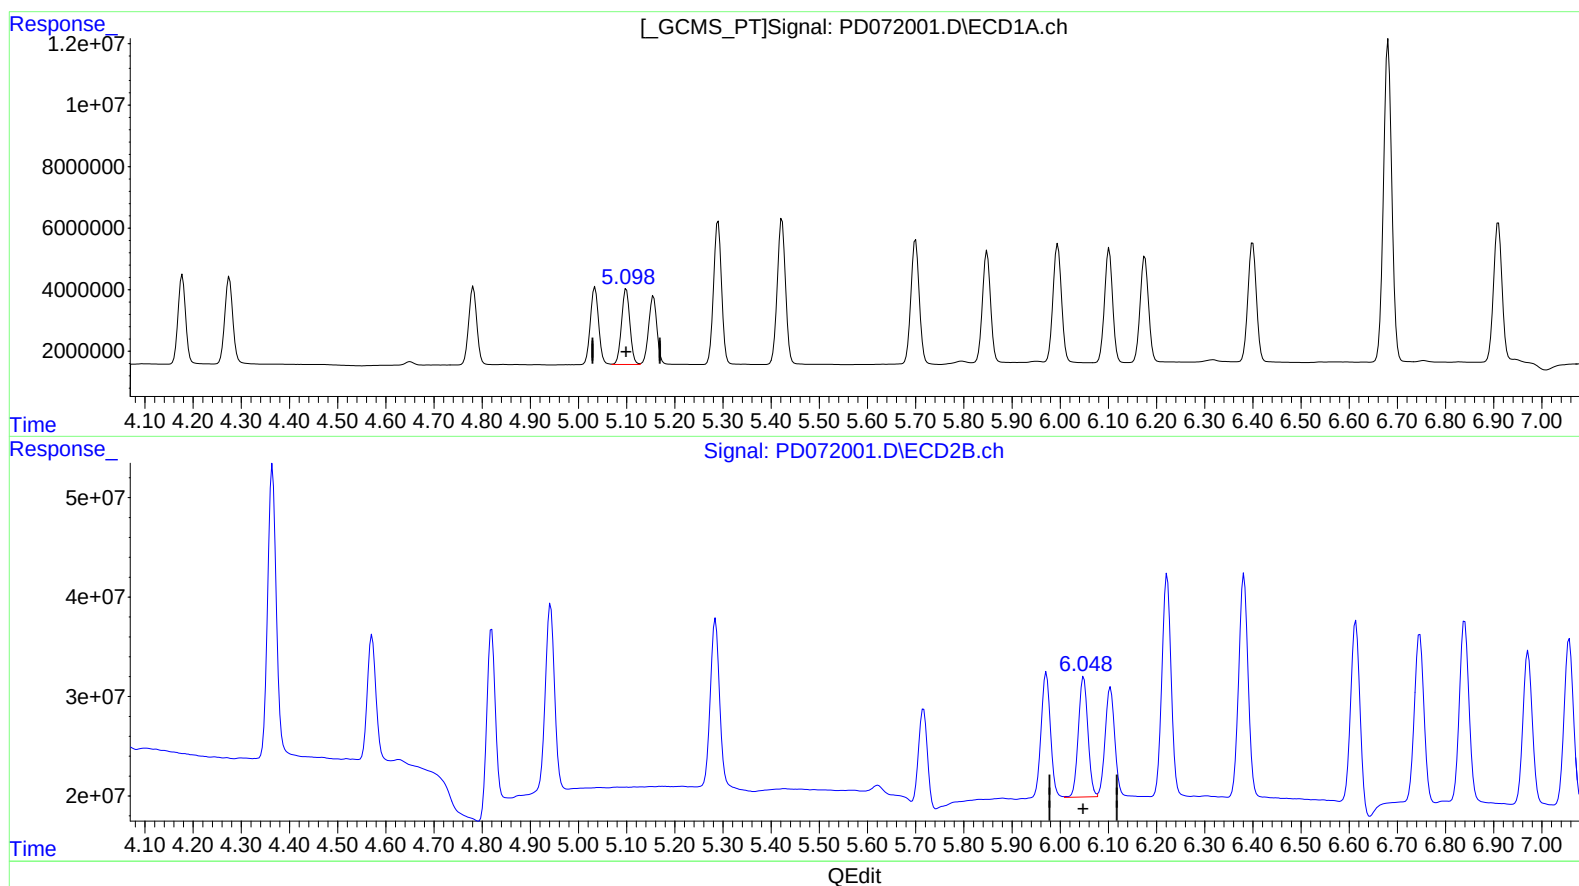

(11) cis-Chlordane (B)

5.099min 9.306 ng/ml

response 29861349

(11) cis-Chlordane #2 (B)

6.049min 9.928 ng/ml


response 167107961

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 13:29
Operator : AR\AJ
Sample : RESC037
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC039

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:47:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

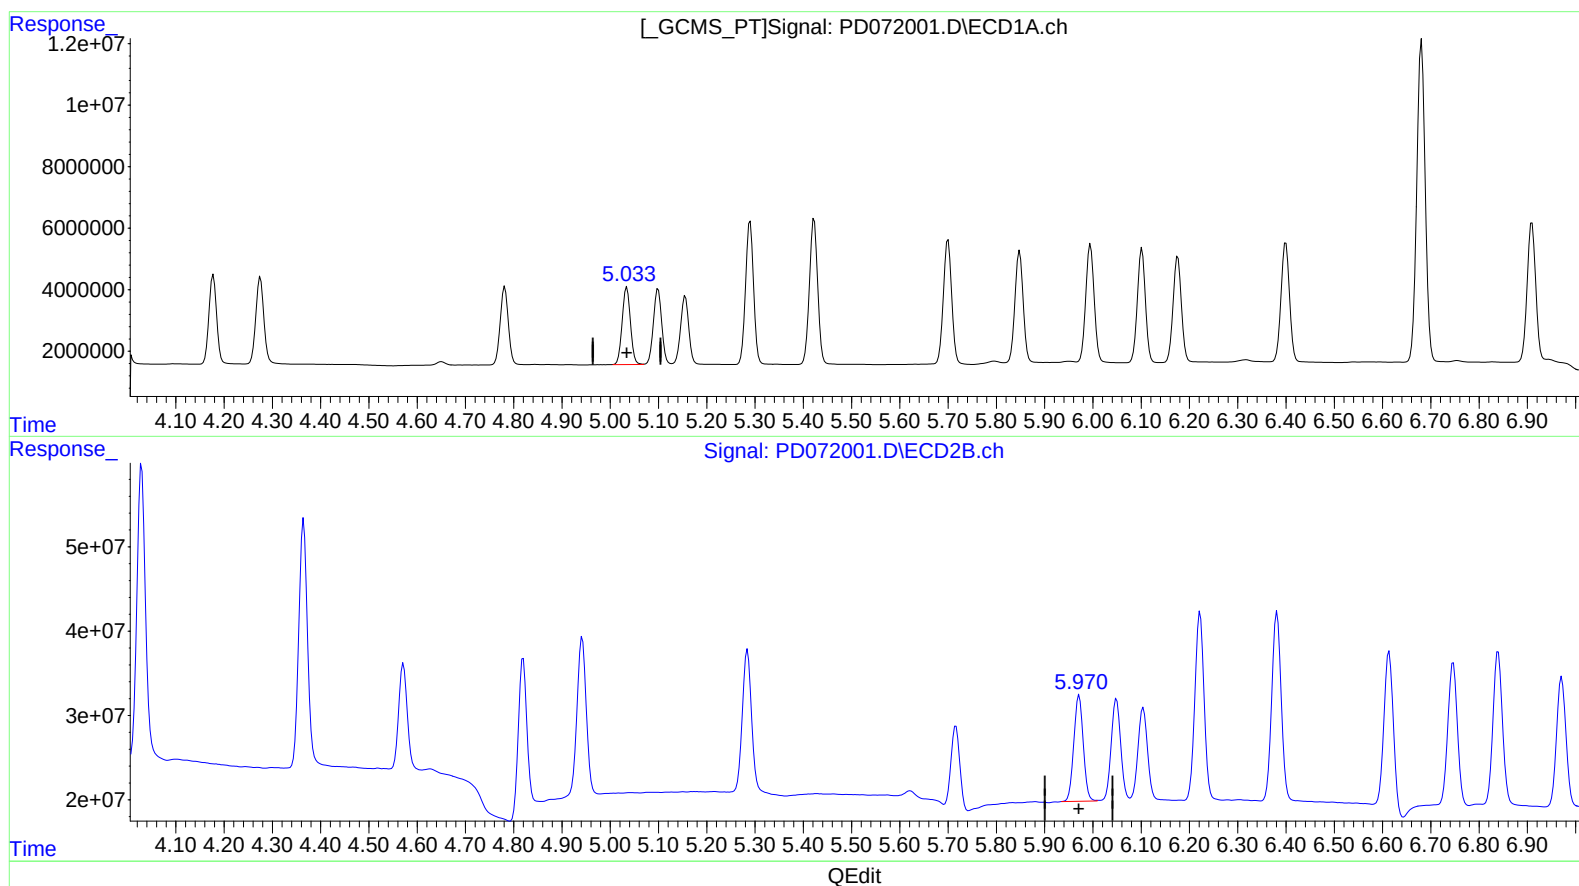

(10) trans-Chlordane (B)

5.034min 9.256 ng/ml

response 30229966

(10) trans-Chlordane #2 (B)

5.971min 9.867 ng/ml


response 170501201

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092422\
Data File : PD072001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 13:29
Operator : AR\AJ
Sample : RESC037
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC039

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 17:47:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

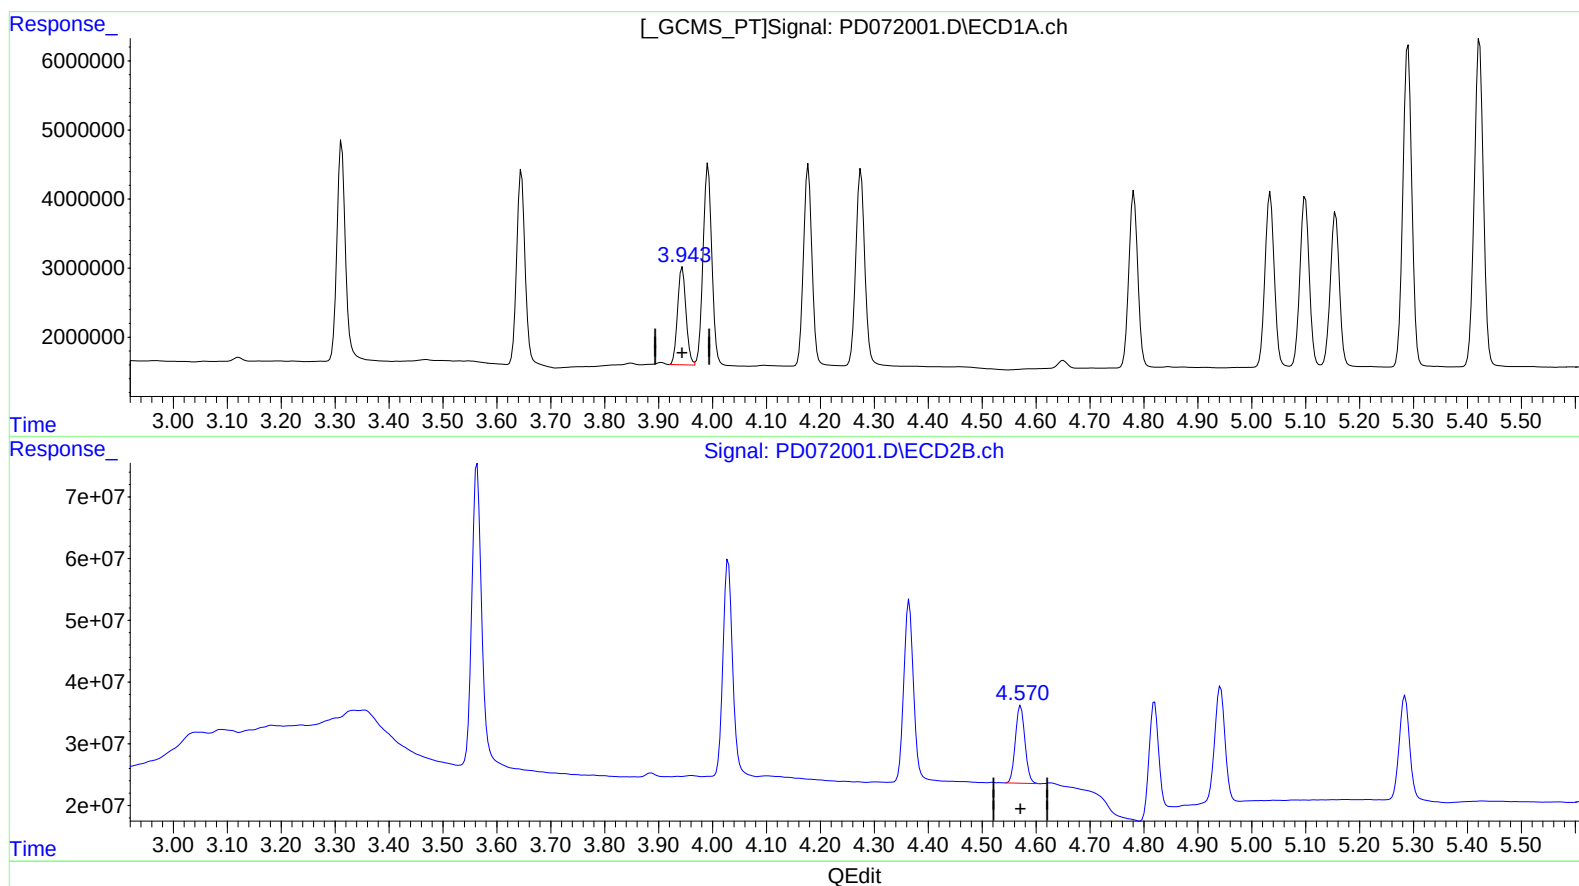

(6) beta-BHC (B)
3.944min 9.595 ng/ml
response 15357640

(6) beta-BHC #2 (B)
4.572min 10.410 ng/ml
response 154886961