

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092424\
 Data File : PD085597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 09:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 05:09:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445f	0.000	2781628	0	2.297	N.D. #
Target Compounds							
3)	MA gamma-BHC...	4.215f	0.000	292.2E6	0	116.787	N.D. #
8)	B Heptachlo...	5.604	0.000	2080293	0	1.041	N.D. #
15)	B Endosulfa...	6.691	0.000	9510120	0	5.187	N.D. #
16)	A 4,4'-DDD	6.691f	0.000	9510120	0	7.218	N.D. #
20)	A Methoxychlor	7.465f	0.000	987965	0	1.350	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092424\
Data File : PD085597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 09:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 05:09:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

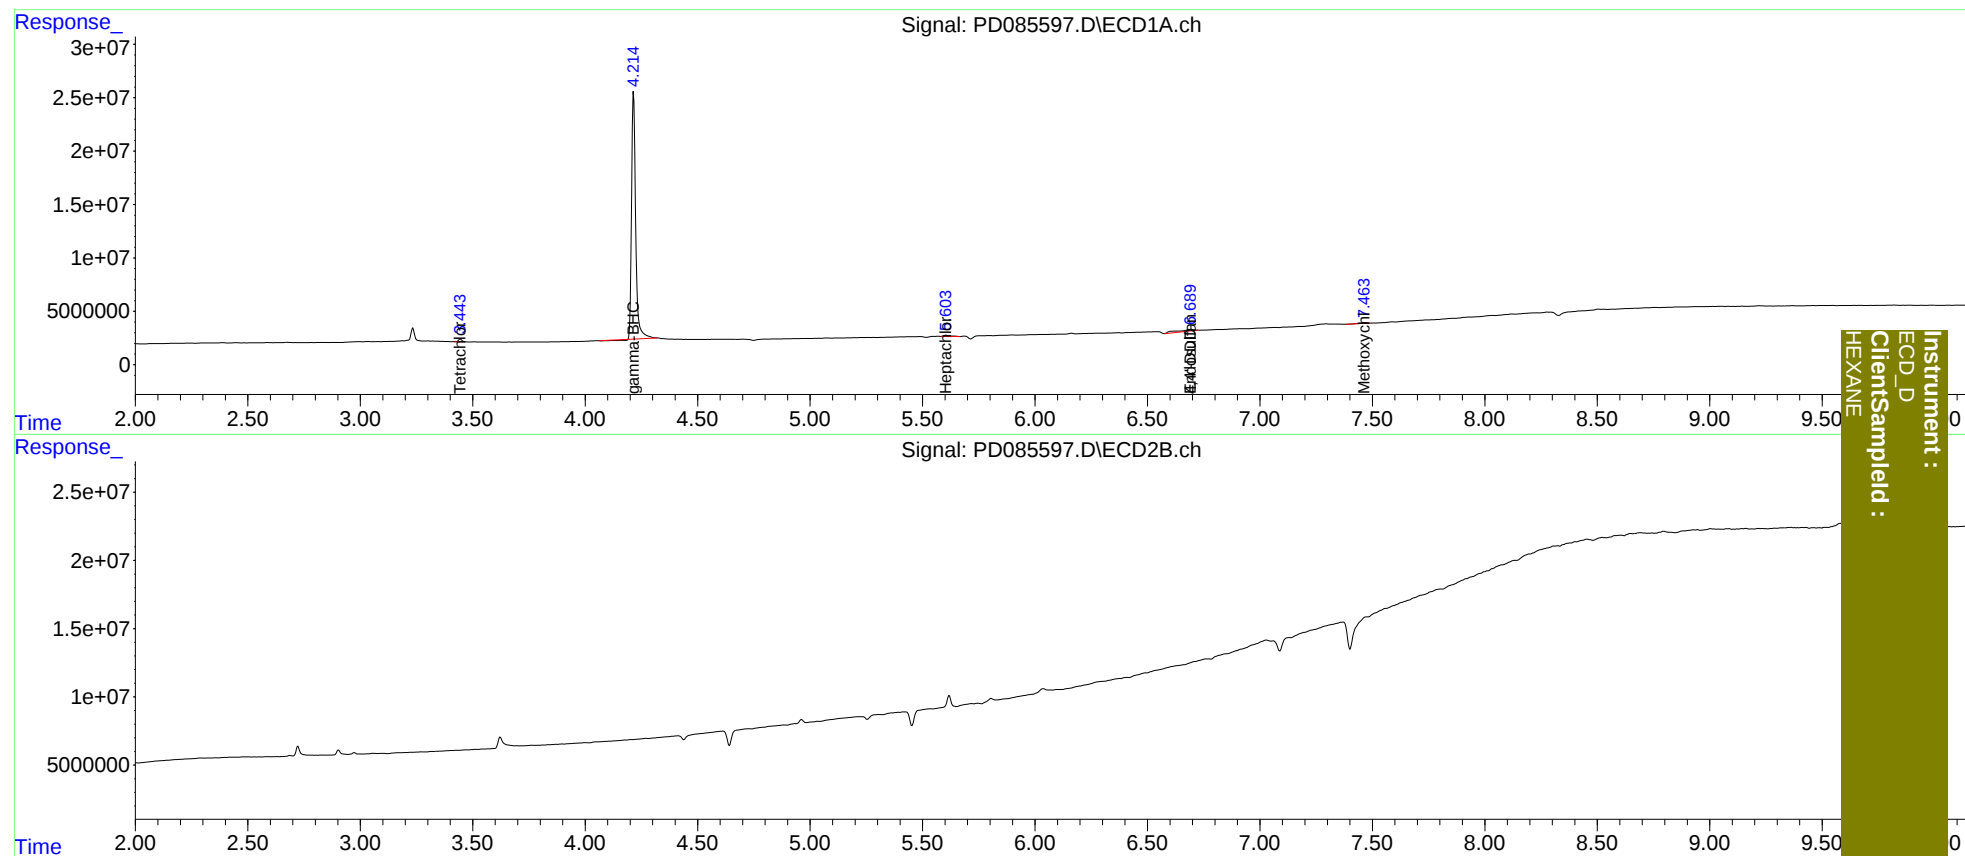


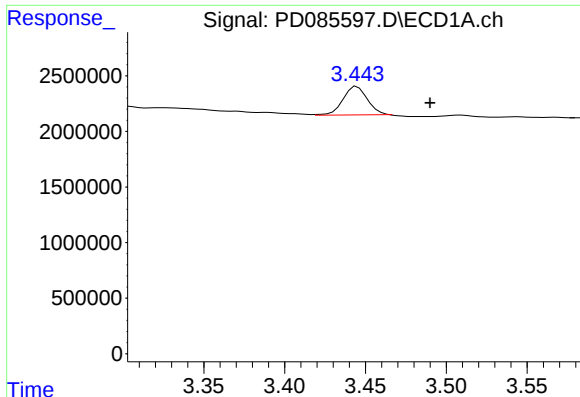

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: -0.045 min
Response: 2781628
Conc: 2.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

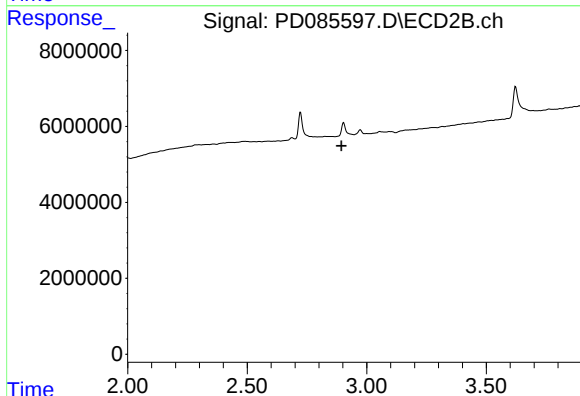


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.894 min
Response: 0
Conc: N.D.

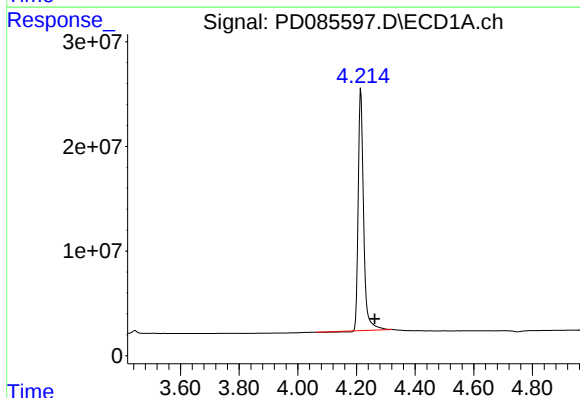


#3 gamma-BHC (Lindane)

R.T.: 4.215 min
Delta R.T.: -0.047 min
Response: 292181717
Conc: 116.79 ng/ml

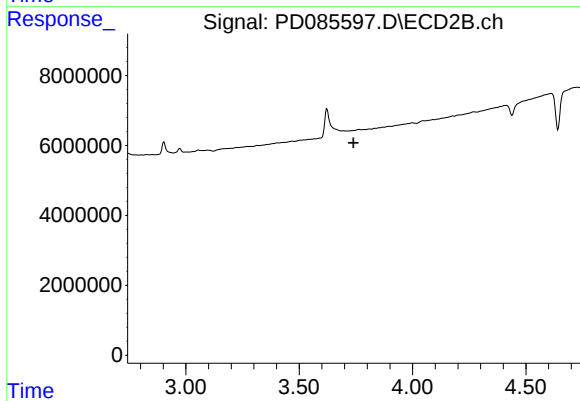

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.739 min
Response: 0
Conc: N.D.

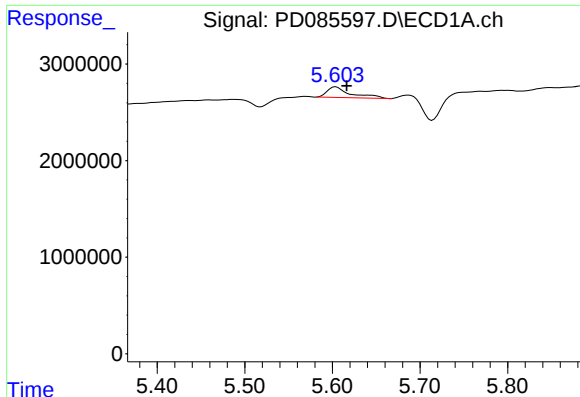

#8 Heptachlor epoxide


R.T.: 5.604 min
Delta R.T.: -0.012 min
Response: 2080293
Conc: 1.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

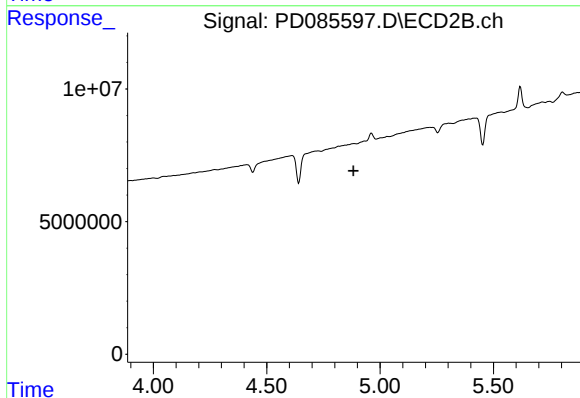


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.883 min
Response: 0
Conc: N.D.

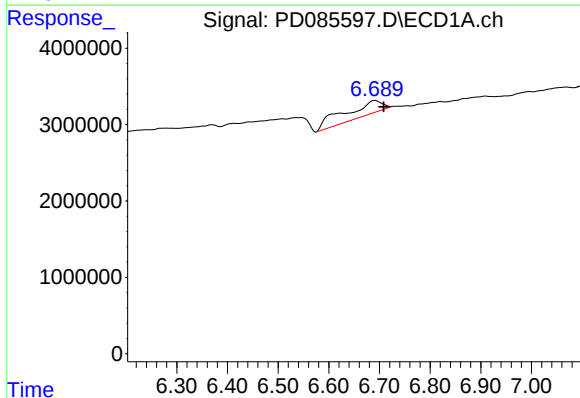


#15 Endosulfan II

R.T.: 6.691 min
Delta R.T.: -0.017 min
Response: 9510120
Conc: 5.19 ng/ml

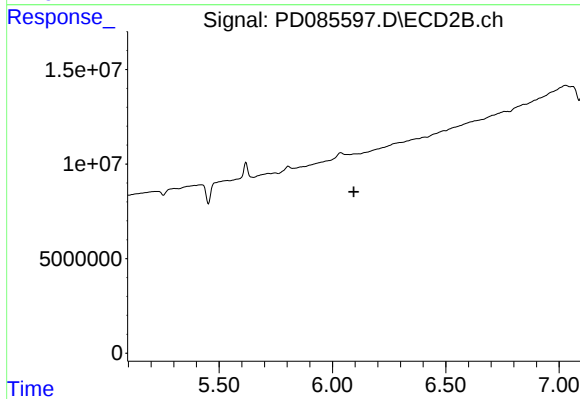

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

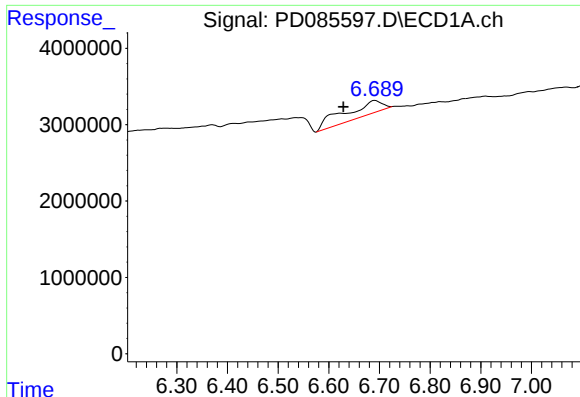

#16 4,4'-DDD


R.T.: 6.691 min
Delta R.T.: 0.062 min
Response: 9510120
Conc: 7.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

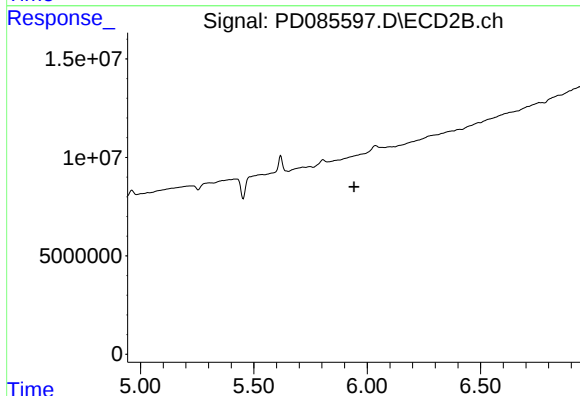


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.942 min
Response: 0
Conc: N.D.

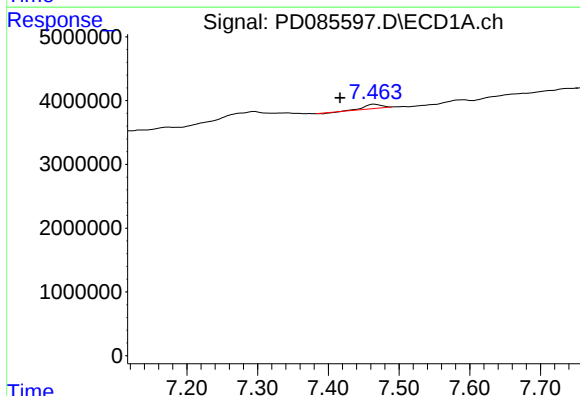


#20 Methoxychlor

R.T.: 7.465 min
Delta R.T.: 0.048 min
Response: 987965
Conc: 1.35 ng/ml

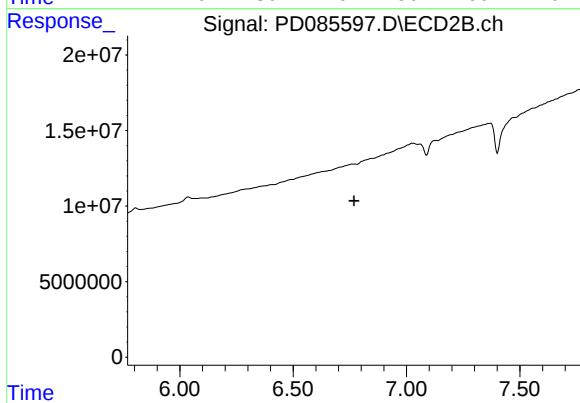

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

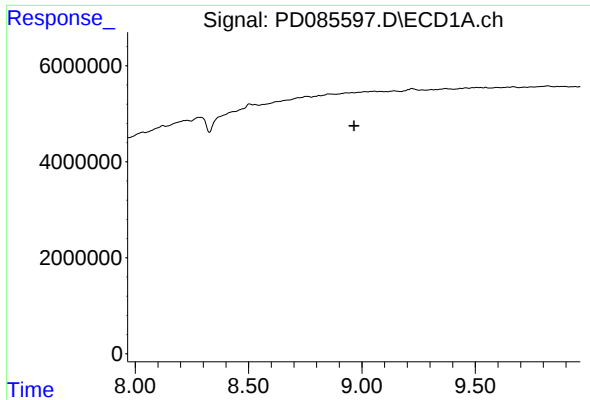

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

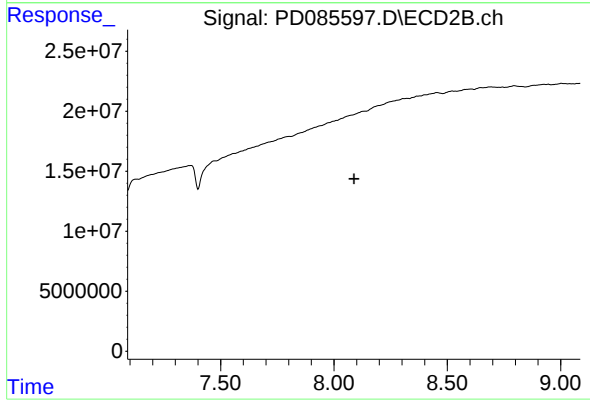

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.089 min
Response: 0
Conc: N.D.