

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092424\
 Data File : PD085601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 10:59
 Operator : AR\AJ
 Sample : P4017-03DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC42DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/07/2024
 Supervised By :Ankita Jodhani 10/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 05:10:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.901	5699610	102.3E6	4.707m	27.061m#
27)	SA Decachlor...	8.954	8.080	5057777	5310166	3.083m	1.986m#
Target Compounds							
2)	A alpha-BHC	3.931	3.401	187.2E6	353.5E6	79.235	64.013
6)	B beta-BHC	4.447	4.024	15785950	9605937	16.553m	4.131m#
7)	B delta-BHC	4.690	4.266	255.5E6	388.3E6	112.065	73.711m#
11)	B cis-Chlor...	5.937	5.202	24185366	59603853	12.064m	12.848
13)	MA Dieldrin	6.271	5.515	25928973	8897891	13.412m	1.911m#
14)	MA Endrin	6.468	5.798	21955234	64644044	13.656m	15.585m
16)	A 4,4'-DDD	6.623	5.937	81001218	136.0E6	61.479m	40.608m#
17)	MA 4,4'-DDT	6.933	6.189	36351027	106.3E6	29.820m	33.546m
20)	A Methoxychlor	7.404	6.749	18920010	58791630	25.859m	36.226m#
21)	B Endrin ke...	7.522	7.002	20010295	34793568	12.516m	7.491m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092424\
Data File : PD085601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 10:59
Operator : AR\AJ
Sample : P4017-03DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 05:10:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

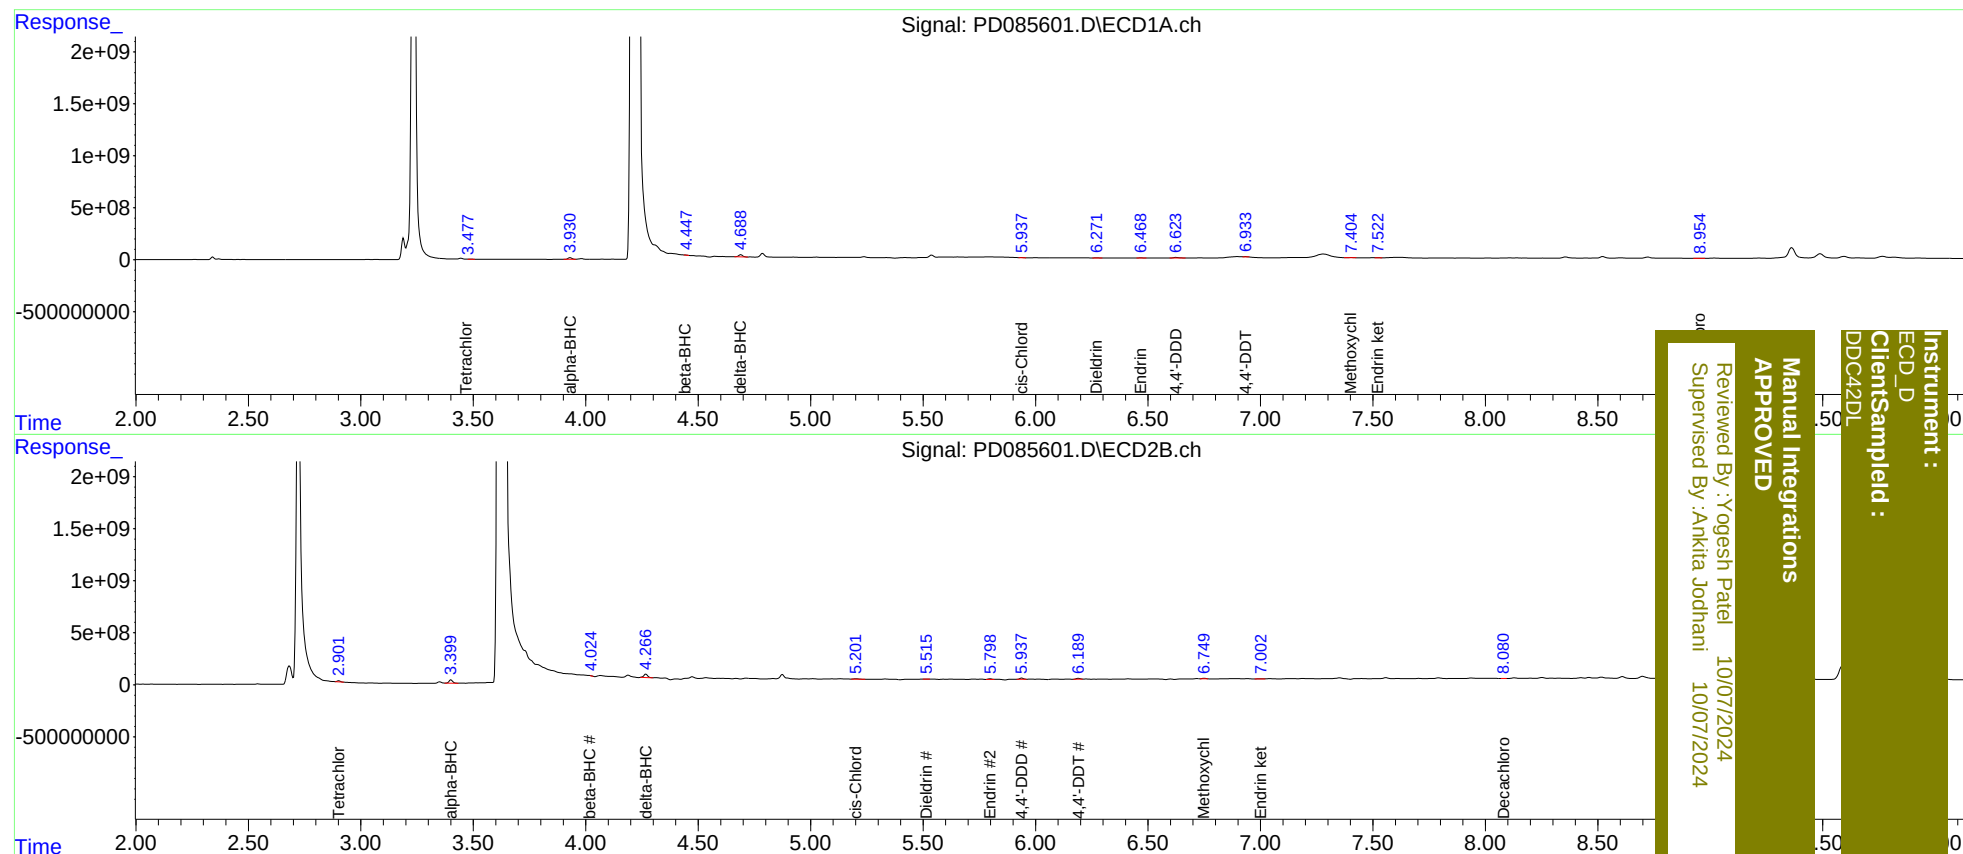

Instrument :
ECD_D
Client Sampled :
DDC42DL

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 10/07/2024
Supervised By : Ankita Jodhani 10/07/2024