

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092424\  
 Data File : PD085602.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Sep 2024 11:13  
 Operator : AR\AJ  
 Sample : P4017-04DL 2X  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 DDC43DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 10/07/2024  
 Supervised By :Ankita Jodhani 10/07/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 25 05:10:59 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD091924CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Sep 20 05:48:22 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|-----------|
| -----                       |                 |       |       |          |          |         |           |
| System Monitoring Compounds |                 |       |       |          |          |         |           |
| 1)                          | SA Tetrachlo... | 3.475 | 2.902 | 15268163 | 716.2E6  | 12.608m | 189.473m# |
| 27)                         | SA Decachlor... | 8.957 | 8.082 | 14394699 | 18937692 | 8.775   | 7.084m    |
| Target Compounds            |                 |       |       |          |          |         |           |
| 2)                          | A alpha-BHC     | 3.931 | 3.401 | 100.0E6  | 180.8E6  | 42.325  | 32.740    |
| 6)                          | B beta-BHC      | 4.442 | 4.026 | 4769834  | 13682475 | 5.002m  | 5.884m    |
| 7)                          | B delta-BHC     | 4.690 | 4.267 | 167.4E6  | 252.5E6  | 73.446  | 47.933 #  |
| 9)                          | A Endosulfan I  | 5.996 | 5.259 | 6930255  | 11047231 | 3.910m  | 2.688m#   |
| 10)                         | B trans-Chl...  | 5.864 | 5.132 | 5832890  | 16513280 | 3.065m  | 3.649m    |
| 14)                         | MA Endrin       | 6.469 | 5.798 | 8279564  | 25997508 | 5.150m  | 6.268m    |
| 16)                         | A 4,4'-DDD      | 6.623 | 5.938 | 51597523 | 100.7E6  | 39.162m | 30.059    |
| 17)                         | MA 4,4'-DDT     | 6.942 | 6.189 | 9872466  | 48638812 | 8.099m  | 15.356m#  |
| -----                       |                 |       |       |          |          |         |           |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092424\  
Data File : PD085602.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Sep 2024 11:13  
Operator : AR\AJ  
Sample : P4017-04DL 2X  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 25 05:10:59 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD091924CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Sep 20 05:48:22 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

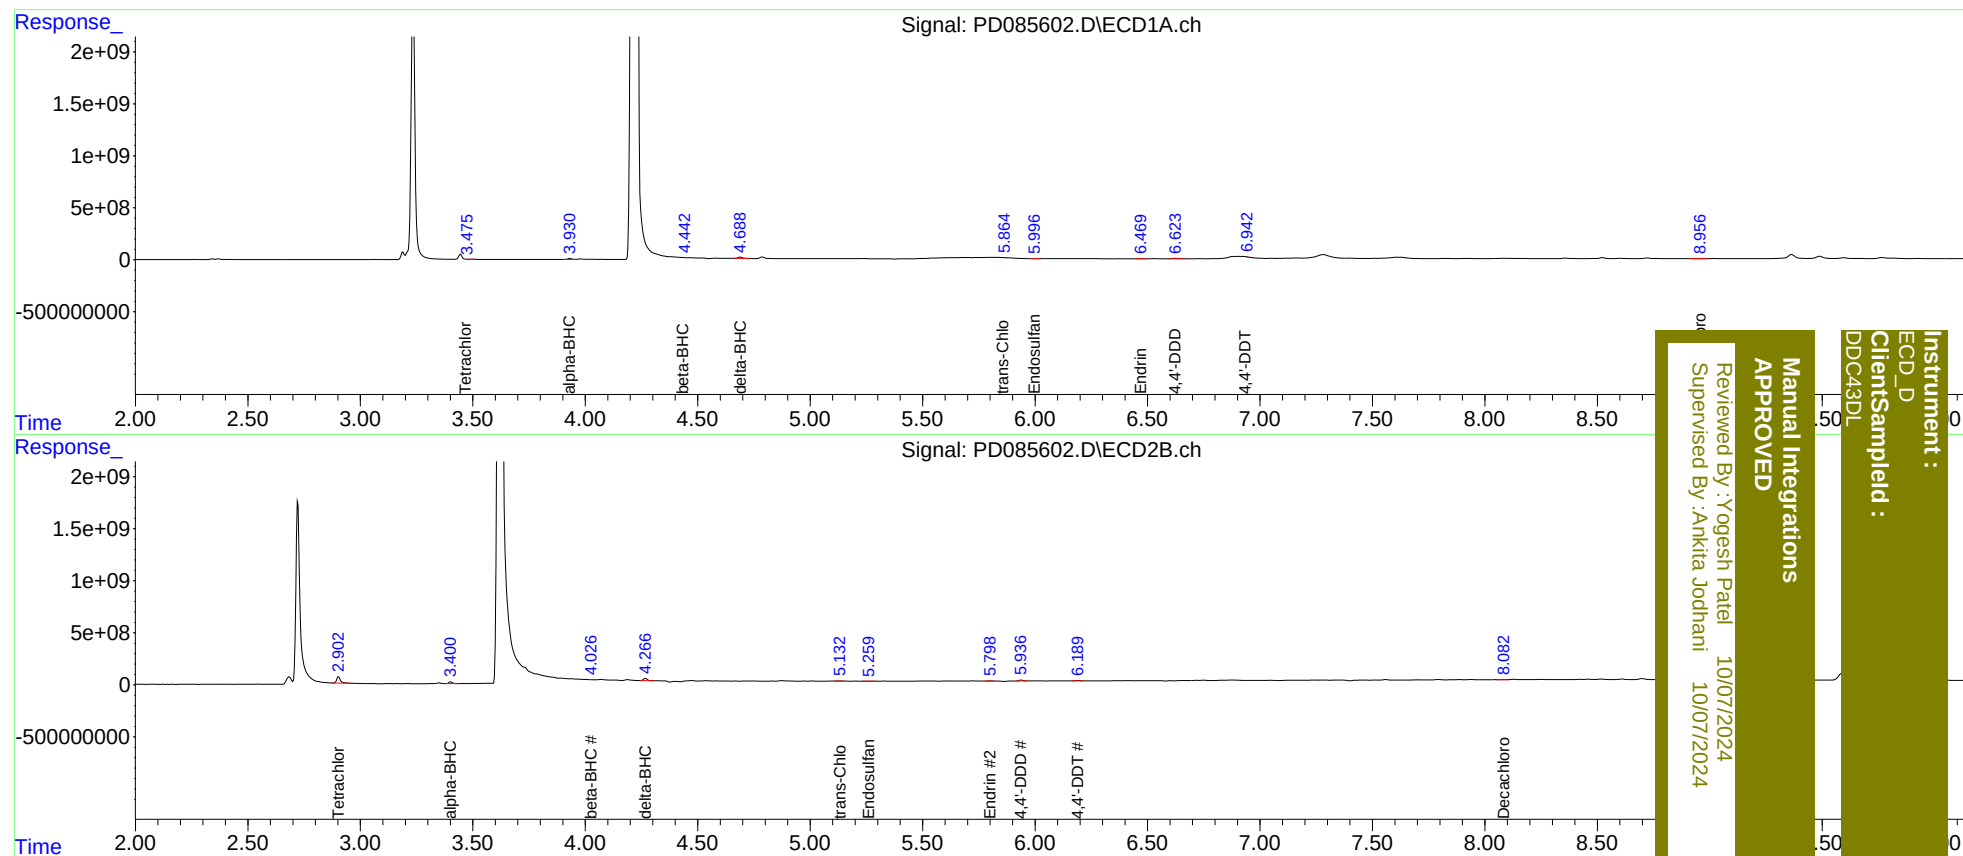

Manual Integrations  
APPROVED  
Reviewed By : Yogesh Patel 10/07/2024  
Supervised By : Ankita Jodhani 10/07/2024

Instrument :  
ECD\_D  
ClientSampled :  
DDC43DL