

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092424\  
 Data File : PD085620.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Sep 2024 17:21  
 Operator : AR\AJ  
 Sample : INDA337  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3236

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 09/26/2024  
 Supervised By :Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 25 05:18:00 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD091924CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Sep 20 05:48:22 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-------|-------|----------|----------|---------|---------|
| -----                       |       |       |          |          |         |         |
| System Monitoring Compounds |       |       |          |          |         |         |
| 1) SA Tetrachlo...          | 3.486 | 2.892 | 24794441 | 76419839 | 20.475m | 20.218  |
| 27) SA Decachlor...         | 8.959 | 8.083 | 65911523 | 123.0E6  | 40.179  | 46.025  |
| Target Compounds            |       |       |          |          |         |         |
| 2) A alpha-BHC              | 3.932 | 3.402 | 47076742 | 112.4E6  | 19.925  | 20.363  |
| 3) MA gamma-BHC...          | 4.259 | 3.737 | 57658805 | 107.3E6  | 23.047  | 20.586  |
| 4) MA Heptachlor            | 4.854 | 4.090 | 43555599 | 99156003 | 20.627  | 20.889  |
| 9) A Endosulfan I           | 5.993 | 5.254 | 38279076 | 89903974 | 21.598m | 21.878m |
| 13) MA Dieldrin             | 6.266 | 5.522 | 84999229 | 201.9E6  | 43.966  | 43.362  |
| 14) MA Endrin               | 6.492 | 5.799 | 69636790 | 175.8E6  | 43.312  | 42.394  |
| 16) A 4,4'-DDD              | 6.626 | 5.938 | 56063242 | 143.0E6  | 42.551  | 42.707  |
| 17) MA 4,4'-DDT             | 6.939 | 6.193 | 58668054 | 154.3E6  | 48.127m | 48.709  |
| 20) A Methoxychlor          | 7.413 | 6.764 | 167.2E6  | 378.7E6  | 228.490 | 233.356 |
| -----                       |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD092424\  
Data File : PD085620.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Sep 2024 17:21  
Operator : AR\AJ  
Sample : INDA337  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 25 05:18:00 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD091924CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Sep 20 05:48:22 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

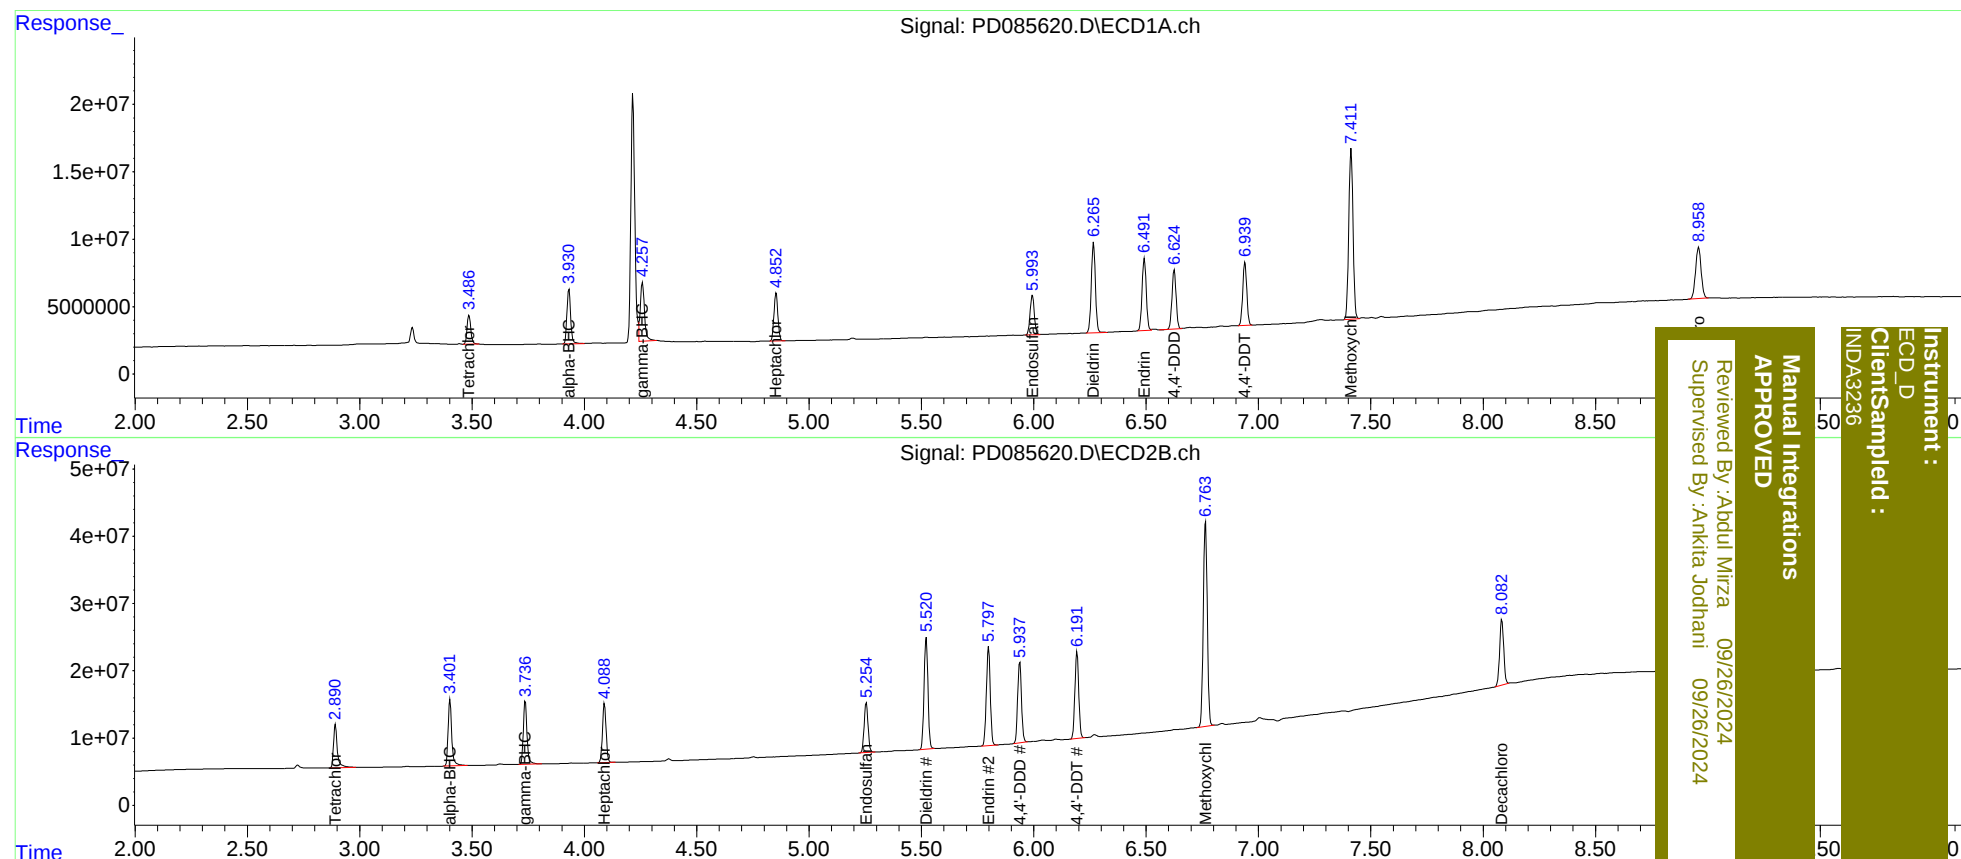

Manual Integrations  
APPROVED  
Reviewed By: Abdul Mirza 09/26/2024  
Supervised By: Ankita Jodhani 09/26/2024

Instrument :  
ECD\_D  
Client Sampled :  
INDA3236