

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092519\
 Data File : PD054949.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2019 9:20
 Operator : SG\AJ
 Sample : MDL-BL-S
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-BL-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 10:29:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.297	3.966	16552445	23054222	21.757	22.466
27)	SA Decachlor...	7.977	9.004	32304933	42706623	38.340	36.656


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092519\
Data File : PD054949.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2019 9:20
Operator : SG\AJ
Sample : MDL-BL-S
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 10:29:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

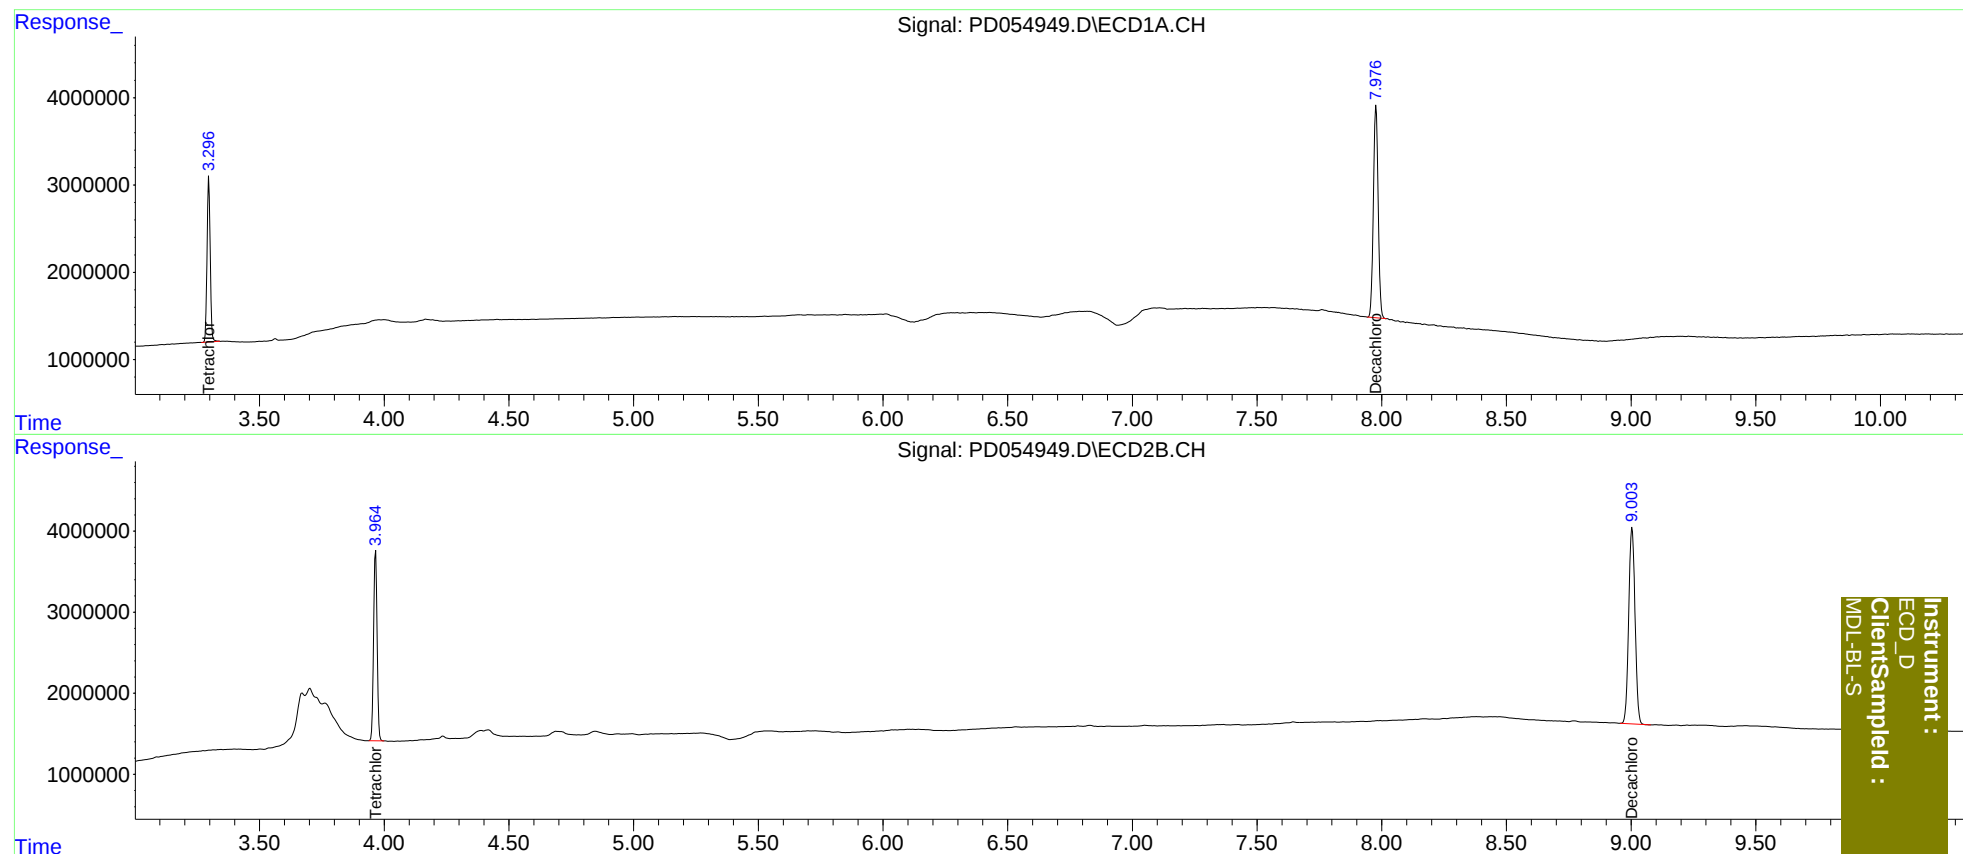


Instrument :
ECD_D
ClientSampled :
MDL-BL-S

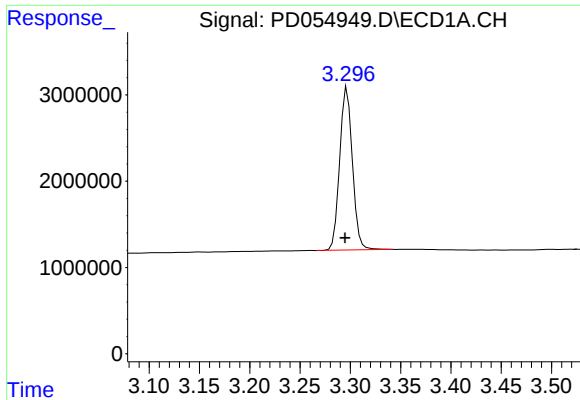

#1 Tetrachloro-m-xylene


R.T.: 3.297 min
Delta R.T.: 0.002 min
Response: 16552445
Conc: 21.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-S

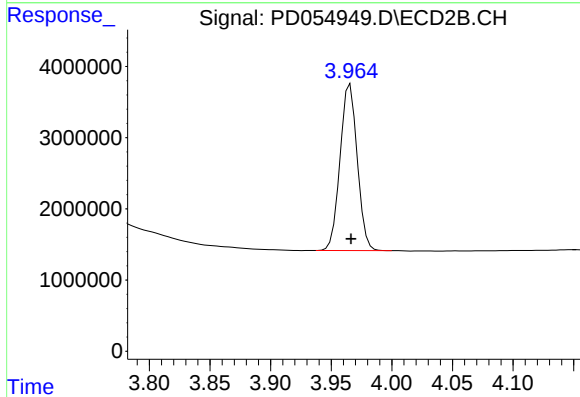


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 23054222
Conc: 22.47 ng/ml

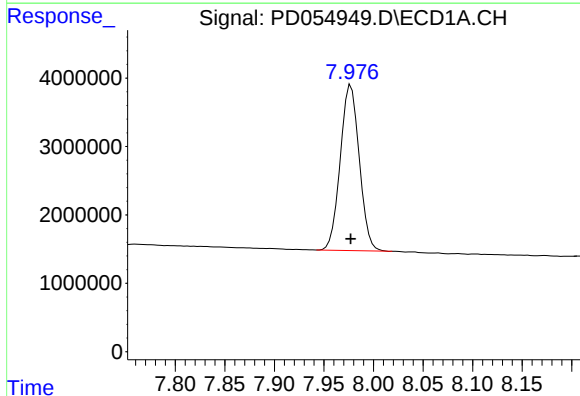

#27 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: 0.000 min
Response: 32304933
Conc: 38.34 ng/ml

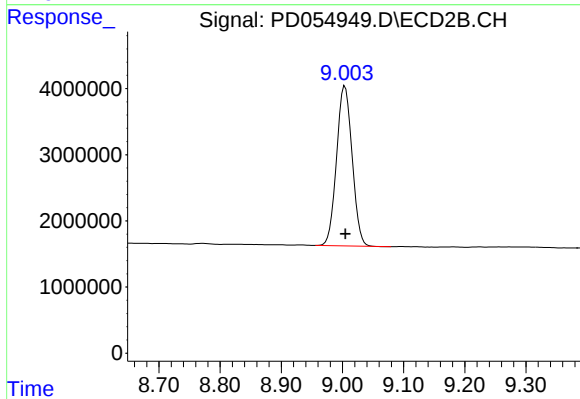

#27 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.000 min
Response: 42706623
Conc: 36.66 ng/ml