

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092520\
 Data File : PD059331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2020 11:10
 Operator : DD\AJ
 Sample : L1955-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 MDL-WATER-02

Manual Integrations
 APPROVED

Ankita
 9/29/2020 9:08:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 08:11:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.025	25293715	35352259	20.165	21.009
27)	SA Decachlor...	8.324	9.109	33646232	49523363	39.871	43.503
Target Compounds							
2)	A alpha-BHC	3.955	4.416	2337728	1804006	1.325	0.737 #
3)	MA gamma-BHC...	4.240	4.701	2395636	2483384	1.420m	1.110
4)	MA Heptachlor	4.551	5.213	1936335	2104432	1.169	0.972
5)	MB Aldrin	4.804	5.520	1767151	1917516	1.093	0.949
6)	B beta-BHC	4.491	4.869	1055726	800117	1.368	0.791 #
7)	B delta-BHC	4.700	5.087	1779871	2303636	1.077	1.013
8)	B Heptachlo...	5.250	5.905	1760942	3886913	1.231m	2.066m#
9)	A Endosulfan I	5.594	6.264	1518363	2058456	1.181	1.242
10)	B trans-Chl...	5.480	6.140	1567686	2183320	1.110m	1.198
11)	B cis-Chlor...	5.540	6.214	1676816	1971091	1.191	1.092
12)	B 4,4'-DDE	5.705	6.368	1477341	1834910	1.109	1.074
13)	MA Dieldrin	5.840	6.521	1496431	2140900	1.110	1.206
14)	MA Endrin	6.099	6.740	872053	1147142	0.883	0.894
15)	B Endosulfa...	6.373	6.948	1256212	1669250	1.169	1.170
16)	A 4,4'-DDD	6.224	6.858	1282875	1491462	1.235m	1.105
17)	MA 4,4'-DDT	6.469	7.156	984476	1239091	0.935	1.115m
18)	B Endrin al...	6.542	7.071	1174992	1203624	1.326m	1.020
19)	B Endosulfa...	6.758	7.295	806072	1623775	0.794	1.114 #
20)	A Methoxychlor	7.026	7.615	563875	648405	1.144	1.046
21)	B Endrin ke...	7.253	7.765	1537438	1650537	1.428	1.179m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092520\
Data File : PD059331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2020 11:10
Operator : DD\AJ
Sample : L1955-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 08:11:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

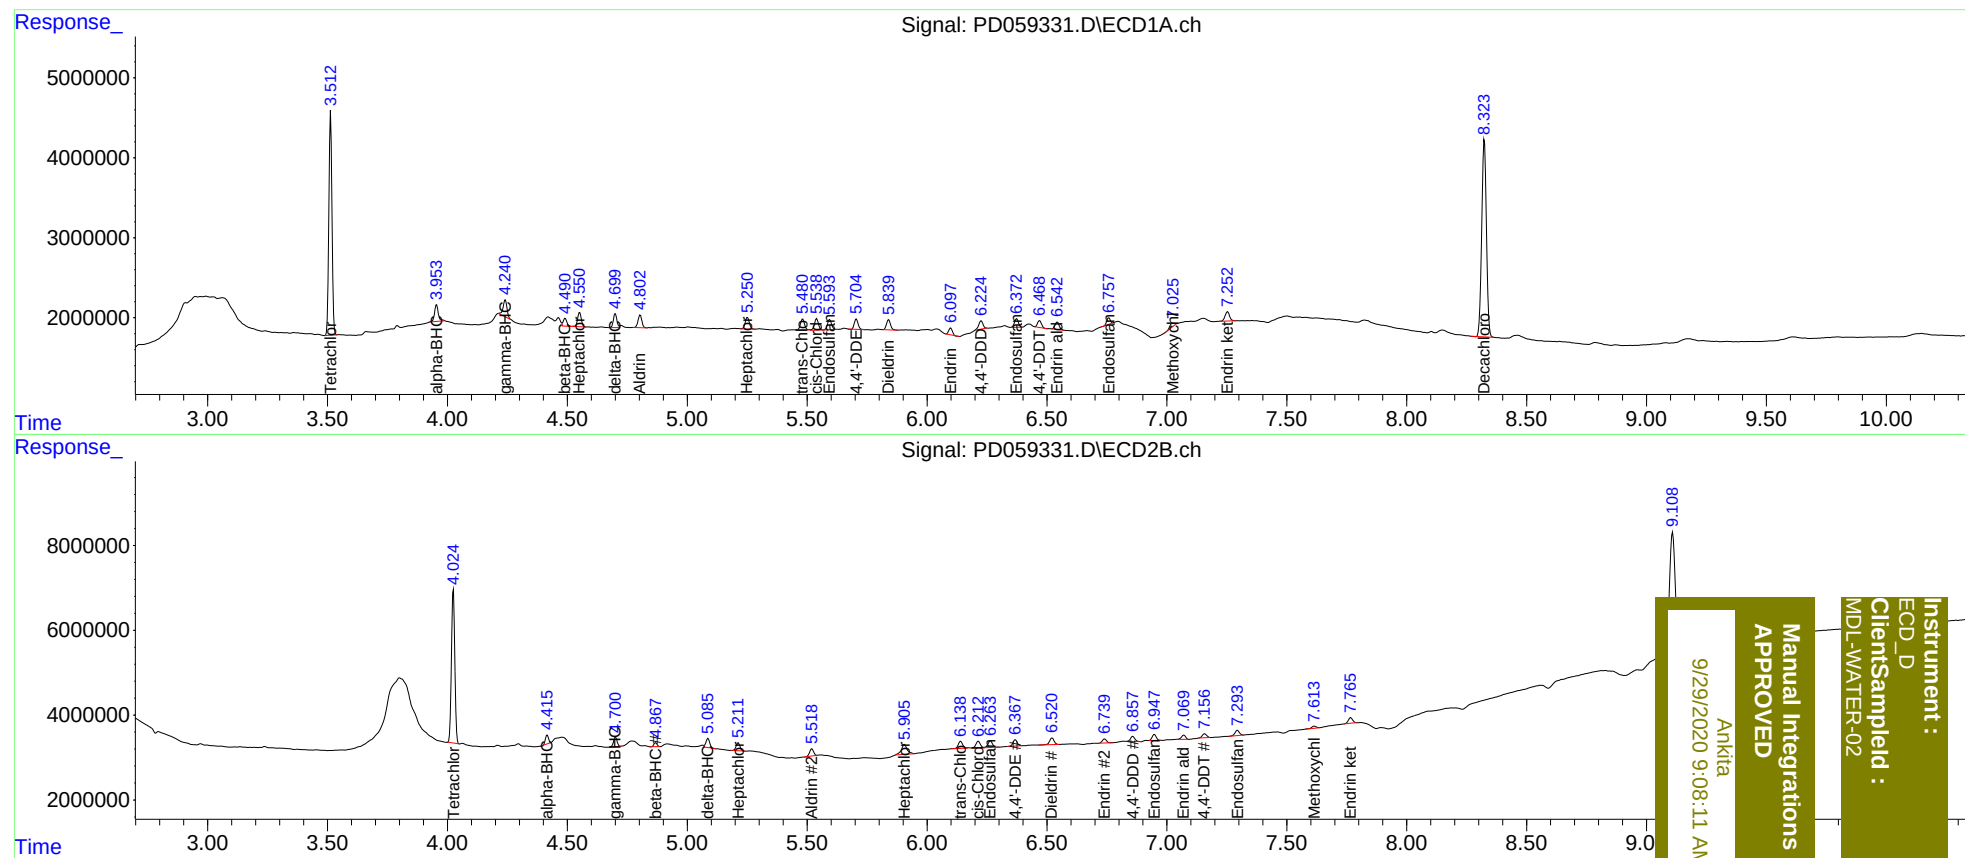

Manual Integrations
APPROVED

Ankita
9/29/2020 9:08:11 AM

Instrument :
ECD_D
Client Sample :
MDL-WATER-02