

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092521\
 Data File : PD065861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2021 16:07
 Operator : AR\AJ
 Sample : M3916-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 05:15:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	21154128	156.4E6	28.565	27.237
28)	SA Decachlor...	8.234	9.085	29161123	92803847	21.349	23.979
Target Compounds							
2)	A alpha-BHC	3.943	4.412	1124885	3086281	1.002	0.367 #
5)	MB Aldrin	0.000	5.482f	0	1034710	N.D.	0.154 #
6)	B beta-BHC	0.000	4.898f	0	1129254	N.D.	0.306 #
7)	B delta-BHC	0.000	5.092	0	1670272	N.D.	0.232 #
15)	B Endosulfa...	6.322	6.945	753588	1290131	0.698	0.266 #
21)	B Endrin ke...	0.000	7.735f	0	5632684	N.D.	0.988 #
24)	Chlordane-2	0.000	5.482	0	1034710	N.D.	4.473 #
27)	Chlordane-5	6.322	0.000	753588	0	15.506	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092521\
Data File : PD065861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2021 16:07
Operator : AR\AJ
Sample : M3916-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 05:15:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

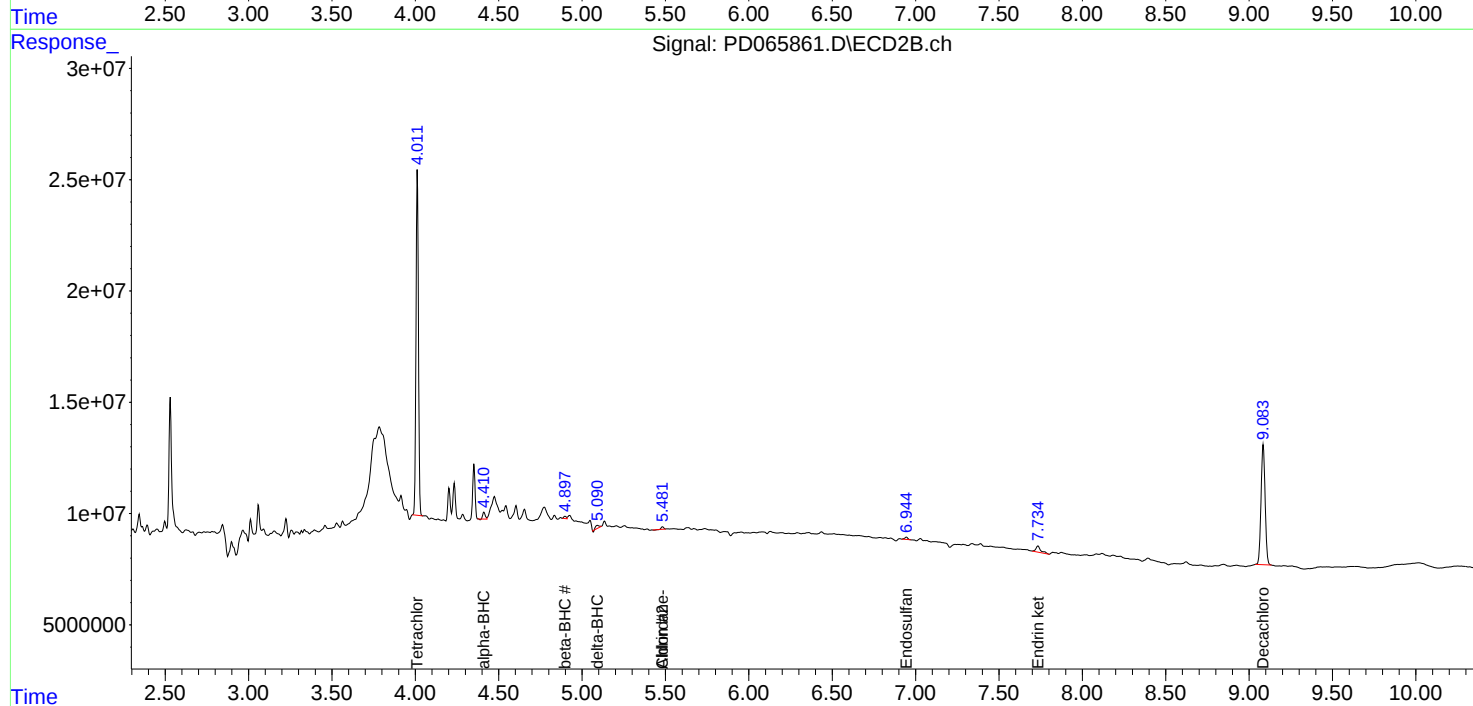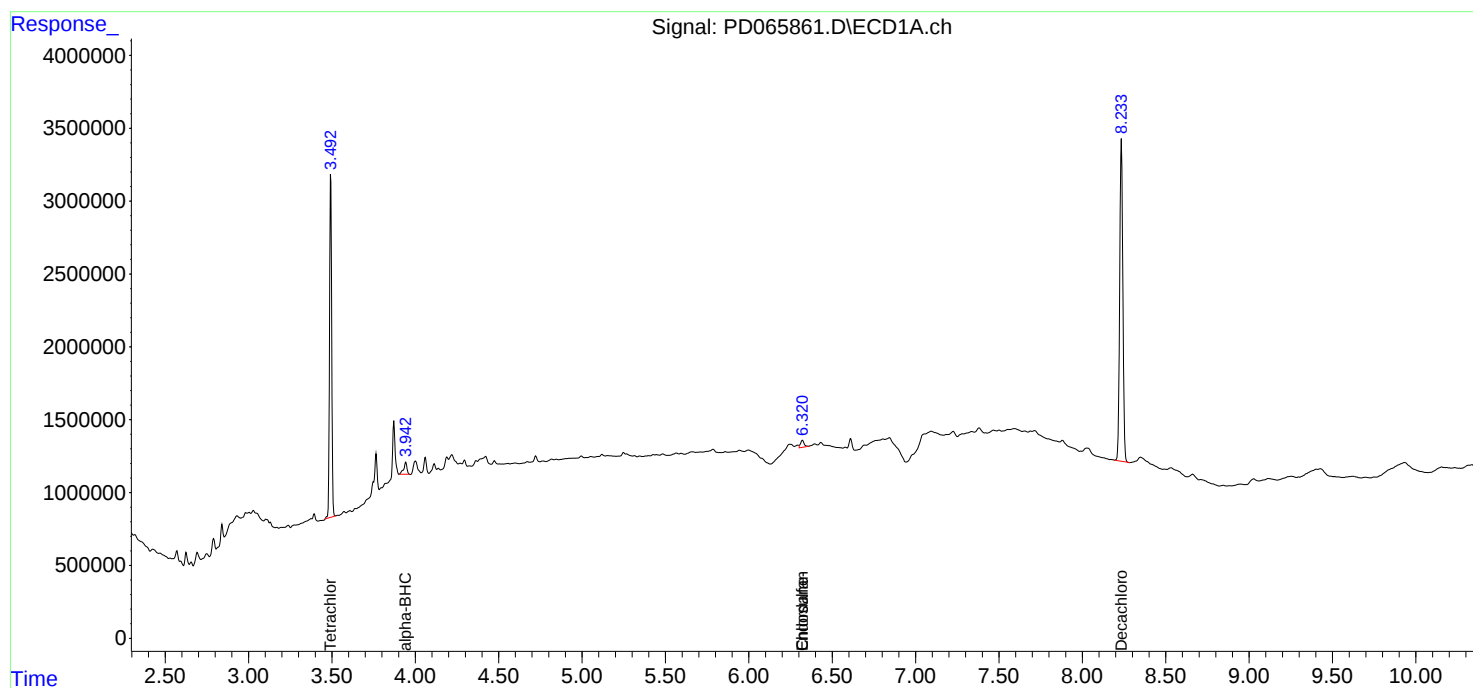


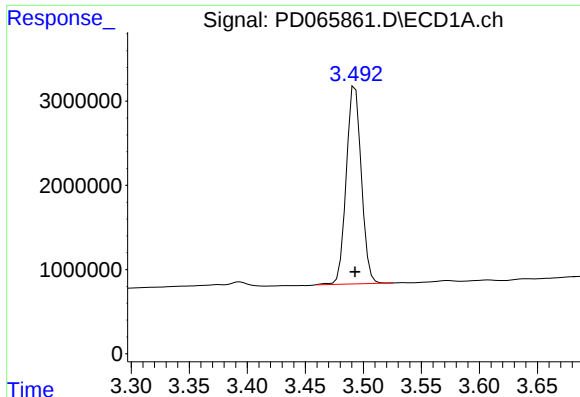

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 21154128
Conc: 28.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

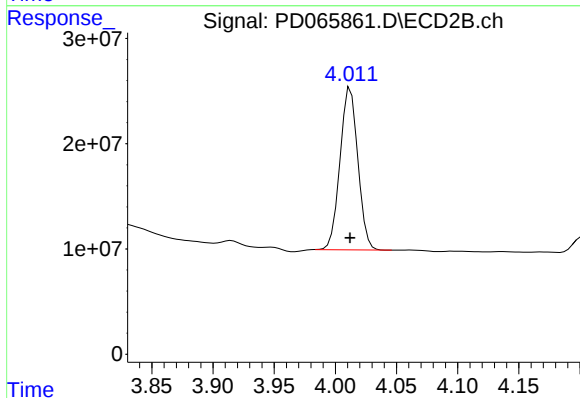


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 156398015
Conc: 27.24 ng/ml

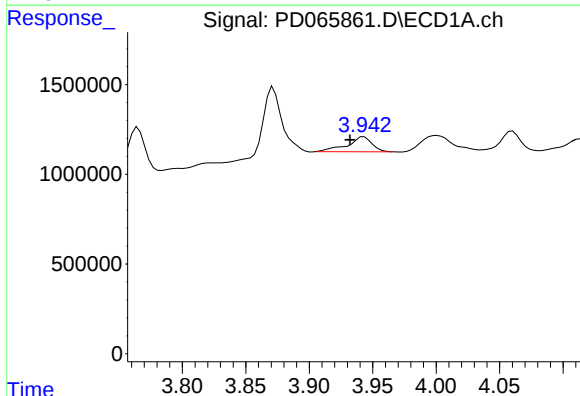


#2 alpha-BHC

R.T.: 3.943 min
Delta R.T.: 0.011 min
Response: 1124885
Conc: 1.00 ng/ml

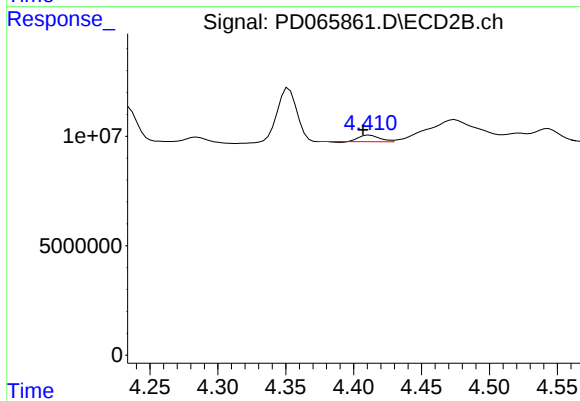

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.005 min
Response: 3086281
Conc: 0.37 ng/ml

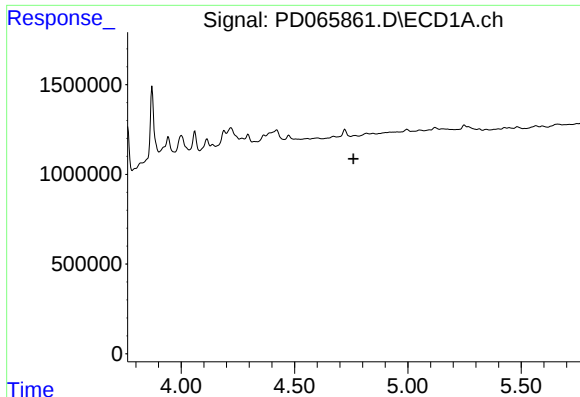

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.761 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

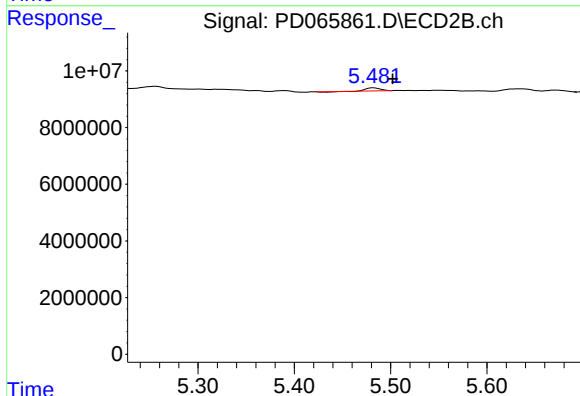


#5 Aldrin

R.T.: 5.482 min
Delta R.T.: -0.020 min
Response: 1034710
Conc: 0.15 ng/ml

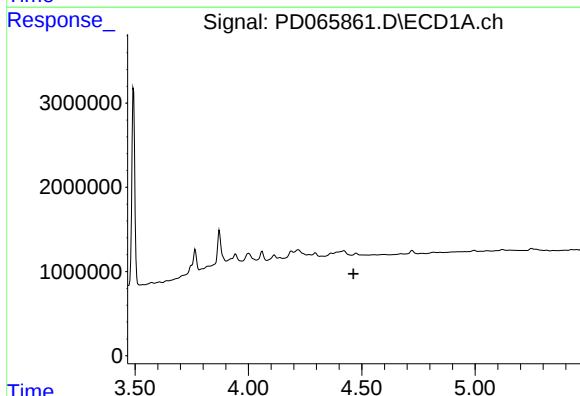


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.464 min
Response: 0
Conc: N.D.

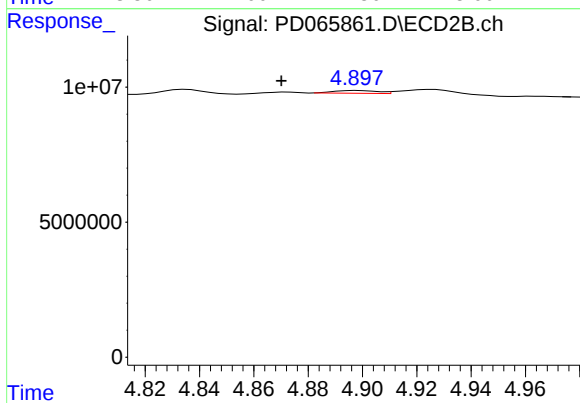

#6 beta-BHC


R.T.: 4.898 min
Delta R.T.: 0.028 min
Response: 1129254
Conc: 0.31 ng/ml

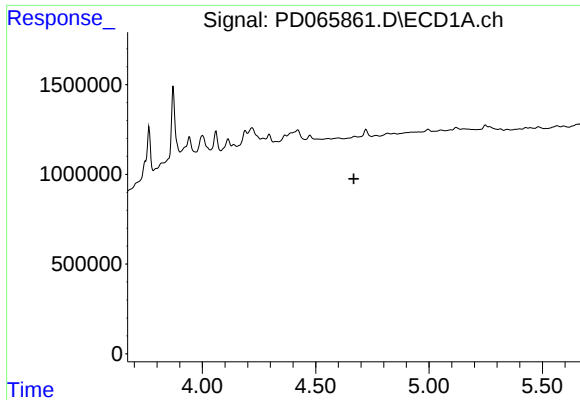

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.668 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

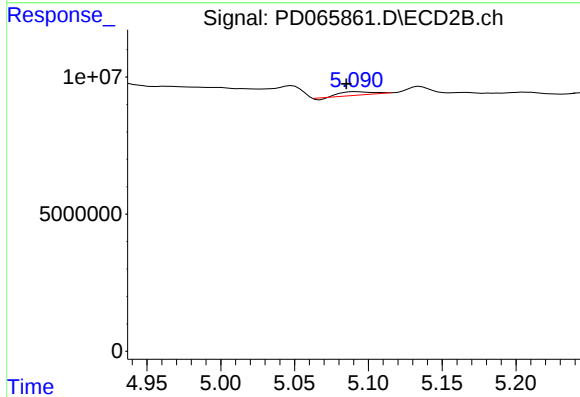


#7 delta-BHC

R.T.: 5.092 min
Delta R.T.: 0.007 min
Response: 1670272
Conc: 0.23 ng/ml

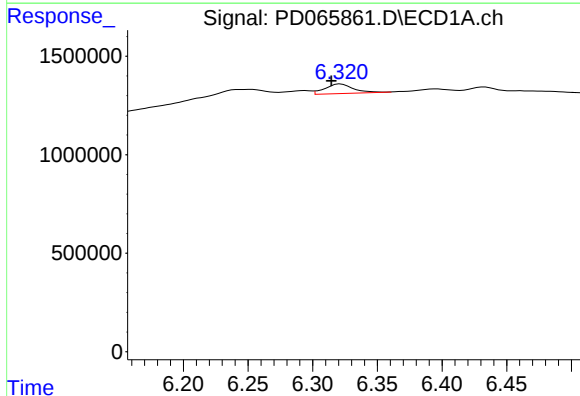


#15 Endosulfan II

R.T.: 6.322 min
Delta R.T.: 0.007 min
Response: 753588
Conc: 0.70 ng/ml

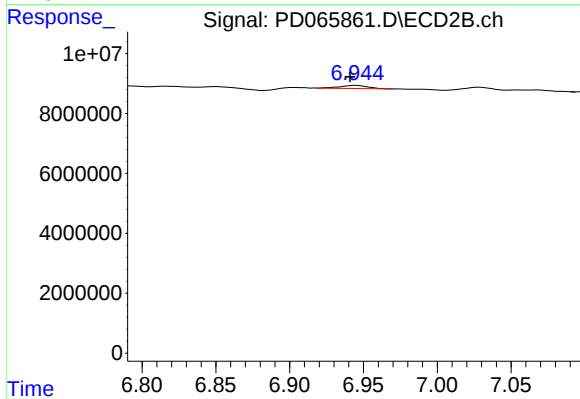

#15 Endosulfan II


R.T.: 6.945 min
Delta R.T.: 0.004 min
Response: 1290131
Conc: 0.27 ng/ml

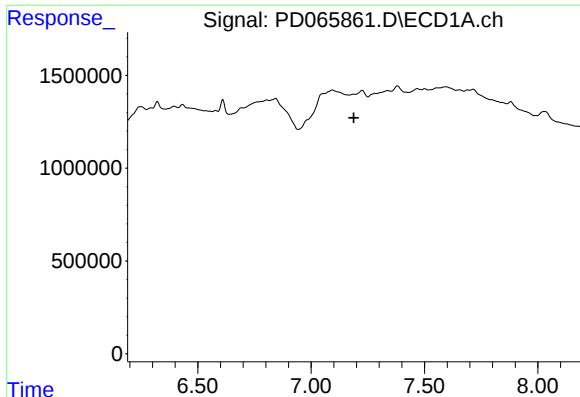

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

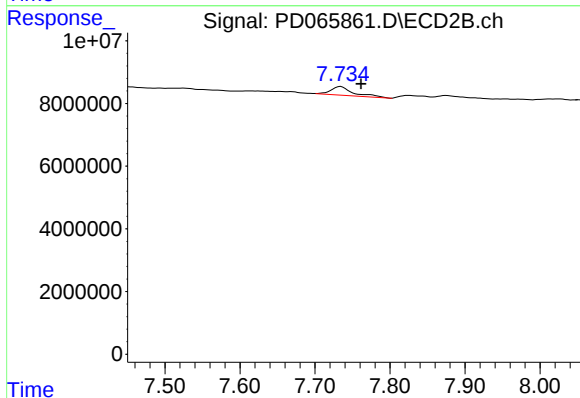


#21 Endrin ketone

R.T.: 7.735 min
Delta R.T.: -0.027 min
Response: 5632684
Conc: 0.99 ng/ml

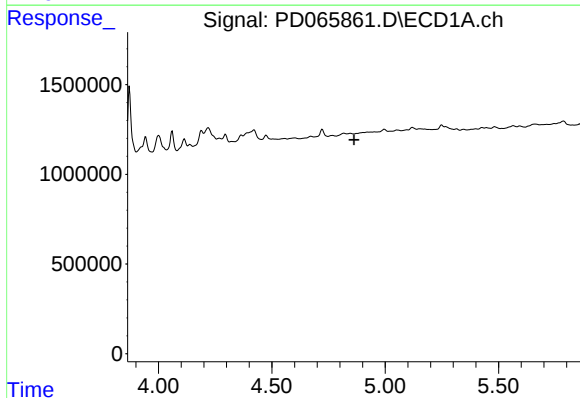


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

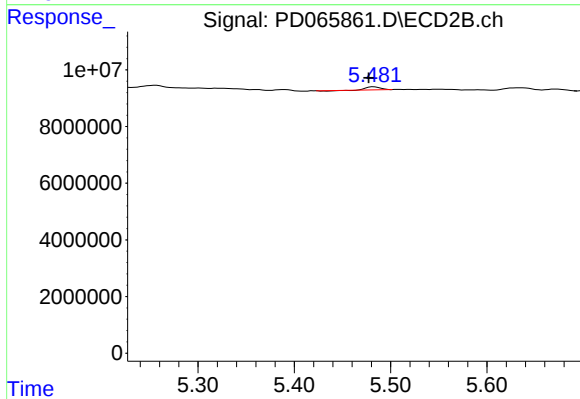

#24 Chlordane-2


R.T.: 5.482 min
Delta R.T.: 0.005 min
Response: 1034710
Conc: 4.47 ng/ml

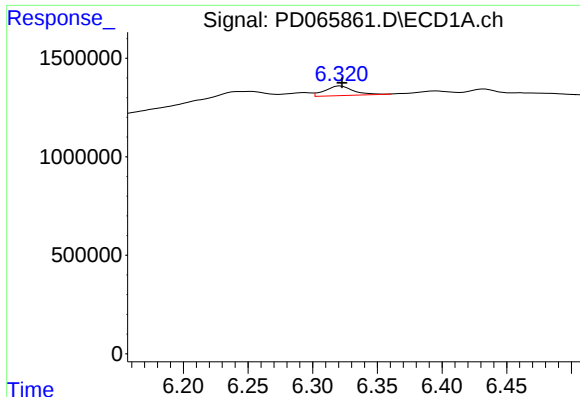

#27 Chlordane-5


R.T.: 6.322 min
Delta R.T.: -0.001 min
Response: 753588
Conc: 15.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

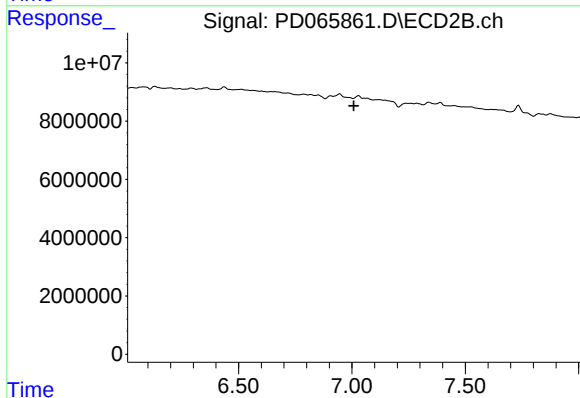


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

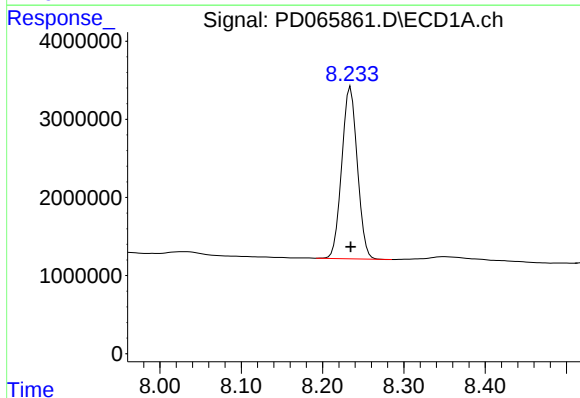

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 29161123
Conc: 21.35 ng/ml

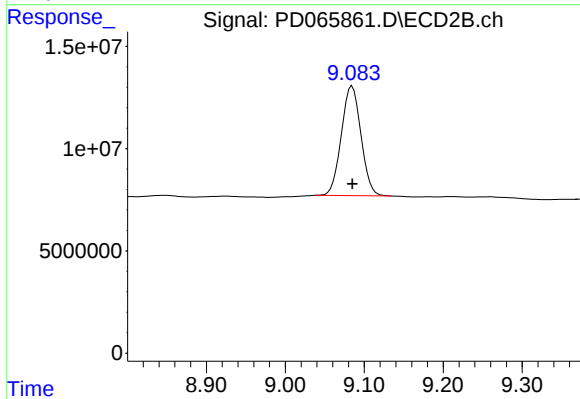

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 92803847
Conc: 23.98 ng/ml