

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092521\
 Data File : PD065872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2021 23:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 05:18:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.011	18845189	149.0E6	25.447	25.952
28)	SA Decachlor...	8.241	9.087	28383327	89440240	20.779	23.110
Target Compounds							
6)	B beta-BHC	4.479f	0.000	570034	0	0.999	N.D. #
15)	B Endosulfa...	6.325	0.000	1483993	0	1.374	N.D. #
19)	B Endosulfa...	6.693	0.000	1423460	0	1.247	N.D. #
22)	Mirex	7.387	8.230f	3048840	5725345	2.525	1.450 #
27)	Chlordane-5	6.325	0.000	1483993	0	30.535	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092521\
Data File : PD065872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2021 23:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 05:18:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

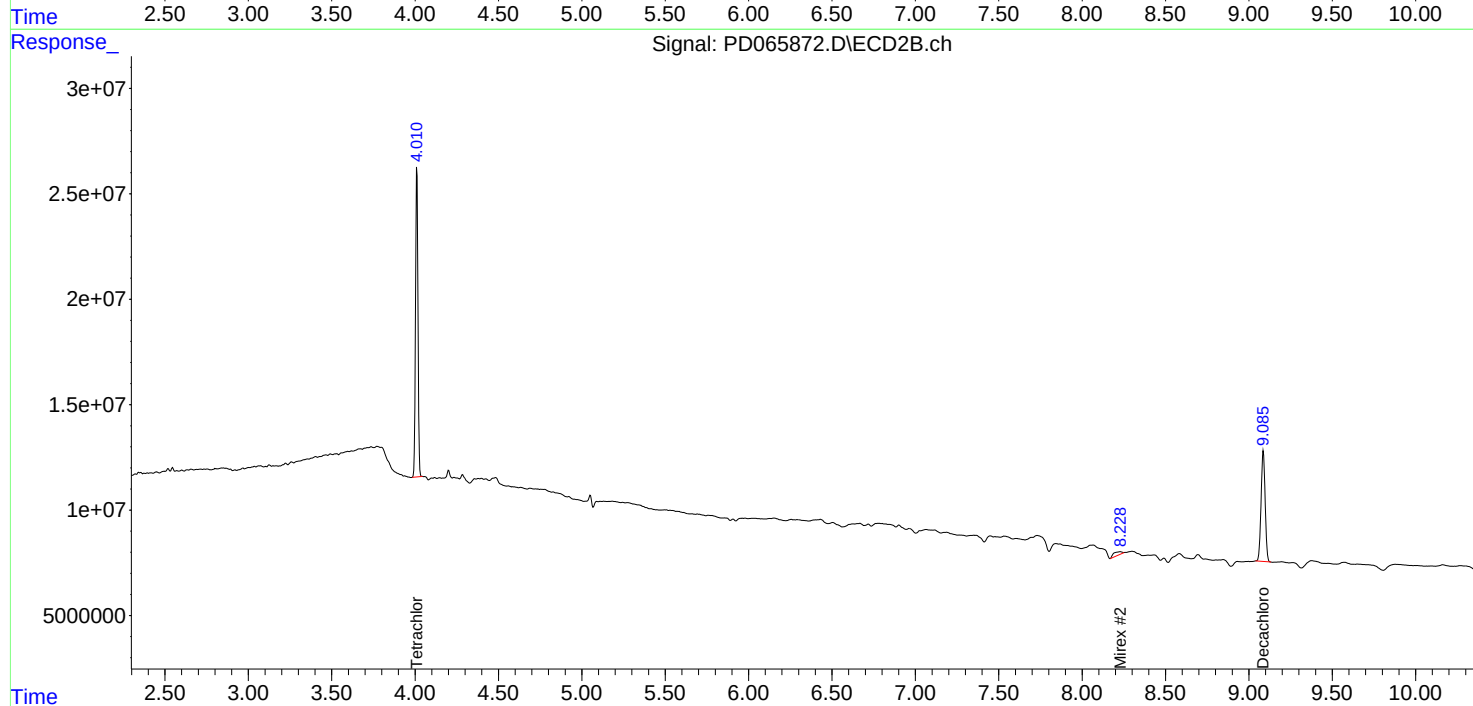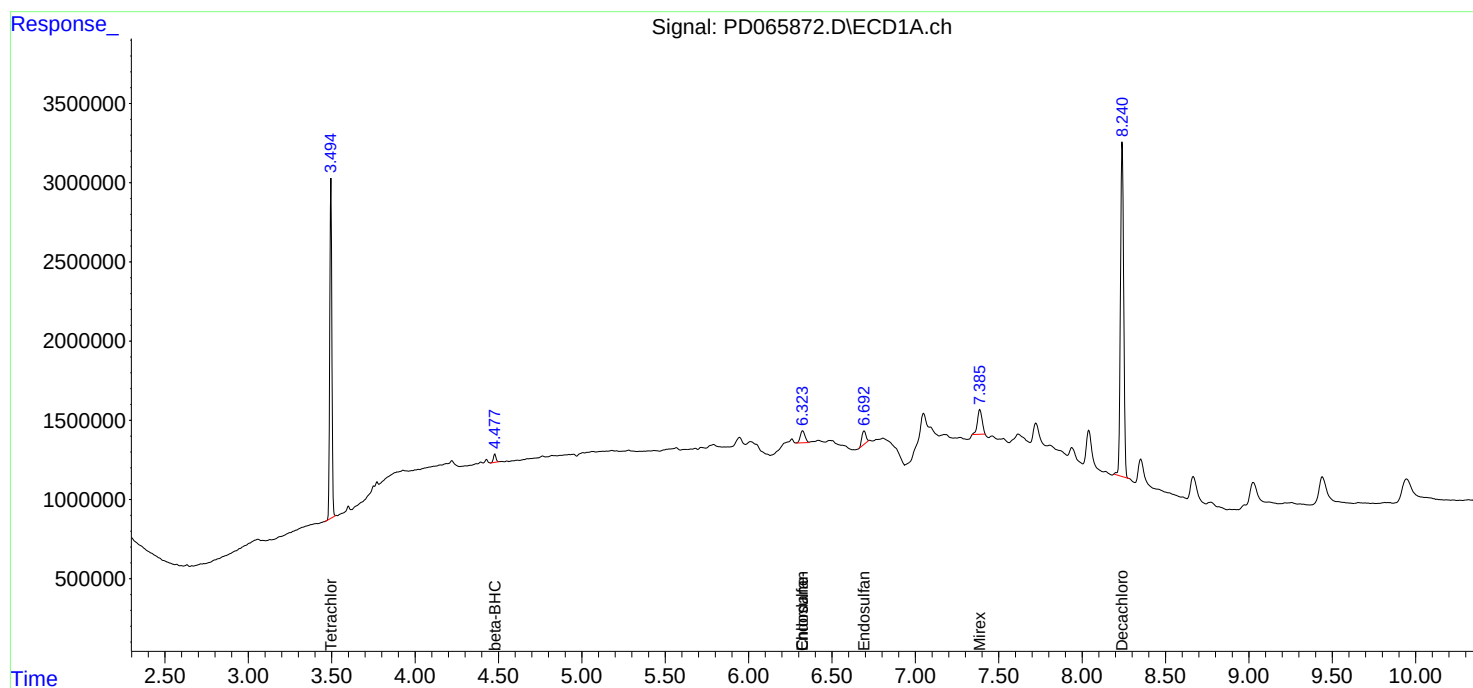


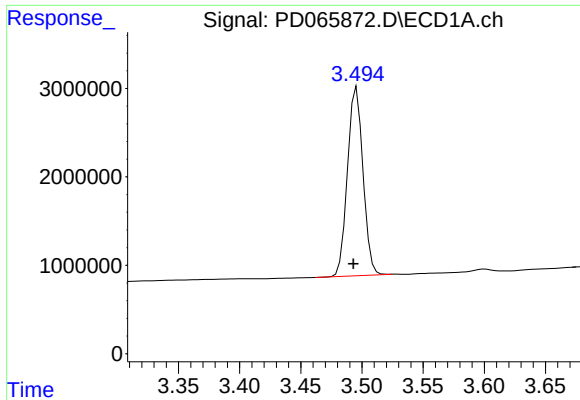

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.003 min
Response: 18845189
Conc: 25.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

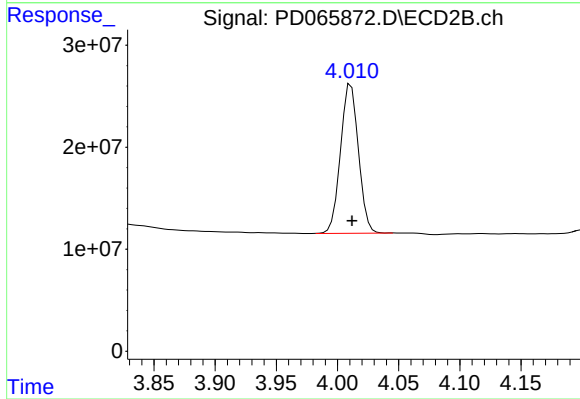


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 149019012
Conc: 25.95 ng/ml

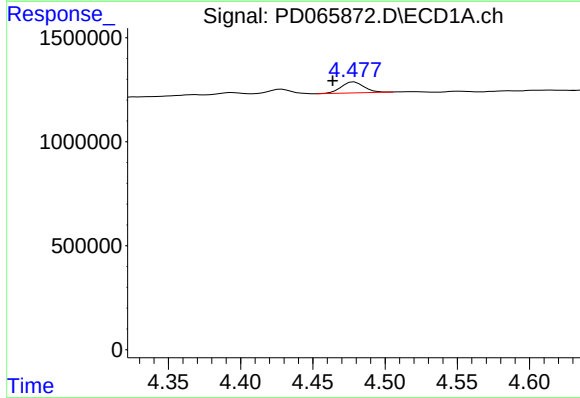


#6 beta-BHC

R.T.: 4.479 min
Delta R.T.: 0.015 min
Response: 570034
Conc: 1.00 ng/ml

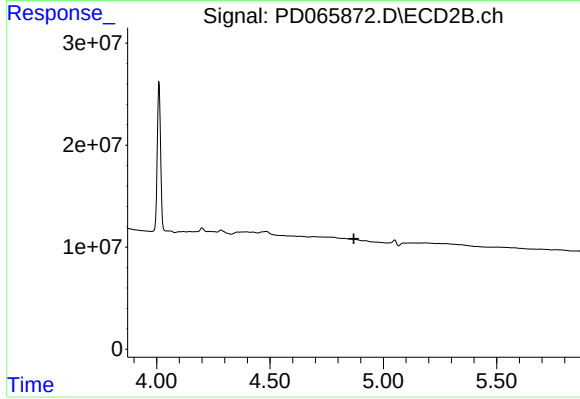

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.870 min
Response: 0
Conc: N.D.

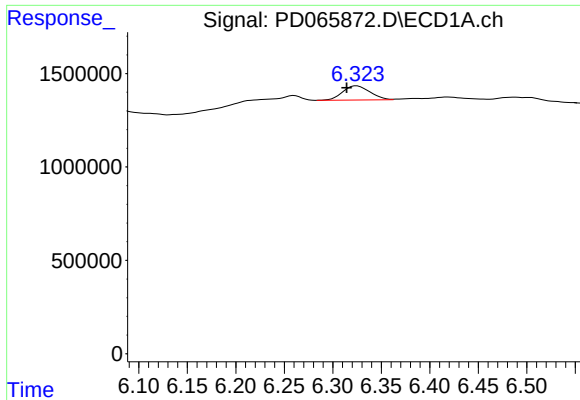

#15 Endosulfan II


R.T.: 6.325 min
Delta R.T.: 0.010 min
Response: 1483993
Conc: 1.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

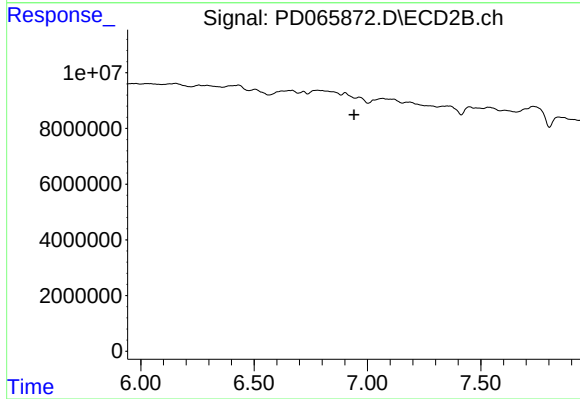


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.941 min
Response: 0
Conc: N.D.

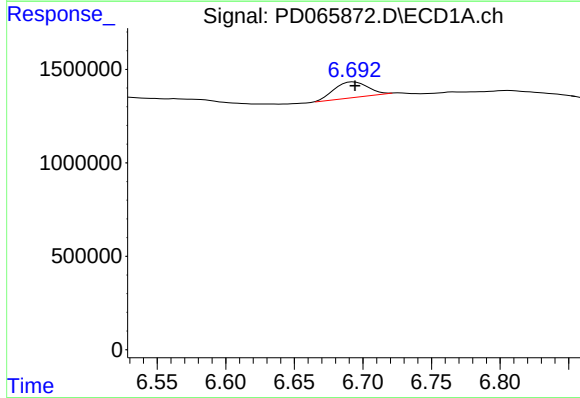


#19 Endosulfan Sulfate

R.T.: 6.693 min
Delta R.T.: -0.001 min
Response: 1423460
Conc: 1.25 ng/ml

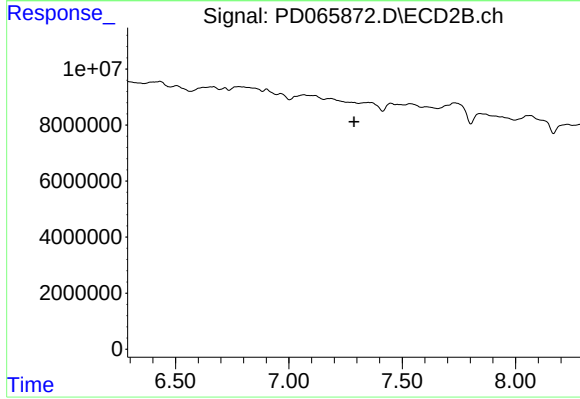

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.288 min
Response: 0
Conc: N.D.

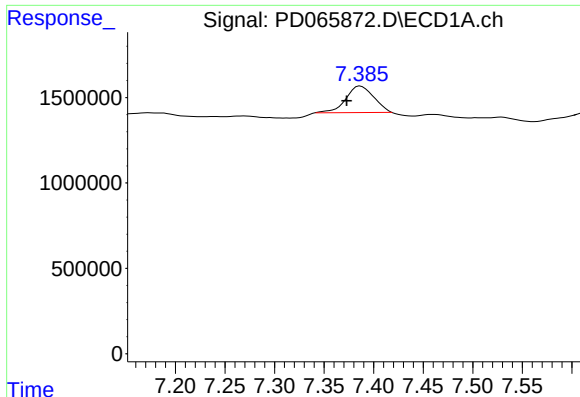

#22 Mirex


R.T.: 7.387 min
Delta R.T.: 0.014 min
Response: 3048840
Conc: 2.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

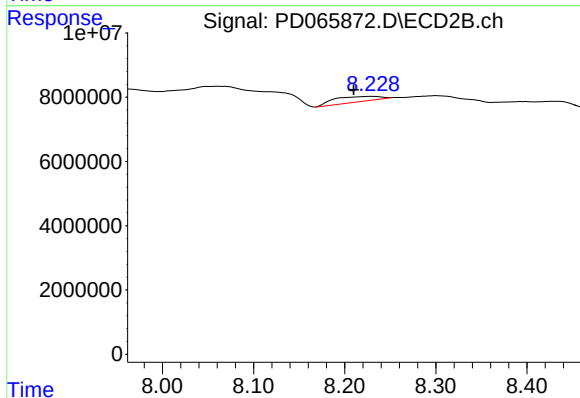


#22 Mirex

R.T.: 8.230 min
Delta R.T.: 0.020 min
Response: 5725345
Conc: 1.45 ng/ml

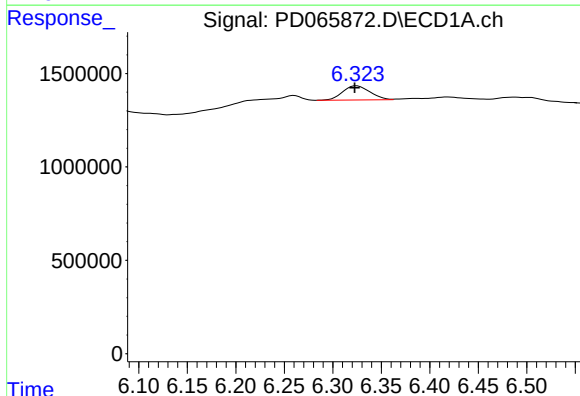


#27 Chlordane-5

R.T.: 6.325 min
Delta R.T.: 0.002 min
Response: 1483993
Conc: 30.53 ng/ml

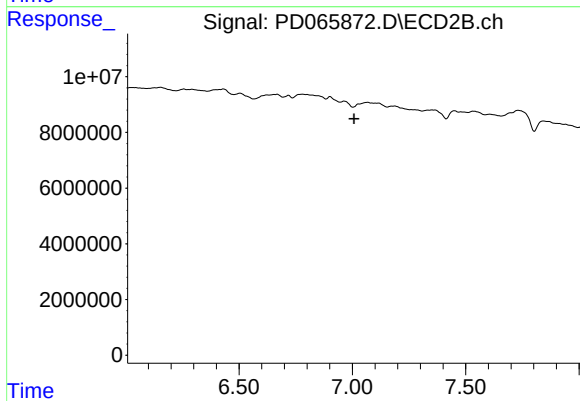

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.008 min
Response: 0
Conc: N.D.

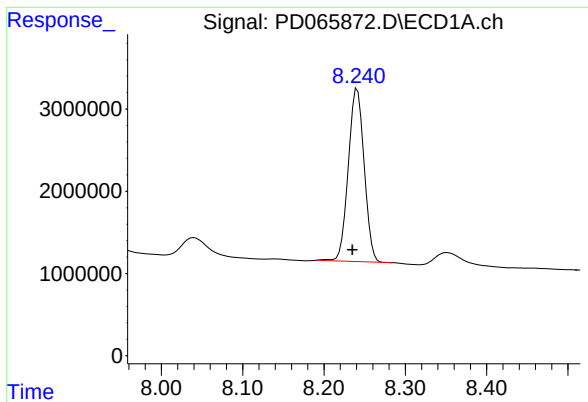

#28 Decachlorobiphenyl


R.T.: 8.241 min

Delta R.T.: 0.006 min

Response: 28383327

Conc: 20.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

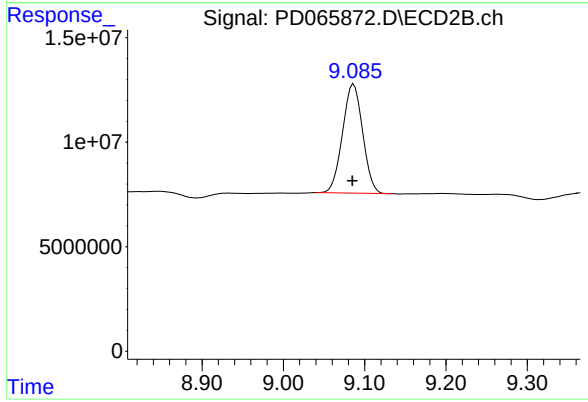

#28 Decachlorobiphenyl

R.T.: 9.087 min

Delta R.T.: 0.002 min

Response: 89440240

Conc: 23.11 ng/ml