

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092525\
 Data File : PD090399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2025 17:40
 Operator : AR\AJ
 Sample : PB169830BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB169830BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/26/2025
 Supervised By : Sohil Jodhani 09/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 05:46:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:52:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.877	42259463	406.7E6	13.001m	14.818
28) SA Decachlor...	9.067	8.064	72591126	292.0E6	15.045m	9.007 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092525\
Data File : PD090399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2025 17:40
Operator : AR\AJ
Sample : PB169830BL
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PB169830BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 05:46:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:52:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

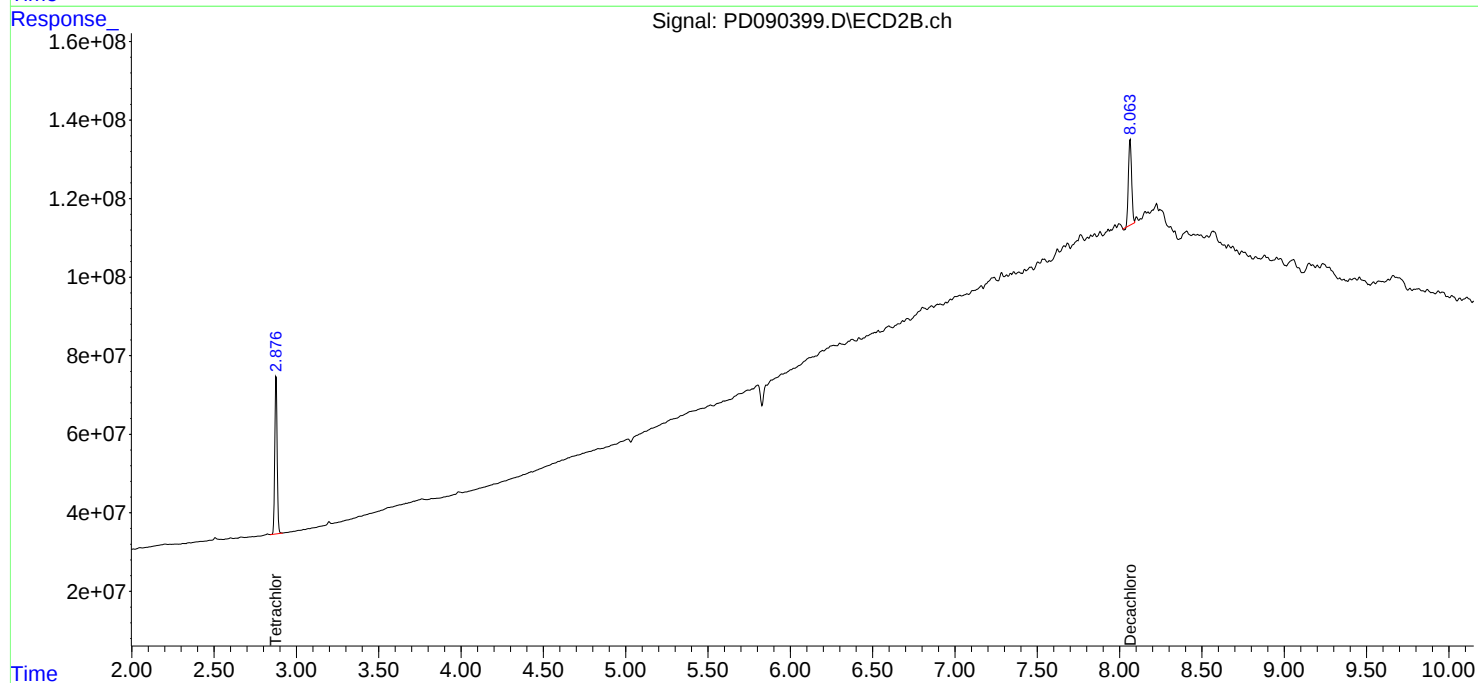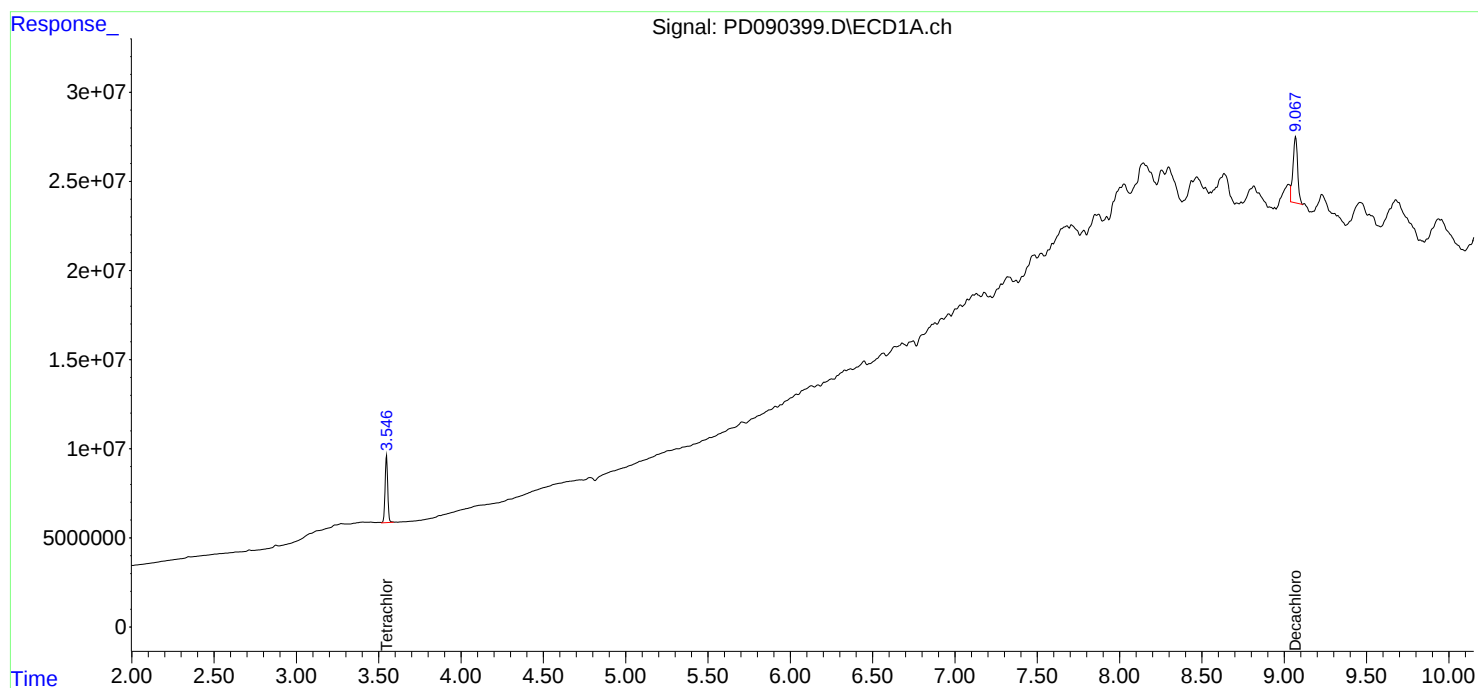

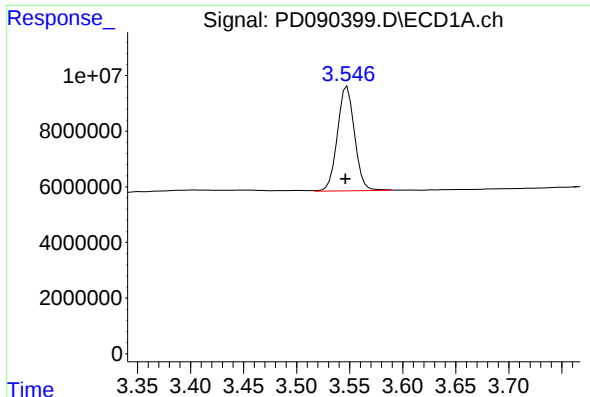


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 42259463
Conc: 13.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB169830BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

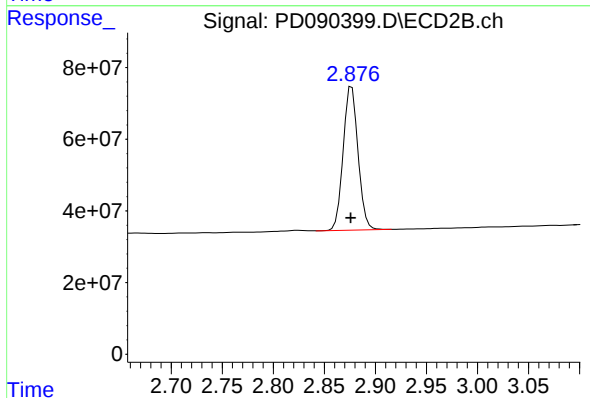


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.001 min
Response: 406739718
Conc: 14.82 ng/ml

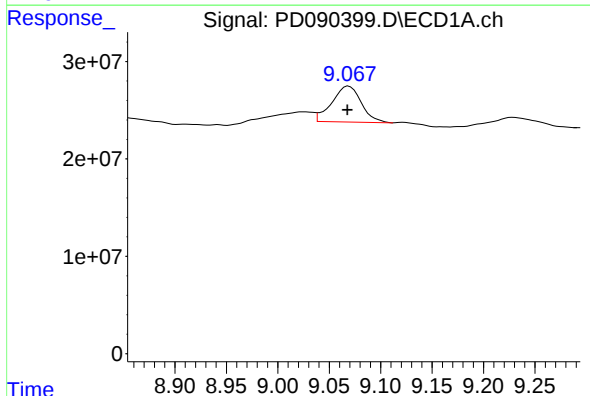

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 72591126
Conc: 15.04 ng/ml m

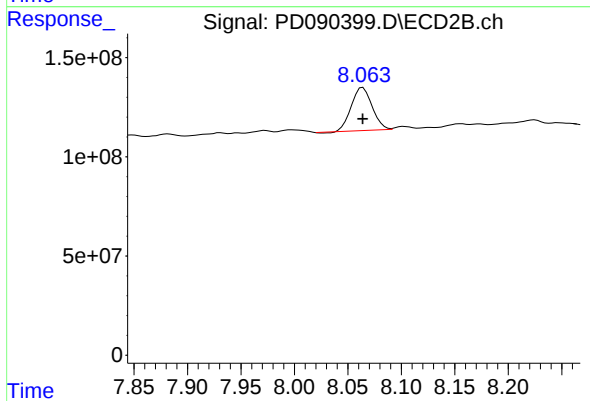

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 291958536
Conc: 9.01 ng/ml