

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
 Data File : PD059368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2020 04:40
 Operator : DD\AJ
 Sample : MDL-BL-TOX-11
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:09:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.025	29205166	40813661	23.283	24.255
27)	SA Decachlor...	8.322	9.109	38488466	55543451	45.610	48.792
Target Compounds							
2)	A alpha-BHC	3.950	0.000	213897	0	0.121	N.D. #
3)	MA gamma-BHC...	4.241	0.000	1252910	0	0.743	N.D. #
6)	B beta-BHC	4.463f	4.919f	1617650	2799553	2.096	2.769 #
10)	B trans-Chl...	0.000	6.077f	0	50903	N.D.	<MDL
15)	B Endosulfa...	0.000	6.955	0	714381	N.D.	0.501
16)	A 4,4'-DDD	0.000	6.820f	0	89413	N.D.	<MDL
19)	B Endosulfa...	0.000	7.312	0	161251	N.D.	0.111
24)	Toxaphene-3	6.298	0.000	899653	0	109.383	N.D. #
26)	Toxaphene-5	7.096	0.000	2164007	0	126.990	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
Data File : PD059368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2020 04:40
Operator : DD\AJ
Sample : MDL-BL-TOX-11
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:09:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

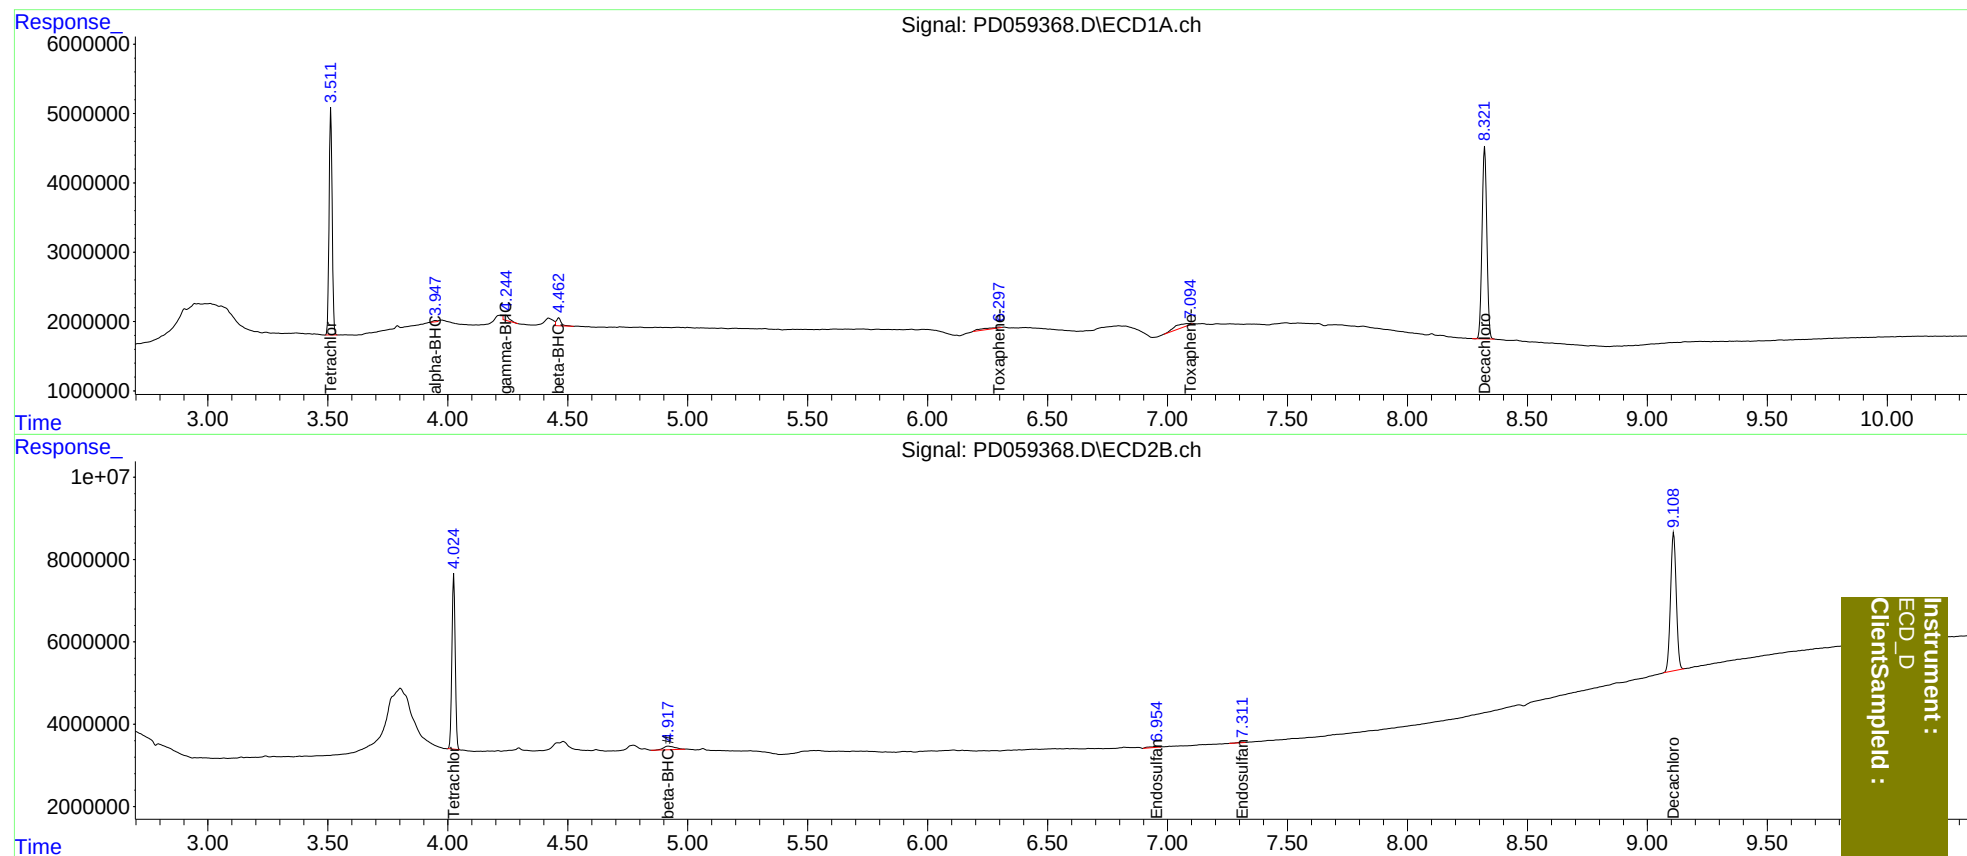


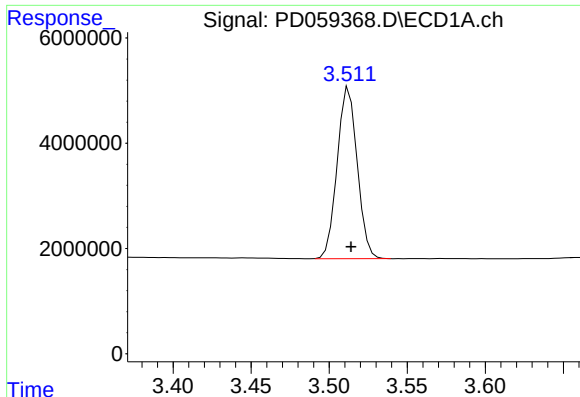

#1 Tetrachloro-m-xylene


R.T.: 3.513 min
Delta R.T.: -0.001 min
Response: 29205166
Conc: 23.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

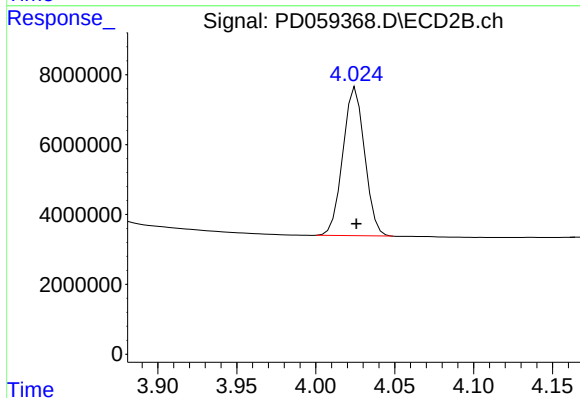


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 40813661
Conc: 24.25 ng/ml

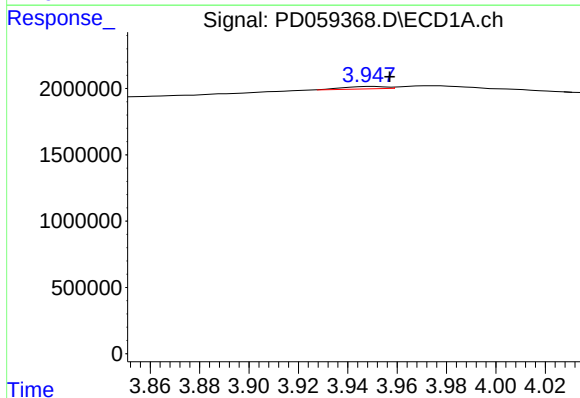


#2 alpha-BHC

R.T.: 3.950 min
Delta R.T.: -0.007 min
Response: 213897
Conc: 0.12 ng/ml

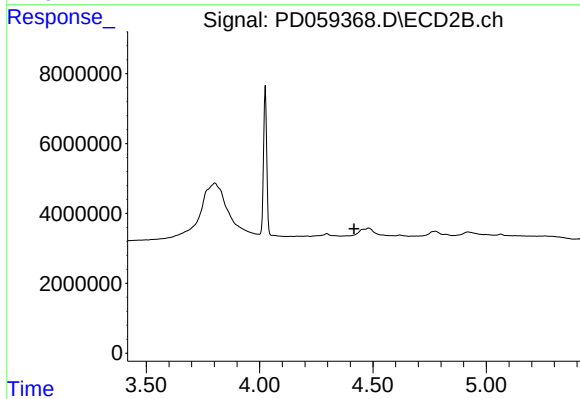

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.416 min
Response: 0
Conc: N.D.

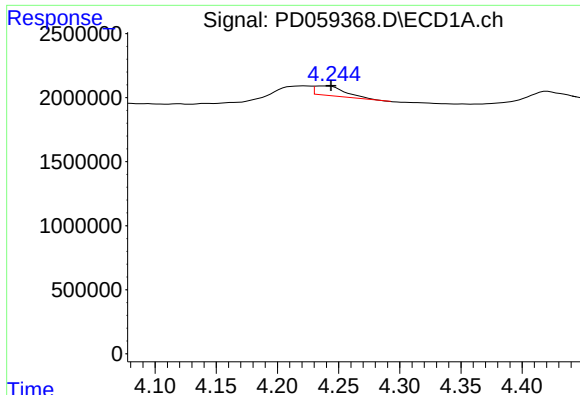

#3 gamma-BHC (Lindane)


R.T.: 4.241 min
Delta R.T.: -0.003 min
Response: 1252910
Conc: 0.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

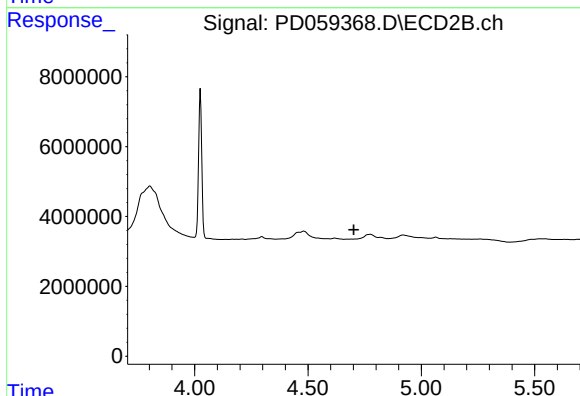


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.702 min
Response: 0
Conc: N.D.

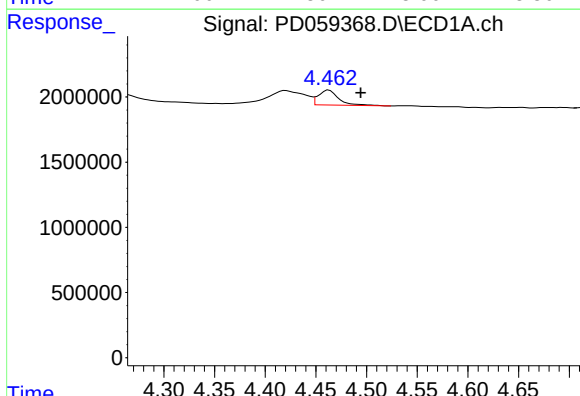


#6 beta-BHC

R.T.: 4.463 min
Delta R.T.: -0.031 min
Response: 1617650
Conc: 2.10 ng/ml

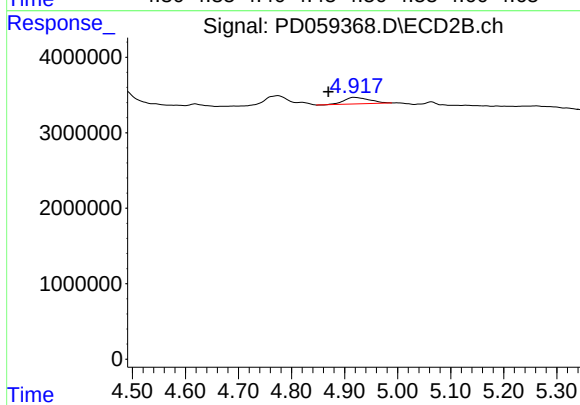

#6 beta-BHC


R.T.: 4.919 min
Delta R.T.: 0.049 min
Response: 2799553
Conc: 2.77 ng/ml

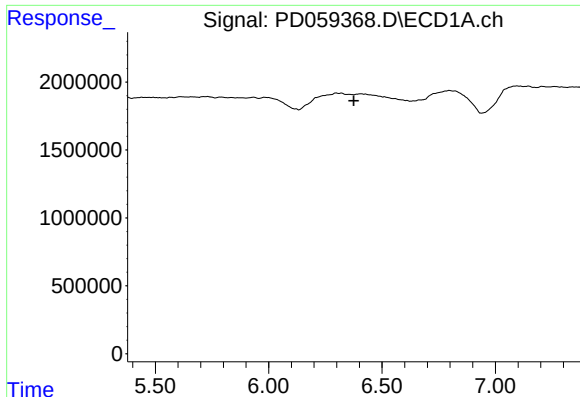

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

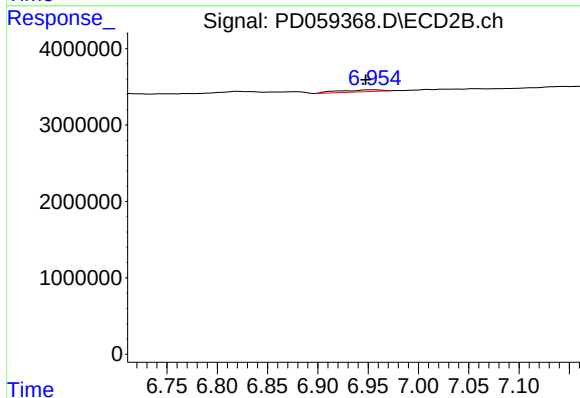


#15 Endosulfan II

R.T.: 6.955 min
Delta R.T.: 0.008 min
Response: 714381
Conc: 0.50 ng/ml

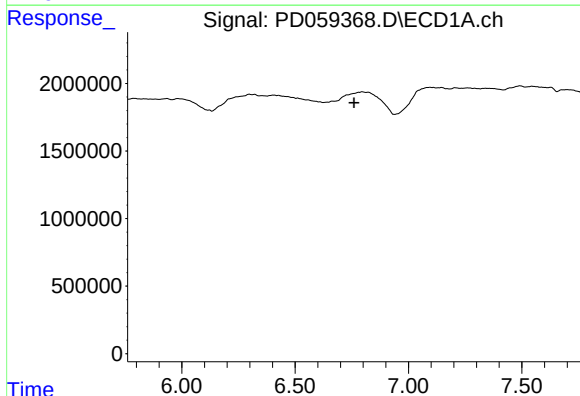


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.761 min
Response: 0
Conc: N.D.

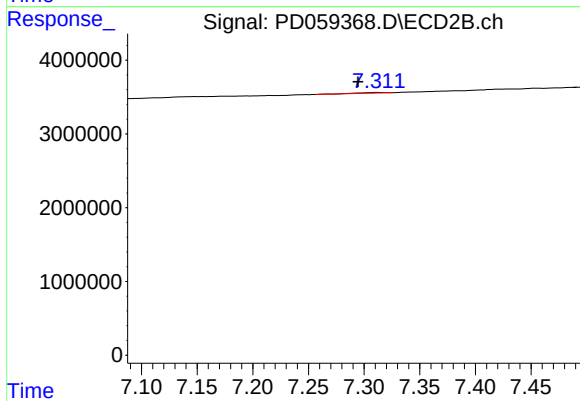

#19 Endosulfan Sulfate


R.T.: 7.312 min
Delta R.T.: 0.018 min
Response: 161251
Conc: 0.11 ng/ml

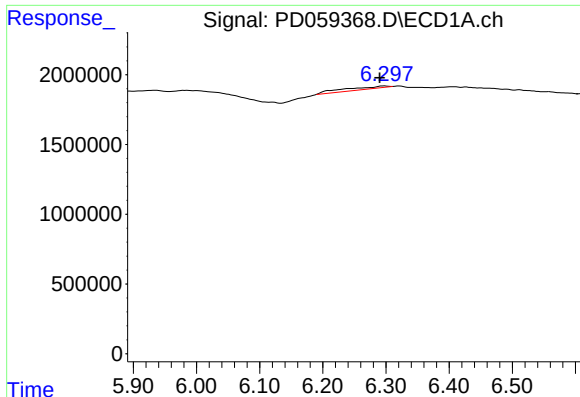

#24 Toxaphene-3


R.T.: 6.298 min
Delta R.T.: 0.008 min
Response: 899653
Conc: 109.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

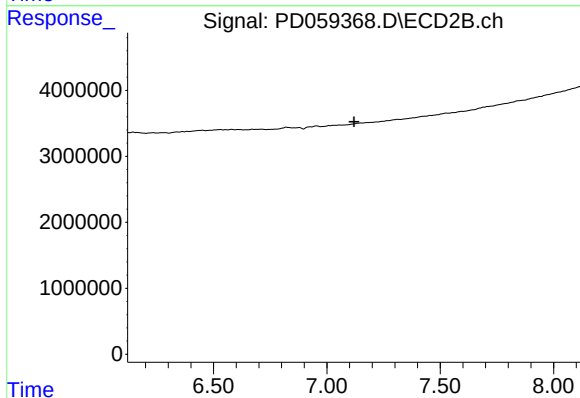


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

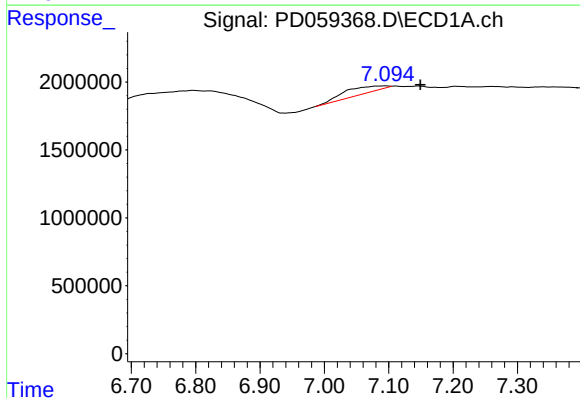


#26 Toxaphene-5

R.T.: 7.096 min
Delta R.T.: -0.054 min
Response: 2164007
Conc: 126.99 ng/ml

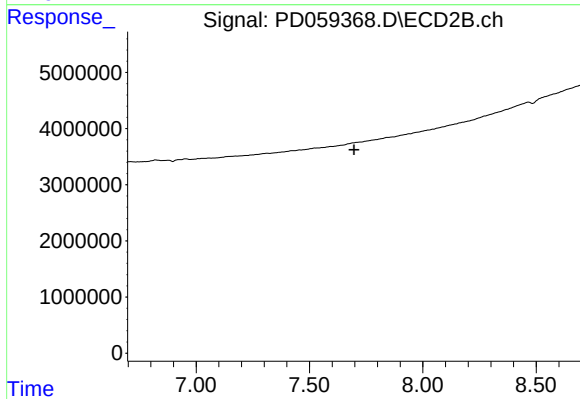

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T. : 7.696 min
Response: 0
Conc: N.D.

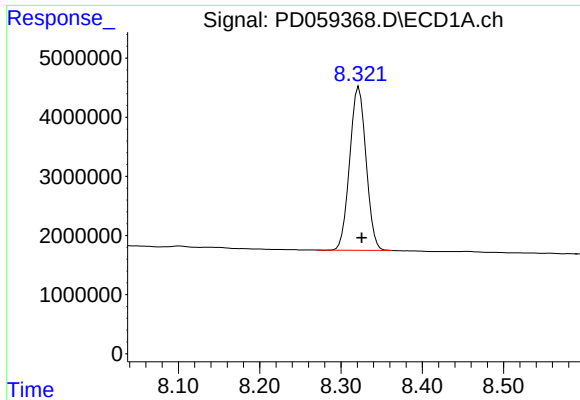

#27 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.004 min
Response: 38488466
Conc: 45.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

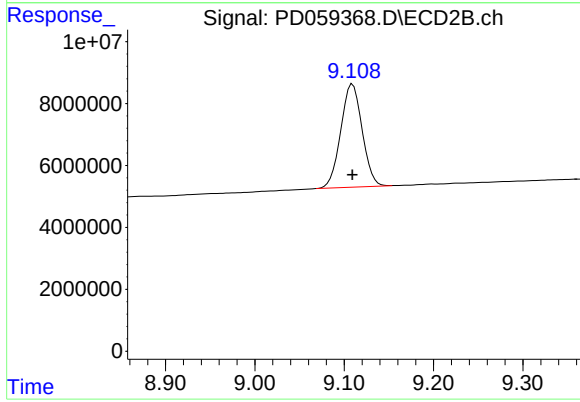

#27 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 55543451
Conc: 48.79 ng/ml