

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
 Data File : PD059363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2020 03:29
 Operator : DD\AJ
 Sample : L1955-12
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 MDL-WATER-05

Manual Integrations
 APPROVED

Ankita
 9/28/2020 2:07:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:53:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.026	28805185	40574939	22.964	24.113
27)	SA Decachlor...	8.323	9.110	38431876	55057904	45.542	48.365
Target Compounds							
2)	A alpha-BHC	3.955	4.416	2546237	2235642	1.443	0.913 #
3)	MA gamma-BHC...	4.242	4.702	3295649	2667274	1.953	1.192 #
4)	MA Heptachlor	4.551	5.213	2098208	2539699	1.267	1.173
5)	MB Aldrin	4.804	5.520	2030189	2709109	1.256	1.340
6)	B beta-BHC	4.492	4.870	1139864	1087076	1.477	1.075 #
7)	B delta-BHC	4.701	5.088	2059274	2722718	1.246	1.197
8)	B Heptachlo...	5.251	5.907	1878587	3087458	1.314	1.641
9)	A Endosulfan I	5.595	6.265	1706535	2082058	1.327	1.256
10)	B trans-Chl...	5.481	6.141	1863573	2349952	1.319	1.289
11)	B cis-Chlor...	5.540	6.214	1842109	2197894	1.308	1.217
12)	B 4,4'-DDE	5.705	6.369	1762118	2106415	1.323	1.233
13)	MA Dieldrin	5.840	6.523	1834641	2274107	1.361	1.281
14)	MA Endrin	6.099	6.741	1018614	1247224	1.031	0.973
15)	B Endosulfa...	6.373	6.949	1485333	2461208	1.382	1.725
16)	A 4,4'-DDD	6.225	6.860	1704095	1853883	1.640	1.373
17)	MA 4,4'-DDT	6.469	7.158	1284036	1328208	1.220	1.195m
18)	B Endrin al...	6.543	7.072	1282969	1308259	1.448	1.108
19)	B Endosulfa...	6.757	7.296	1259418	1744845	1.240	1.197
20)	A Methoxychlor	7.021	7.615	571278	747026	1.159m	1.205
21)	B Endrin ke...	7.252	7.769	1631899	1656030	1.516	1.183

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
Data File : PD059363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2020 03:29
Operator : DD\AJ
Sample : L1955-12
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:53:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

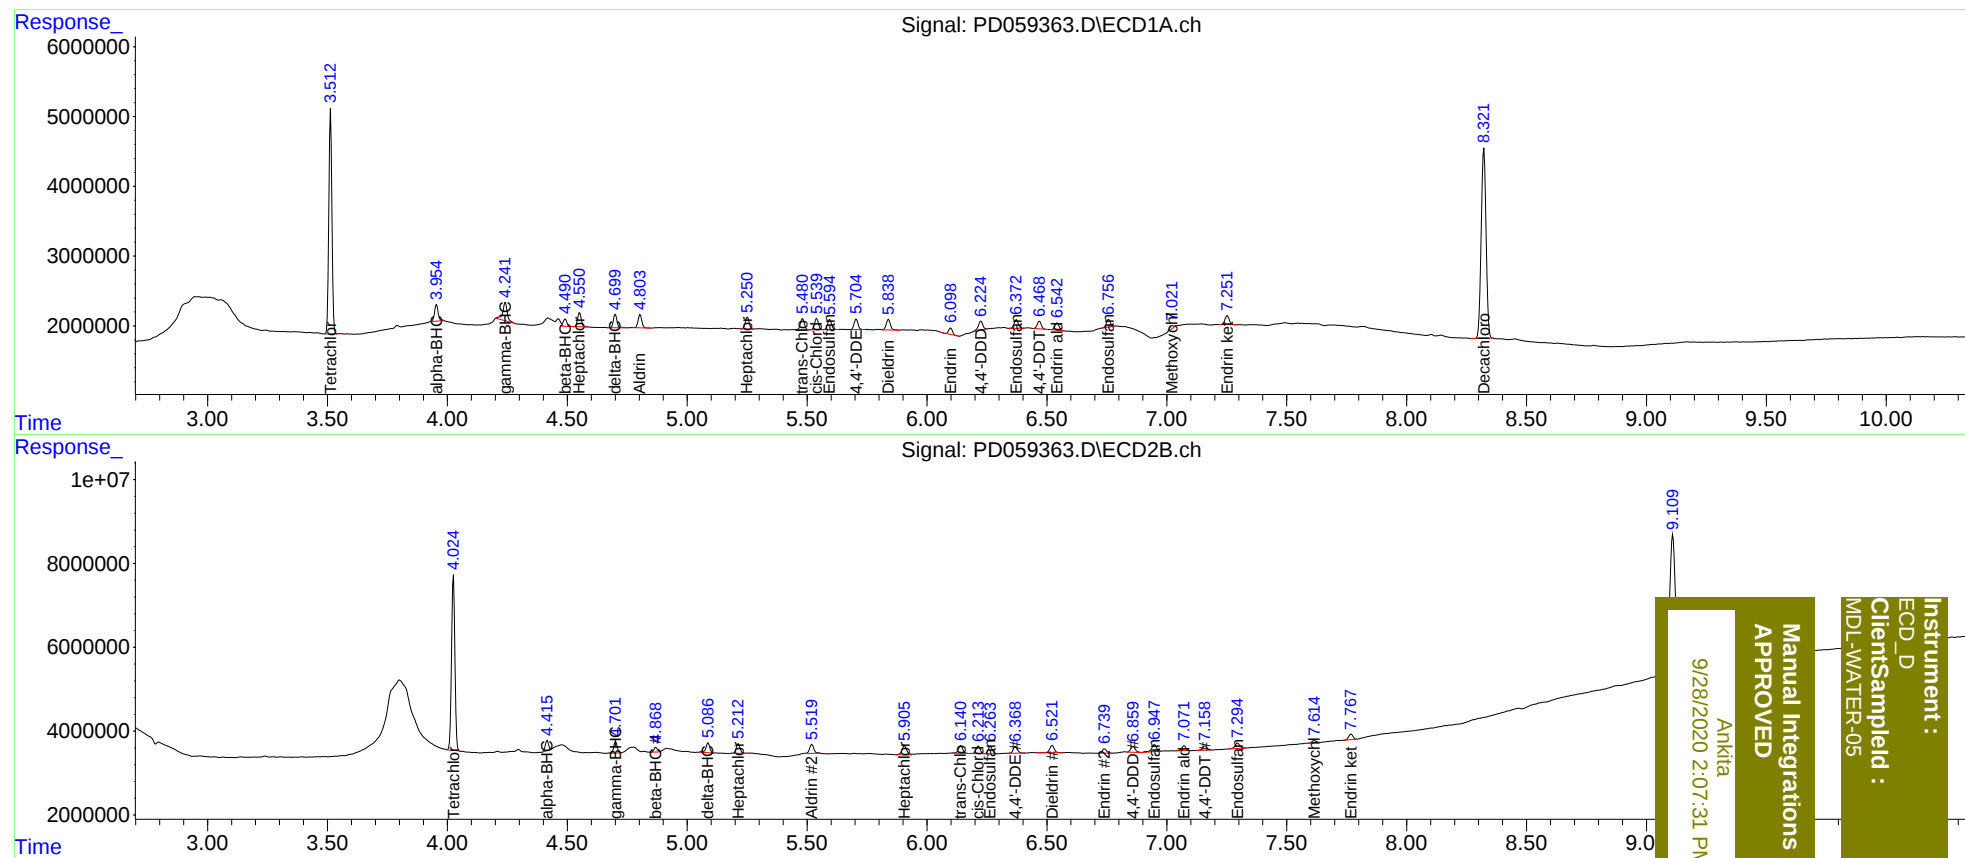

Manual Integrations
APPROVED

9/28/2020 2:07:31 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-05

Ankita