

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
 Data File : PD059367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2020 04:26
 Operator : DD\AJ
 Sample : MDL-TOX-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-TOX-05

Manual Integrations
 APPROVED

Ankita
 9/28/2020 2:07:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:09:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.026	30821714	43261419	24.572	25.709
27)	SA Decachlor...	8.322	9.110	41117432	58580934	48.725	51.460
Target Compounds							
22)	Toxaphene-1	5.800	6.422	1301559	1219437	163.235	150.079
23)	Toxaphene-2	5.964	6.711	1141720	1515758	150.643	155.324m
24)	Toxaphene-3	6.286	7.120	1338533	1712650	162.743	134.192
25)	Toxaphene-4	6.407	7.195	3011272	4640401	158.583	144.282
26)	Toxaphene-5	7.146	7.697	2732322	2715738	160.340	144.426

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
Data File : PD059367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2020 04:26
Operator : DD\AJ
Sample : MDL-TOX-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:09:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

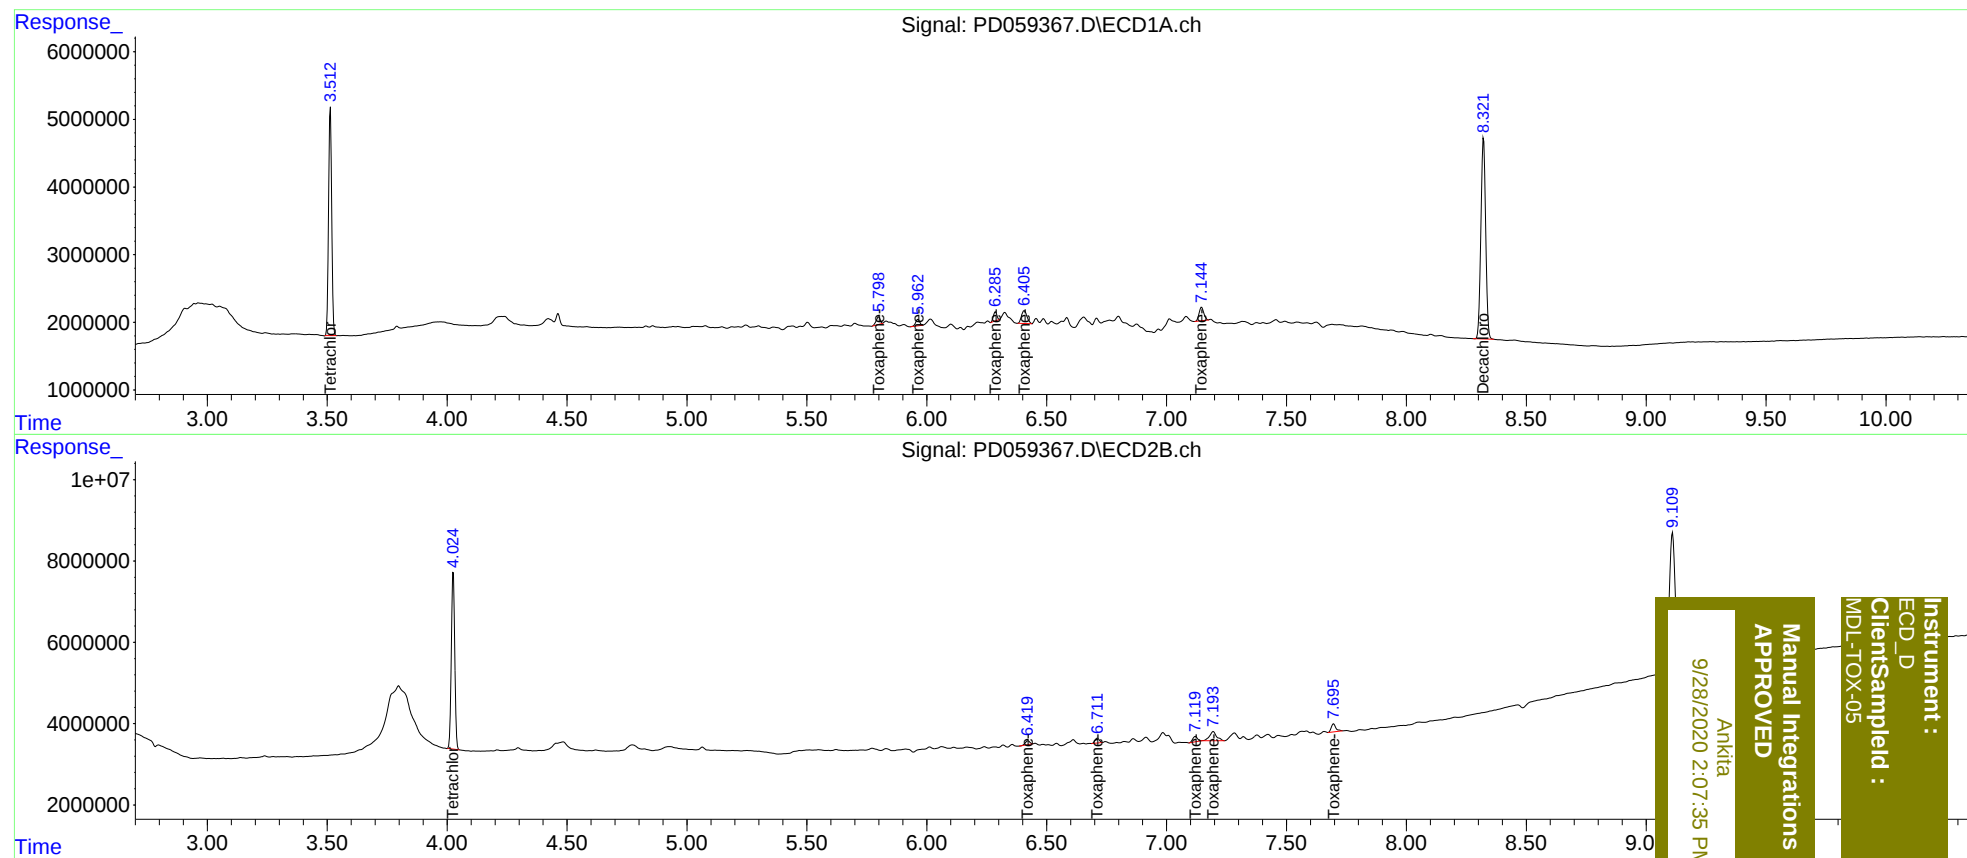

Manual Integrations
APPROVED

Ankita
9/28/2020 2:07:35 PM

Instrument :
ECD_D
Client Sampled :
MDL-TOX-05