

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
 Data File : PD059362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2020 03:14
 Operator : DD\AJ
 Sample : L1955-11
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-04

Manual Integrations
 APPROVED

Ankita
 9/28/2020 2:07:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:52:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 25 05:12:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.026	29250704	41230931	23.319	24.503
2)	SA Decachlor...	8.322	9.111	38938737	56133315	46.143	49.310
Target Compounds							
2)	A alpha-BHC	3.955	4.417	2576638	2377720	1.461	0.971 #
3)	MA gamma-BHC...	4.242	4.702	3311209	2725591	1.963	1.218 #
4)	MA Heptachlor	4.551	5.214	2157124	2535790	1.302	1.171
5)	MB Aldrin	4.804	5.521	2092921	2634242	1.295	1.303
6)	B beta-BHC	4.492	4.870	1172204	1143530	1.519	1.131 #
7)	B delta-BHC	4.701	5.088	2127850	2879281	1.287	1.266
8)	B Heptachlo...	5.251	5.907	1895935	3030671	1.326	1.611
9)	A Endosulfan I	5.595	6.265	1801687	2217629	1.401	1.338
10)	B trans-Chl...	5.481	6.141	1844631	2262002	1.306	1.241
11)	B cis-Chlor...	5.541	6.215	1831523	2212832	1.301	1.226
12)	B 4,4'-DDE	5.705	6.369	1768740	2066052	1.328	1.210
13)	MA Dieldrin	5.840	6.523	1818570	2277696	1.349	1.283
14)	MA Endrin	6.099	6.741	1060259	1388460	1.074	1.083
15)	B Endosulfa...	6.373	6.949	1519213	2545232	1.414	1.784 #
16)	A 4,4'-DDD	6.225	6.860	1665017	2007627	1.602	1.487
17)	MA 4,4'-DDT	6.469	7.159	1250574	1285574	1.188	1.157
18)	B Endrin al...	6.543	7.072	1299440	1556788	1.466	1.319
19)	B Endosulfa...	6.758	7.295	1419501	1770531	1.398	1.215
20)	A Methoxychlor	7.022	7.616	540823	724152	1.097m	1.168
21)	B Endrin ke...	7.252	7.768	1692749	2016793	1.572	1.441

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092620\
Data File : PD059362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2020 03:14
Operator : DD\AJ
Sample : L1955-11
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:52:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 25 05:12:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

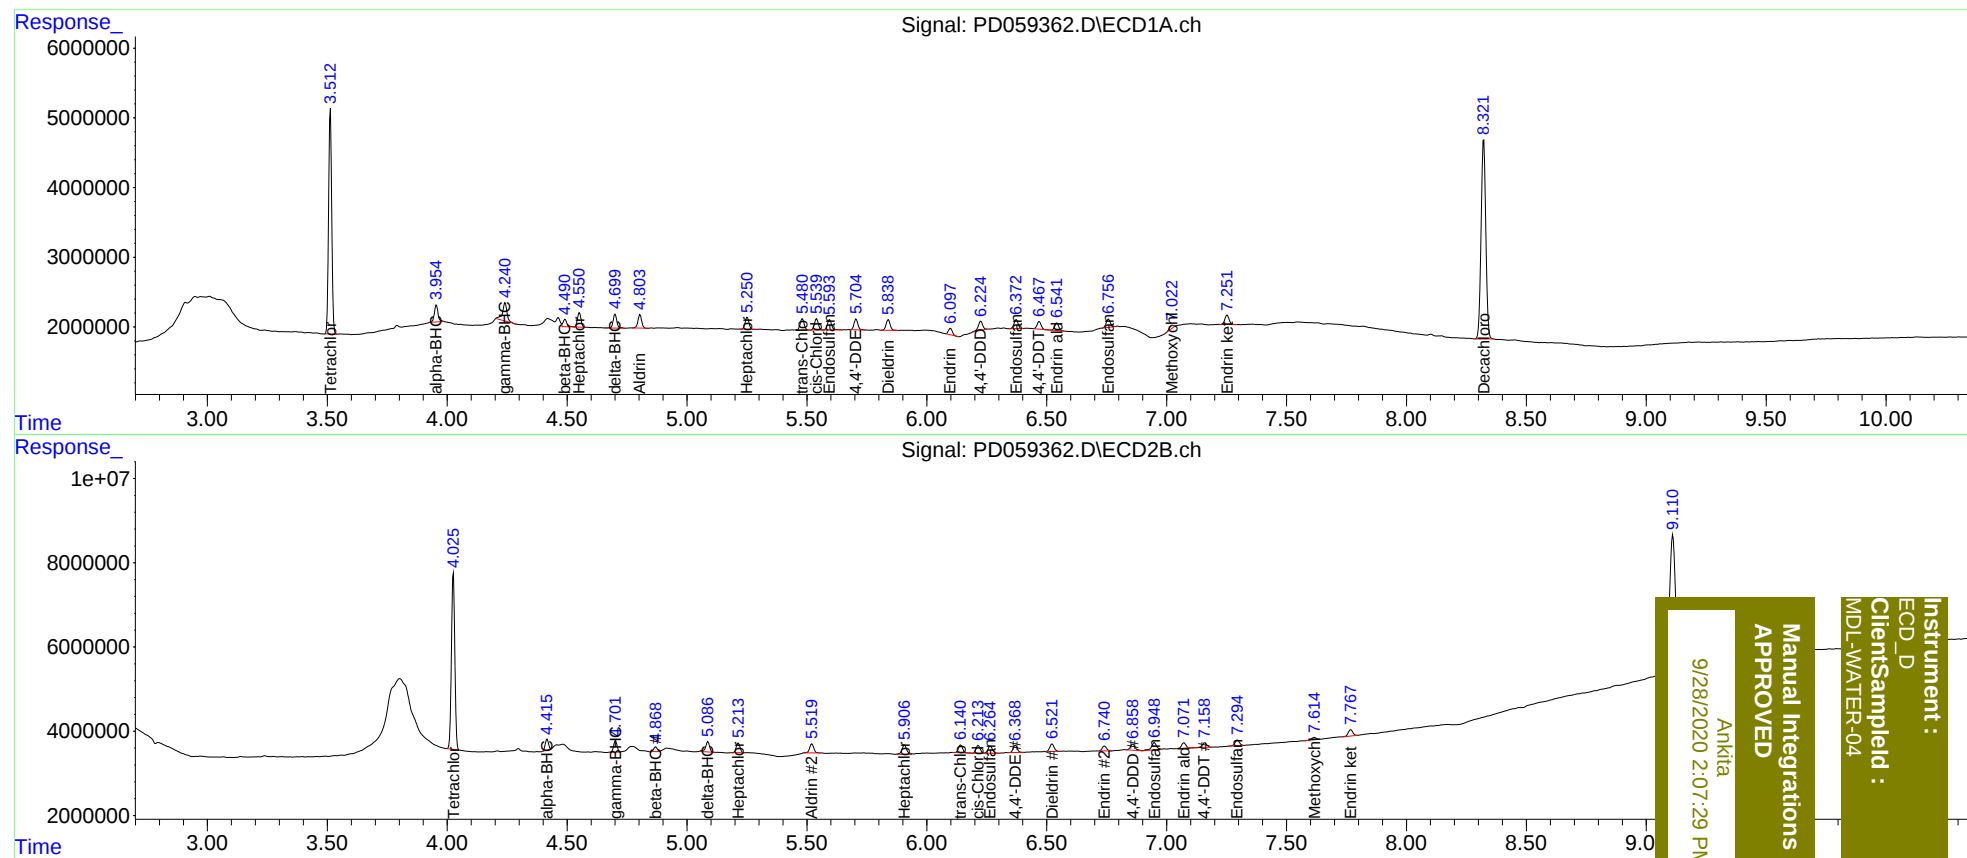

Manual Integrations
APPROVED

9/28/2020 2:07:29 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-04