

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
 Data File : PD072033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 15:37
 Operator : AR\AJ
 Sample : TOXAPHENE312
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TOXAPH3177

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/27/2022
 Supervised By : Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 05:23:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.809	3.563	51065600	678.4E6	20.141	22.019
27)	SA Decachlor...	7.998	9.092	97131050	366.3E6	41.431m	40.893
Target Compounds							
22)	Toxaphene-1	5.391	5.888	32778454	124.2E6	2085.856m	2151.793m
23)	Toxaphene-2	5.753	6.271	34905758	156.3E6	2078.895m	2120.467
24)	Toxaphene-3	6.037	7.095	39465598	361.8E6	2069.824m	1945.889
25)	Toxaphene-4	6.802	7.186	160.8E6	525.8E6	2052.194m	2069.349m
26)	Toxaphene-5	7.119	7.614	71815881	299.5E6	2147.310m	1989.302m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 05:23:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

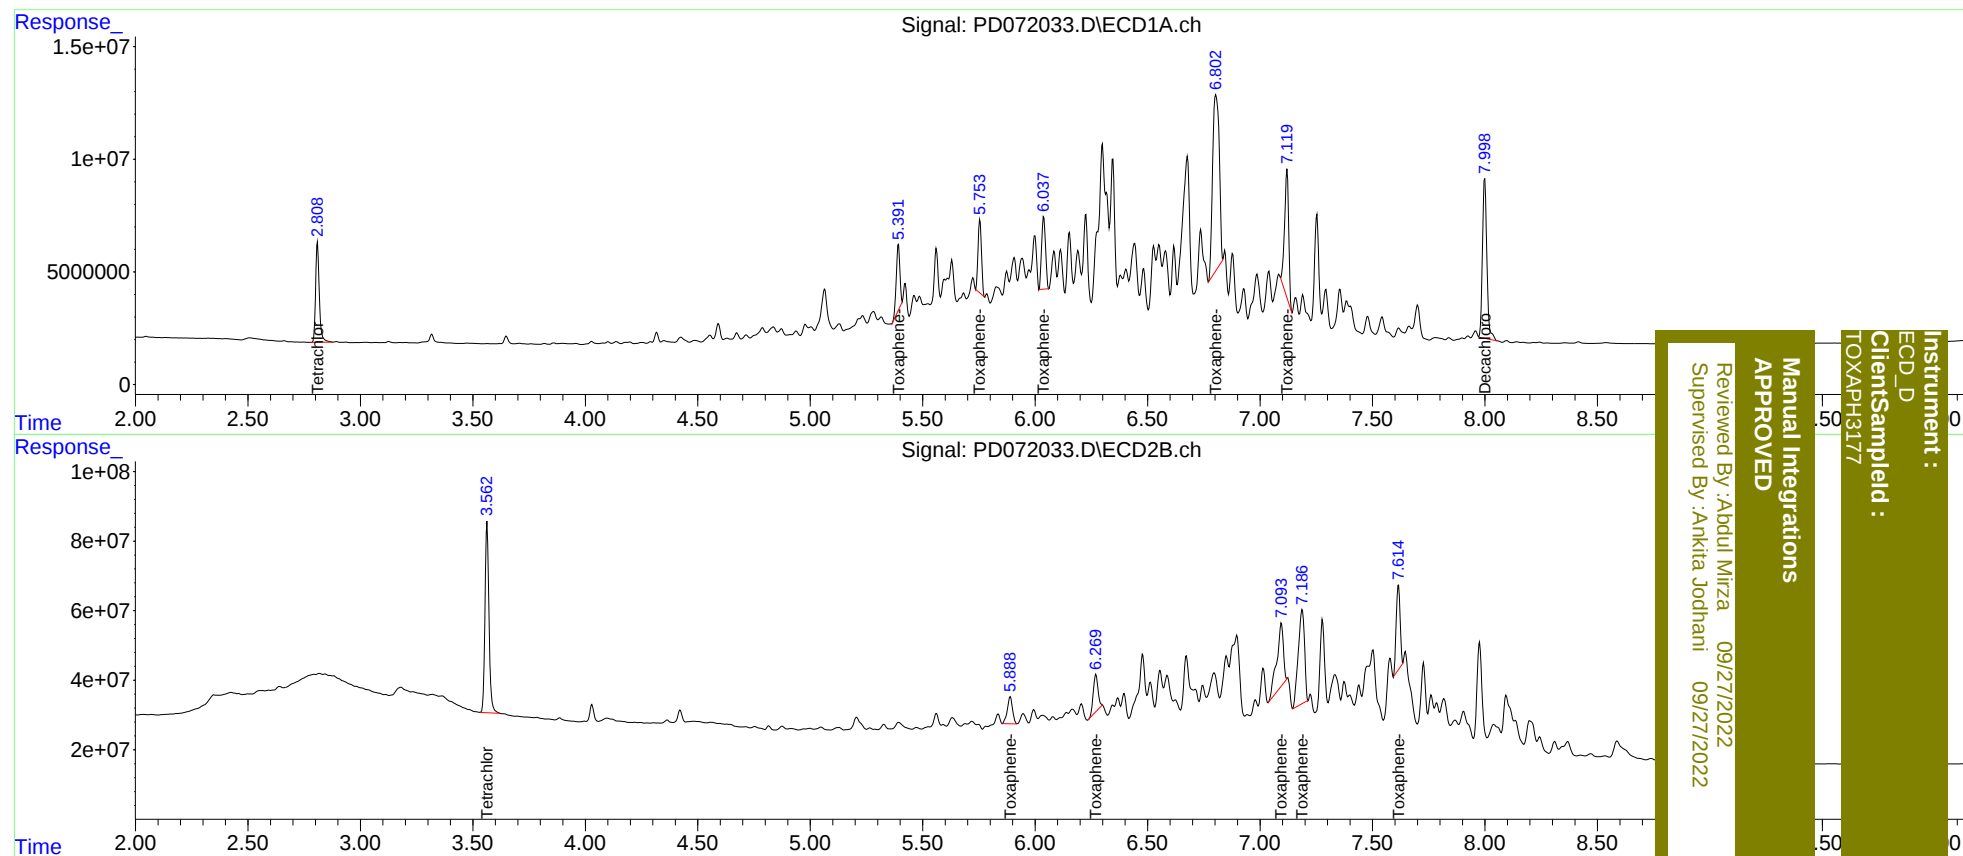

Reviewed By: Abdul Mirza 09/27/2022
Supervised By: Ankita Jodhani 09/27/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampleId :
TOXAPH3177