

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
 Data File : PD072040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 17:36
 Operator : AR\AJ
 Sample : N4748-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQS0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/27/2022
 Supervised By : Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 05:24:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.805	3.564	47385442	600.0E6	18.690	19.473
2) SA Decachlor...	7.993	9.089	64961750	248.3E6	27.709m	27.717m
Target Compounds						
10) B trans-Chl...	5.034	5.972	3737985	20410345	1.145	1.181
11) B cis-Chlor...	5.099	6.049	4381286	26214827	1.365	1.557

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
Data File : PD072040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 17:36
Operator : AR\AJ
Sample : N4748-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 05:24:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

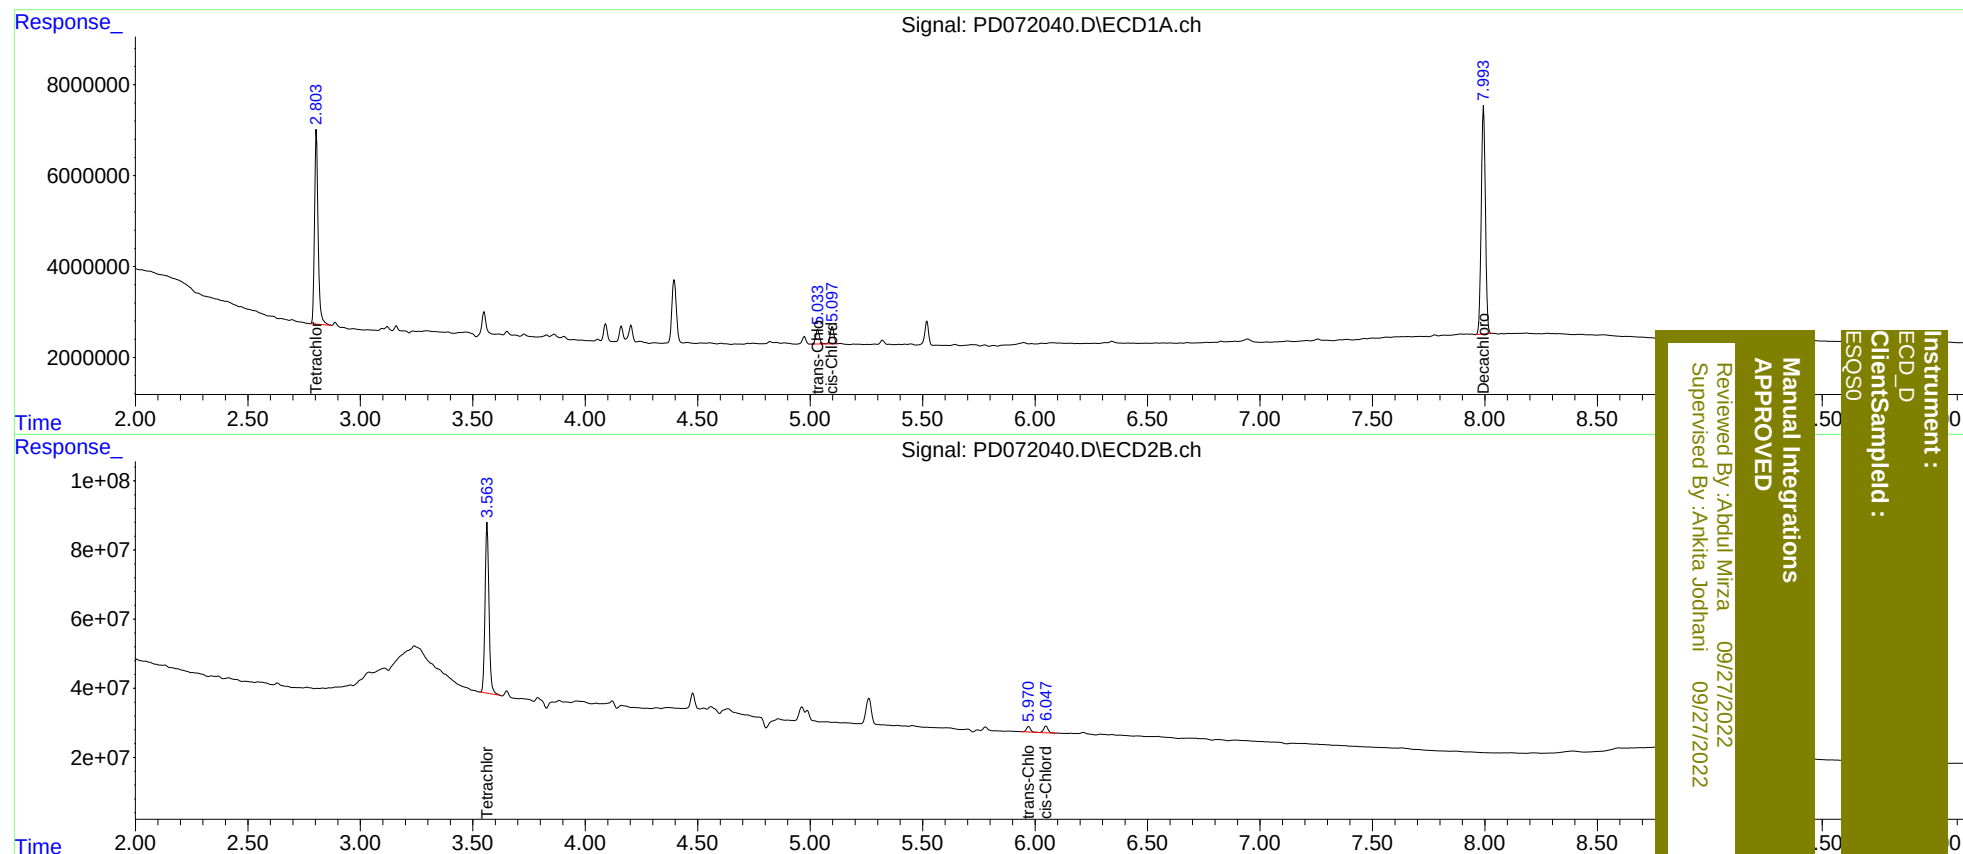

Reviewed By: Abdul Mirza 09/27/2022
Supervised By: Ankita Jodhani 09/27/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
ESQSO