

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
 Data File : PD072041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 17:49
 Operator : AR\AJ
 Sample : N4748-02MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQS0MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/27/2022
 Supervised By : Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 05:24:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.805	3.564	50385259	615.5E6	19.873	19.978
2) SA Decachlor...	7.995	9.089	64171891	248.6E6	27.372	27.749
Target Compounds						
2) A alpha-BHC	3.313	4.030	223.7E6	2304.6E6	60.408	54.171
3) MA gamma-BHC...	3.646	4.366	209.6E6	1869.3E6	59.942	52.836
4) MA Heptachlor	3.992	4.941	207.4E6	1394.4E6	58.362	55.289m
5) MB Aldrin	4.275	5.284	204.1E6	1279.1E6	57.423	58.208m
6) B beta-BHC	3.944	4.572	81933559	724.0E6	51.191	48.659
7) B delta-BHC	4.178	4.820	211.9E6	1379.8E6	59.848	55.368
8) B Heptachlo...	4.782	5.716	176.5E6	872.3E6	55.449	57.205
9) A Endosulfan I	5.155	6.104	167.7E6	804.7E6	59.509	53.984
10) B trans-Chl...	5.035	5.971	189.0E6	883.8E6	57.864	51.149
11) B cis-Chlor...	5.099	6.049	187.2E6	892.6E6	58.324	53.030
12) B 4,4'-DDE	5.290	6.221	335.5E6	1580.1E6	113.340	105.295
13) MA Dieldrin	5.423	6.382	371.6E6	1671.3E6	120.859	110.685
14) MA Endrin	5.700	6.614	327.5E6	1423.9E6	123.525	115.508
15) B Endosulfa...	5.995	6.840	297.3E6	1331.4E6	119.136	109.600
16) A 4,4'-DDD	5.849	6.746	278.8E6	1276.6E6	119.404	110.522
17) MA 4,4'-DDT	6.102	7.057	298.8E6	1344.3E6	124.715	118.151
18) B Endrin al...	6.176	6.971	233.9E6	1065.2E6	107.730	102.724
19) B Endosulfa...	6.400	7.204	275.1E6	1197.9E6	109.013	103.979
20) A Methoxychlor	6.681	7.534	727.2E6	2848.6E6	565.825	547.969
21) B Endrin ke...	6.910	7.695	333.5E6	1355.3E6	117.940	108.519

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
Data File : PD072041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 17:49
Operator : AR\AJ
Sample : N4748-02MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 05:24:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

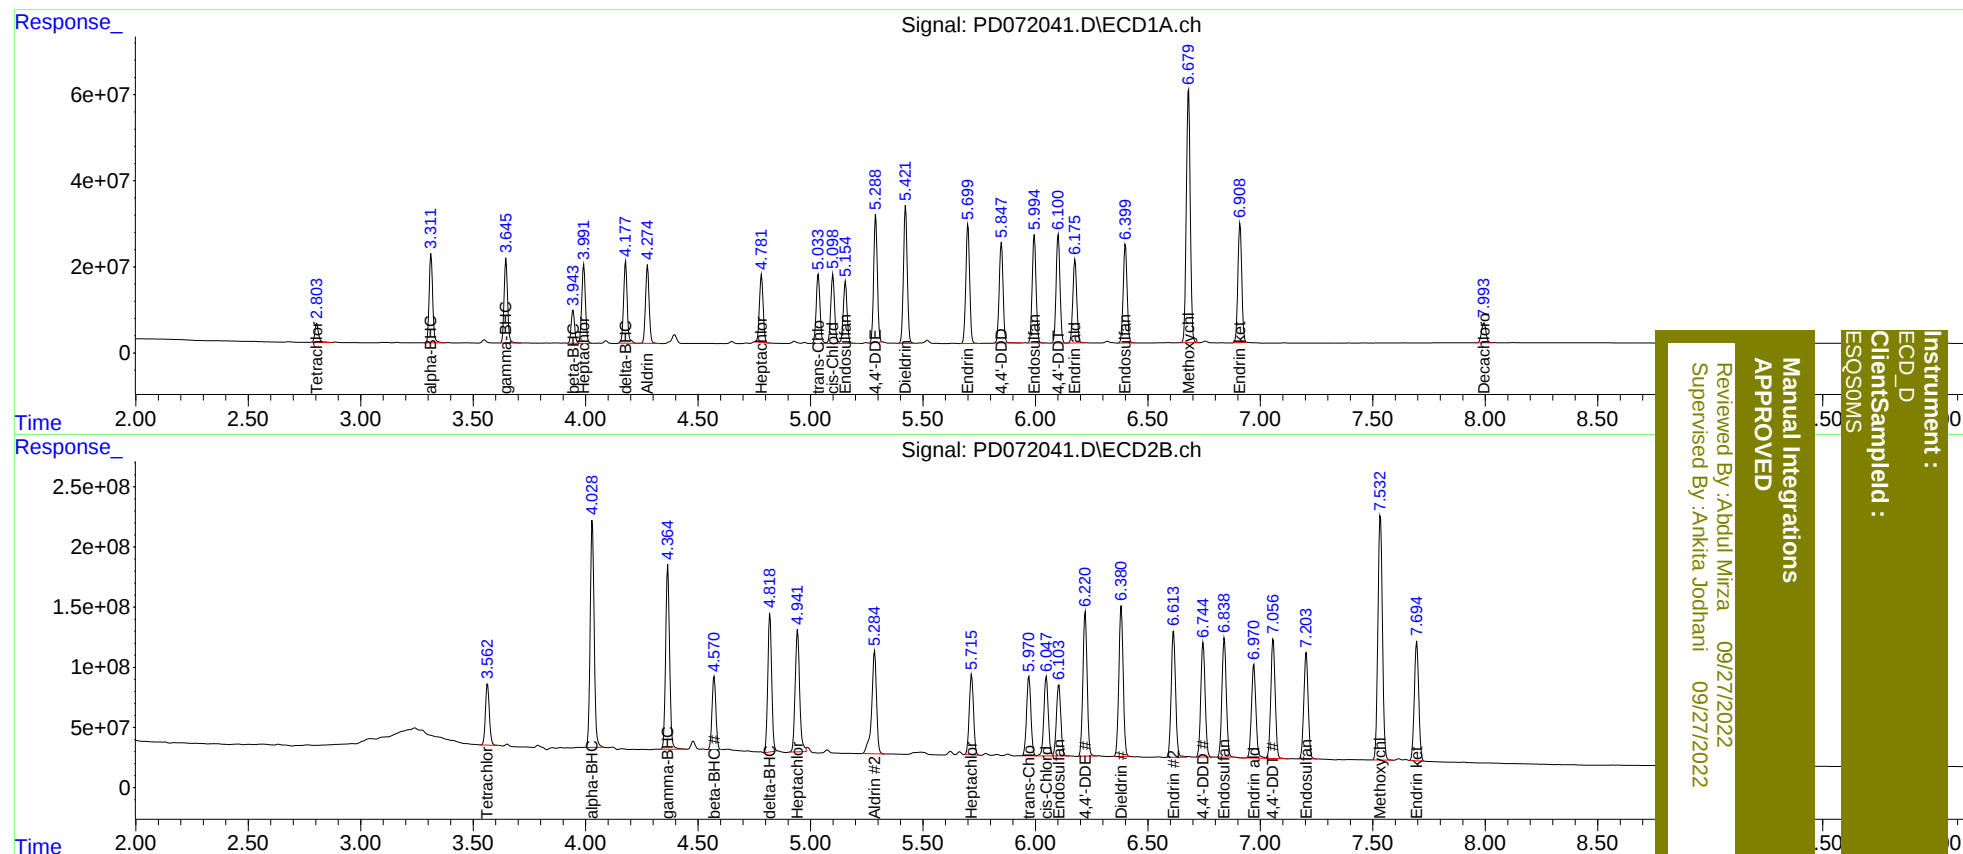

Instrument :
ECD_D
ClientSampled :
ESQ50MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/27/2022
Supervised By: Ankita Jodhani 09/27/2022