

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
 Data File : PD072042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 18:03
 Operator : AR\AJ
 Sample : N4748-03MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQS0MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/27/2022
 Supervised By :Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 05:24:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 23 17:46:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	49655657	629.3E6	19.585	20.424
27)	SA Decachlor...	7.993	9.089	64246362	248.9E6	27.404	27.785
Target Compounds							
2)	A alpha-BHC	3.313	4.029	224.4E6	2288.8E6	60.591	53.800
3)	MA gamma-BHC...	3.646	4.366	209.6E6	1853.8E6	59.951	52.398
4)	MA Heptachlor	3.992	4.941	208.3E6	1403.7E6	58.624	55.656m
5)	MB Aldrin	4.275	5.283	206.1E6	1256.2E6	57.993	57.163m
6)	B beta-BHC	3.944	4.572	81994370	723.6E6	51.229	48.633
7)	B delta-BHC	4.178	4.820	211.6E6	1390.8E6	59.750	55.811
8)	B Heptachlo...	4.781	5.716	178.8E6	863.8E6	56.161	56.650
9)	A Endosulfan I	5.155	6.105	169.8E6	803.2E6	60.252	53.878
10)	B trans-Chl...	5.034	5.971	190.3E6	882.6E6	58.253	51.078
11)	B cis-Chlor...	5.099	6.048	189.0E6	892.2E6	58.890	53.005
12)	B 4,4'-DDE	5.290	6.221	343.4E6	1577.7E6	116.036	105.134
13)	MA Dieldrin	5.422	6.381	377.2E6	1679.3E6	122.688	111.211
14)	MA Endrin	5.700	6.614	335.8E6	1433.4E6	126.638	116.281
15)	B Endosulfa...	5.995	6.840	299.6E6	1332.8E6	120.056	109.711
16)	A 4,4'-DDD	5.848	6.746	282.3E6	1279.4E6	120.924	110.765
17)	MA 4,4'-DDT	6.101	7.057	304.8E6	1353.6E6	127.217	118.967
18)	B Endrin al...	6.175	6.971	236.3E6	1073.7E6	108.844	103.535
19)	B Endosulfa...	6.399	7.204	276.0E6	1202.2E6	109.378	104.348
20)	A Methoxychlor	6.681	7.534	725.6E6	2861.2E6	564.576	550.384
21)	B Endrin ke...	6.909	7.695	331.7E6	1357.2E6	117.300	108.672

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092622\
Data File : PD072042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 18:03
Operator : AR\AJ
Sample : N4748-03MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 05:24:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092422CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 23 17:46:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

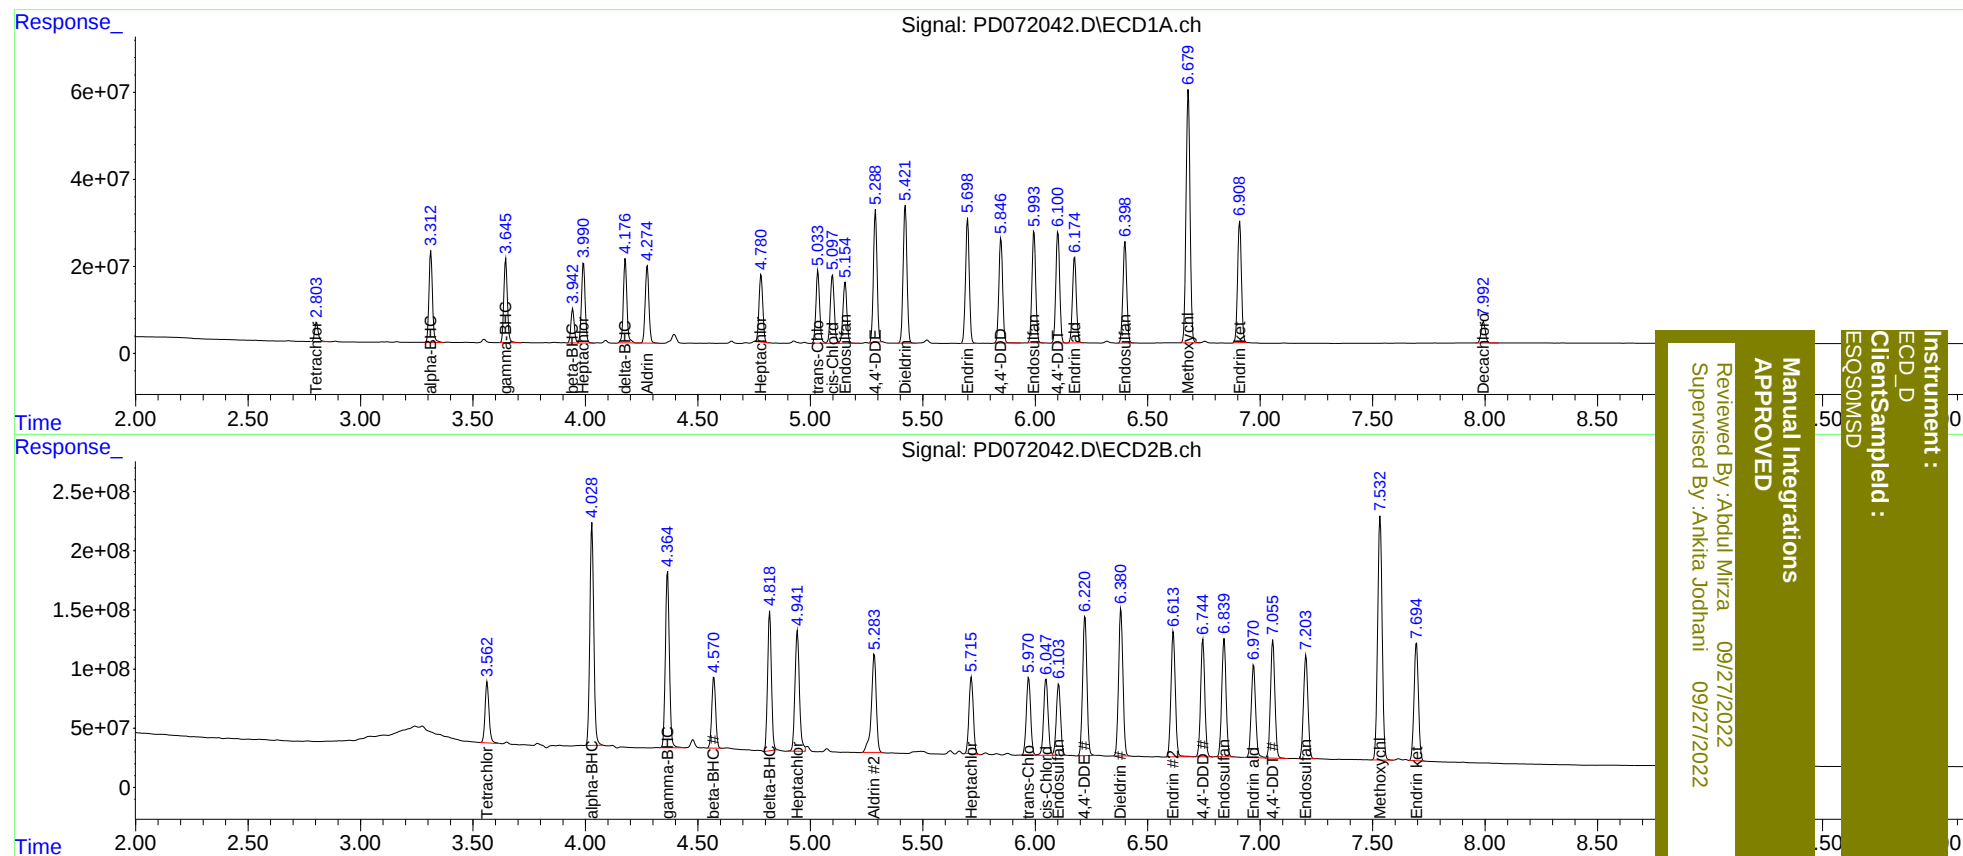

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/27/2022
Supervised By: Ankita Jodhani 09/27/2022

Instrument :
ECD_D
Client Sampled :
ESQ50MSD